

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033230.D
 Acq On : 11 Dec 2023 22:19
 Operator : SY/MD
 Sample : 05730-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	92918	96394	11.52%	1.394%
2	1.532	145	153	164	rBV	74109	85895	10.27%	1.242%
3	2.060	306	317	330	rBV2	164807	245374	29.33%	3.549%
4	2.220	358	367	381	rBV4	4905	9927	1.19%	0.144%
5	2.288	386	388	393	rVV	293	209	0.02%	0.003%
6	2.449	435	438	440	rBV2	587	365	0.04%	0.005%
7	2.671	504	507	508	rVB	379	168	0.02%	0.002%
8	2.683	508	511	512	rBV	192	127	0.02%	0.002%
9	2.700	515	516	520	rBV2	401	206	0.02%	0.003%
10	2.854	562	564	567	rBV	306	147	0.02%	0.002%
11	2.896	574	577	580	rVB	301	226	0.03%	0.003%
12	2.918	580	584	588	rBV2	227	208	0.02%	0.003%
13	2.970	595	600	602	rBV	318	327	0.04%	0.005%
14	3.127	643	649	651	rBV3	297	289	0.03%	0.004%
15	3.220	676	678	681	rBV	209	147	0.02%	0.002%
16	3.265	690	692	696	rVB	295	162	0.02%	0.002%
17	3.301	699	703	705	rBV2	472	325	0.04%	0.005%
18	3.474	755	757	758	rBV	270	140	0.02%	0.002%
19	3.632	803	806	809	rBV2	342	220	0.03%	0.003%
20	3.780	844	852	881	rBV	55977	154559	18.47%	2.235%
21	4.249	980	998	1024	rBV	142589	371237	44.37%	5.369%
22	4.507	1075	1078	1079	rBV	640	330	0.04%	0.005%
23	4.645	1118	1121	1123	rBV	245	136	0.02%	0.002%
24	4.658	1123	1125	1126	rBV	251	115	0.01%	0.002%
25	4.757	1154	1156	1157	rBV	307	147	0.02%	0.002%
26	4.806	1166	1171	1172	rBV	310	218	0.03%	0.003%
27	4.835	1178	1180	1181	rBV	319	127	0.02%	0.002%
28	4.902	1198	1201	1202	rBV2	266	134	0.02%	0.002%
29	4.957	1202	1218	1245	rBV2	312806	836738	100.00%	12.101%
30	5.298	1322	1324	1326	rBV2	389	152	0.02%	0.002%
31	5.378	1346	1349	1351	rBV	359	192	0.02%	0.003%
32	5.452	1368	1372	1377	rBV2	354	400	0.05%	0.006%
33	5.474	1377	1379	1382	rBV2	285	174	0.02%	0.003%
34	5.532	1385	1397	1422	rBV	292334	600495	71.77%	8.684%
35	5.831	1478	1490	1504	rBV2	13004	27322	3.27%	0.395%
36	5.986	1526	1538	1563	rBV2	177214	370050	44.23%	5.352%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033230.D
 Acq On : 11 Dec 2023 22:19
 Operator : SY/MD
 Sample : 05730-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.214	1605	1609	1613	rVB3	384	297	0.04%	0.004%
38	6.236	1613	1616	1617	rBV	425	194	0.02%	0.003%
39	6.301	1633	1636	1638	rBV	284	185	0.02%	0.003%
40	6.362	1652	1655	1657	rBV	329	232	0.03%	0.003%
41	6.461	1683	1686	1689	rBV	226	170	0.02%	0.002%
42	6.584	1719	1724	1729	rBV2	350	513	0.06%	0.007%
43	6.632	1736	1739	1741	rBV2	300	220	0.03%	0.003%
44	6.690	1754	1757	1760	rBV	336	186	0.02%	0.003%
45	6.706	1760	1762	1768	rVV2	244	227	0.03%	0.003%
46	6.912	1815	1826	1847	rBV	103085	191821	22.92%	2.774%
47	7.124	1889	1892	1893	rBV	259	136	0.02%	0.002%
48	7.140	1893	1897	1898	rVV	284	186	0.02%	0.003%
49	7.243	1917	1929	1960	rBV	383368	676978	80.91%	9.790%
50	7.551	2015	2025	2047	rBV	75222	136238	16.28%	1.970%
51	7.735	2077	2082	2083	rBV	494	420	0.05%	0.006%
52	7.815	2103	2107	2110	rBV2	724	531	0.06%	0.008%
53	7.857	2116	2120	2122	rBV2	436	331	0.04%	0.005%
54	7.873	2123	2125	2132	rVB2	835	895	0.11%	0.013%
55	7.905	2132	2135	2136	rBV	401	199	0.02%	0.003%
56	8.024	2162	2172	2213	rVV	187114	374833	44.80%	5.421%
57	8.471	2309	2311	2312	rBV	229	118	0.01%	0.002%
58	8.674	2373	2374	2378	rBV	245	167	0.02%	0.002%
59	8.786	2397	2409	2431	rBV	461962	763216	91.21%	11.037%
60	9.059	2491	2494	2496	rBV2	238	156	0.02%	0.002%
61	9.268	2557	2559	2562	rBV2	370	250	0.03%	0.004%
62	9.317	2571	2574	2577	rVB2	201	137	0.02%	0.002%
63	9.342	2577	2582	2584	rBV2	323	240	0.03%	0.003%
64	9.410	2600	2603	2605	rBV2	367	287	0.03%	0.004%
65	9.715	2693	2698	2701	rVB2	268	222	0.03%	0.003%
66	9.735	2701	2704	2708	rVB2	285	255	0.03%	0.004%
67	9.764	2708	2713	2716	rBV2	243	241	0.03%	0.003%
68	9.940	2763	2768	2772	rBV2	313	362	0.04%	0.005%
69	9.969	2774	2777	2781	rVV2	227	192	0.02%	0.003%
70	10.101	2814	2818	2819	rBV	366	217	0.03%	0.003%
71	10.153	2823	2834	2858	rVV	275160	428956	51.27%	6.203%
72	10.275	2869	2872	2875	rBV4	385	362	0.04%	0.005%
73	10.326	2884	2888	2894	rVB3	1218	1141	0.14%	0.017%
74	10.400	2907	2911	2915	rBV2	228	205	0.02%	0.003%
75	10.490	2934	2939	2940	rBV	343	342	0.04%	0.005%
76	10.641	2980	2986	2990	rBV2	257	317	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033230.D
 Acq On : 11 Dec 2023 22:19
 Operator : SY/MD
 Sample : 05730-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.725	3008	3012	3017	rBV2	192	194	0.02%	0.003%
78	10.866	3052	3056	3059	rBV2	589	433	0.05%	0.006%
79	11.014	3099	3102	3107	rVB2	151	134	0.02%	0.002%
80	11.124	3132	3136	3137	rBV3	711	409	0.05%	0.006%
81	11.185	3144	3155	3180	rBV	501660	776545	92.81%	11.230%
82	11.381	3214	3216	3221	rBV2	278	264	0.03%	0.004%
83	11.561	3259	3272	3295	rBV	462792	738673	88.28%	10.682%
84	11.715	3318	3320	3322	rBV	399	206	0.02%	0.003%
85	11.741	3326	3328	3332	rVB3	563	301	0.04%	0.004%
86	11.889	3370	3374	3376	rBV	272	197	0.02%	0.003%
87	12.056	3424	3426	3429	rVV2	230	107	0.01%	0.002%
88	12.561	3579	3583	3586	rVB2	440	322	0.04%	0.005%
89	12.593	3586	3593	3596	rBV6	1569	2014	0.24%	0.029%
90	12.670	3615	3617	3618	rBV	278	115	0.01%	0.002%
91	12.751	3636	3642	3643	rBV2	342	337	0.04%	0.005%
92	12.818	3659	3663	3665	rBV2	422	278	0.03%	0.004%
93	12.834	3665	3668	3670	rBV	285	200	0.02%	0.003%
94	13.159	3764	3769	3772	rBV2	334	391	0.05%	0.006%
95	13.204	3778	3783	3784	rBV3	1458	1103	0.13%	0.016%
96	13.271	3801	3804	3810	rBV4	419	536	0.06%	0.008%
97	13.413	3845	3848	3849	rBV4	396	235	0.03%	0.003%
98	13.455	3853	3861	3872	rVB2	3412	5644	0.67%	0.082%
99	13.580	3897	3900	3903	rBV2	397	243	0.03%	0.004%
100	14.223	4096	4100	4102	rBV3	496	422	0.05%	0.006%




Sum of corrected areas: 6914860

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033230.D
Acq On : 11 Dec 2023 22:19
Operator : SY/MD
Sample : 05730-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

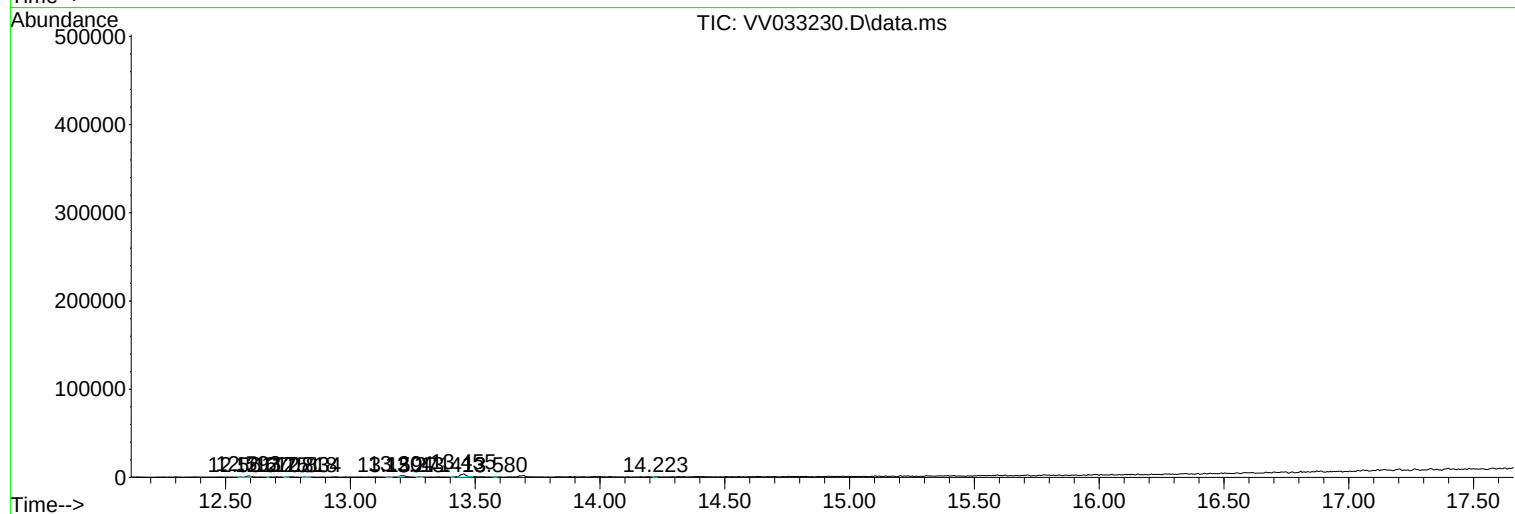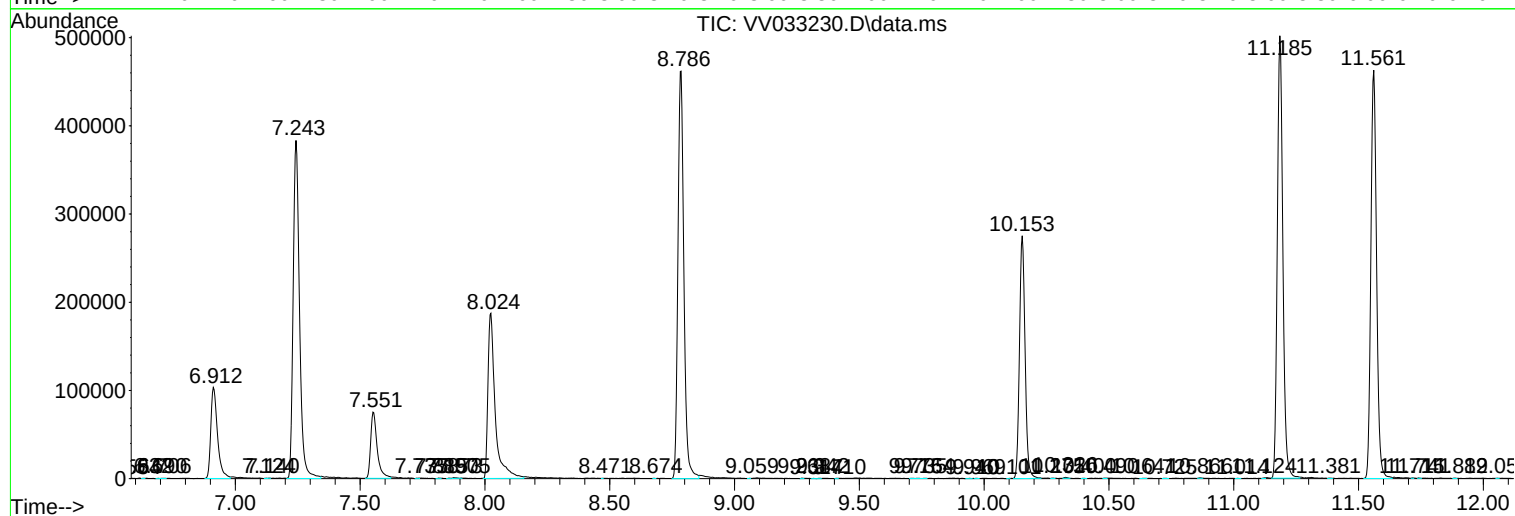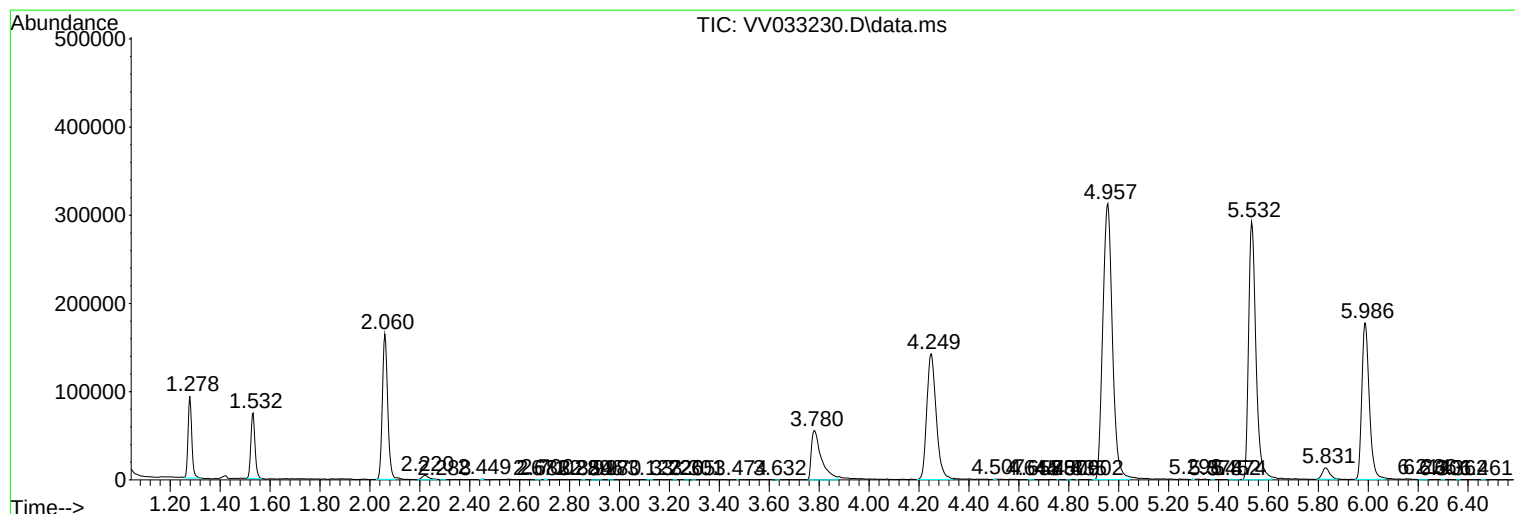

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033230.D
Acq On : 11 Dec 2023 22:19
Operator : SY/MD
Sample : 05730-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033230.D
Acq On : 11 Dec 2023 22:19
Operator : SY/MD
Sample : 05730-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------