

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033231.D
 Acq On : 11 Dec 2023 22:42
 Operator : SY/MD
 Sample : 05730-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	95453	100660	11.66%	1.338%
2	1.532	145	153	167	rVB	77908	92625	10.73%	1.231%
3	1.947	279	282	286	rBV2	586	528	0.06%	0.007%
4	2.060	306	317	332	rBV2	166373	252982	29.30%	3.362%
5	2.220	361	367	377	rVB2	3168	5041	0.58%	0.067%
6	2.310	392	395	397	rBV	274	184	0.02%	0.002%
7	2.436	431	434	436	rBV2	333	243	0.03%	0.003%
8	2.558	465	472	477	rBV3	771	1118	0.13%	0.015%
9	2.655	500	502	507	rVB	265	209	0.02%	0.003%
10	2.812	546	551	560	rVV2	336	422	0.05%	0.006%
11	2.864	560	567	571	rVB2	236	344	0.04%	0.005%
12	2.902	573	579	583	rBV2	245	315	0.04%	0.004%
13	3.040	621	622	625	rBV	367	232	0.03%	0.003%
14	3.082	632	635	638	rBV	293	232	0.03%	0.003%
15	3.098	638	640	642	rBV2	284	202	0.02%	0.003%
16	3.201	667	672	675	rBV2	294	289	0.03%	0.004%
17	3.269	690	693	696	rBV	300	239	0.03%	0.003%
18	3.288	697	699	705	rVB2	311	316	0.04%	0.004%
19	3.333	710	713	715	rVB2	305	201	0.02%	0.003%
20	3.500	763	765	771	rVV2	187	179	0.02%	0.002%
21	3.548	776	780	783	rBB	170	175	0.02%	0.002%
22	3.581	783	790	791	rBV2	307	353	0.04%	0.005%
23	3.635	804	807	810	rVB	355	190	0.02%	0.003%
24	3.706	827	829	835	rVB	239	238	0.03%	0.003%
25	3.783	843	853	883	rBV2	55332	163878	18.98%	2.178%
26	4.249	981	998	1029	rBV	146386	376691	43.63%	5.006%
27	4.593	1103	1105	1110	rVB3	369	245	0.03%	0.003%
28	4.654	1121	1124	1126	rVB	367	203	0.02%	0.003%
29	4.671	1126	1129	1131	rBV2	471	259	0.03%	0.003%
30	4.693	1134	1136	1138	rVV	320	171	0.02%	0.002%
31	4.728	1145	1147	1149	rVV	418	205	0.02%	0.003%
32	4.757	1152	1156	1158	rBV	404	177	0.02%	0.002%
33	4.806	1168	1171	1173	rBV	342	205	0.02%	0.003%
34	4.957	1201	1218	1246	rBV2	321356	863414	100.00%	11.474%
35	5.256	1308	1311	1314	rBV	562	334	0.04%	0.004%
36	5.445	1366	1370	1373	rBV2	443	343	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033231.D
 Acq On : 11 Dec 2023 22:42
 Operator : SY/MD
 Sample : 05730-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.474	1375	1379	1382	rVB2	560	460	0.05%	0.006%
38	5.532	1385	1397	1420	rBV	300913	613690	71.08%	8.155%
39	5.783	1473	1475	1477	rBV2	702	278	0.03%	0.004%
40	5.831	1478	1490	1515	rVV2	222343	459716	53.24%	6.109%
41	5.989	1526	1539	1562	rBV2	182226	375180	43.45%	4.986%
42	6.323	1638	1643	1647	rVB2	603	523	0.06%	0.007%
43	6.442	1676	1680	1683	rBV2	432	374	0.04%	0.005%
44	6.490	1693	1695	1699	rVV	278	208	0.02%	0.003%
45	6.523	1702	1705	1709	rVB2	403	271	0.03%	0.004%
46	6.825	1797	1799	1803	rBV	335	295	0.03%	0.004%
47	6.912	1816	1826	1853	rBV	106018	199754	23.14%	2.655%
48	7.150	1897	1900	1902	rBV2	406	262	0.03%	0.003%
49	7.243	1918	1929	1949	rBV	394806	692766	80.24%	9.206%
50	7.551	2016	2025	2055	rBV	78779	144644	16.75%	1.922%
51	7.915	2136	2138	2142	rVB2	456	279	0.03%	0.004%
52	8.024	2163	2172	2209	rBV	188780	374856	43.42%	4.981%
53	8.384	2279	2284	2286	rBV3	603	490	0.06%	0.007%
54	8.461	2306	2308	2309	rBV3	455	208	0.02%	0.003%
55	8.635	2359	2362	2367	rVB2	344	275	0.03%	0.004%
56	8.783	2397	2408	2440	rBV	476380	785481	90.97%	10.438%
57	8.950	2457	2460	2463	rBV3	597	513	0.06%	0.007%
58	9.085	2496	2502	2504	rBV2	534	558	0.06%	0.007%
59	9.201	2535	2538	2545	rVB2	358	526	0.06%	0.007%
60	9.233	2545	2548	2549	rBV	409	201	0.02%	0.003%
61	9.281	2561	2563	2565	rBV	278	161	0.02%	0.002%
62	9.352	2582	2585	2589	rBV2	285	255	0.03%	0.003%
63	9.410	2599	2603	2609	rBV	281	365	0.04%	0.005%
64	9.522	2633	2638	2640	rBV	377	302	0.03%	0.004%
65	9.555	2644	2648	2650	rVB2	308	229	0.03%	0.003%
66	9.574	2651	2654	2658	rBV	342	333	0.04%	0.004%
67	9.593	2658	2660	2664	rVB2	370	232	0.03%	0.003%
68	9.622	2664	2669	2673	rBV2	223	287	0.03%	0.004%
69	9.667	2678	2683	2684	rBV2	311	270	0.03%	0.004%
70	9.702	2691	2694	2701	rVB2	297	336	0.04%	0.004%
71	9.953	2770	2772	2778	rVB2	438	225	0.03%	0.003%
72	10.001	2782	2787	2790	rBV2	318	340	0.04%	0.005%
73	10.037	2794	2798	2799	rBV	393	250	0.03%	0.003%
74	10.153	2822	2834	2862	rBV	278502	438192	50.75%	5.823%
75	10.487	2934	2938	2944	rVB3	570	663	0.08%	0.009%
76	10.548	2954	2957	2961	rBV2	469	495	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033231.D
 Acq On : 11 Dec 2023 22:42
 Operator : SY/MD
 Sample : 05730-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.628	2980	2982	2986	rBV2	422	383	0.04%	0.005%
78	10.680	2996	2998	3001	rVB	423	204	0.02%	0.003%
79	10.699	3001	3004	3006	rBV2	360	307	0.04%	0.004%
80	10.902	3063	3067	3070	rBV2	250	228	0.03%	0.003%
81	10.940	3075	3079	3081	rBV	206	184	0.02%	0.002%
82	10.985	3090	3093	3097	rVB2	209	178	0.02%	0.002%
83	11.185	3144	3155	3179	rBV	512788	791492	91.67%	10.518%
84	11.352	3204	3207	3208	rBV	490	301	0.03%	0.004%
85	11.561	3260	3272	3299	rBV	488590	765072	88.61%	10.167%
86	11.857	3362	3364	3369	rBV	201	189	0.02%	0.003%
87	12.008	3406	3411	3416	rBV2	222	287	0.03%	0.004%
88	12.525	3569	3572	3573	rBV2	468	246	0.03%	0.003%
89	12.587	3584	3591	3593	rBV3	907	816	0.09%	0.011%
90	13.262	3797	3801	3803	rBV2	459	345	0.04%	0.005%
91	13.320	3817	3819	3822	rBV	400	273	0.03%	0.004%
92	13.452	3854	3860	3867	rBV2	2703	3515	0.41%	0.047%
93	13.593	3899	3904	3906	rBV2	490	370	0.04%	0.005%
94	13.773	3957	3960	3962	rBV2	353	264	0.03%	0.004%
95	13.831	3973	3978	3981	rBV3	384	448	0.05%	0.006%
96	13.853	3983	3985	3989	rVV3	318	212	0.02%	0.003%
97	13.931	4007	4009	4010	rBV	397	167	0.02%	0.002%
98	14.352	4135	4140	4144	rBV3	495	508	0.06%	0.007%
99	14.558	4202	4204	4207	rBV3	640	355	0.04%	0.005%
100	14.705	4249	4250	4253	rBV2	710	313	0.04%	0.004%


Sum of corrected areas: 7525042

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033231.D
Acq On : 11 Dec 2023 22:42
Operator : SY/MD
Sample : 05730-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

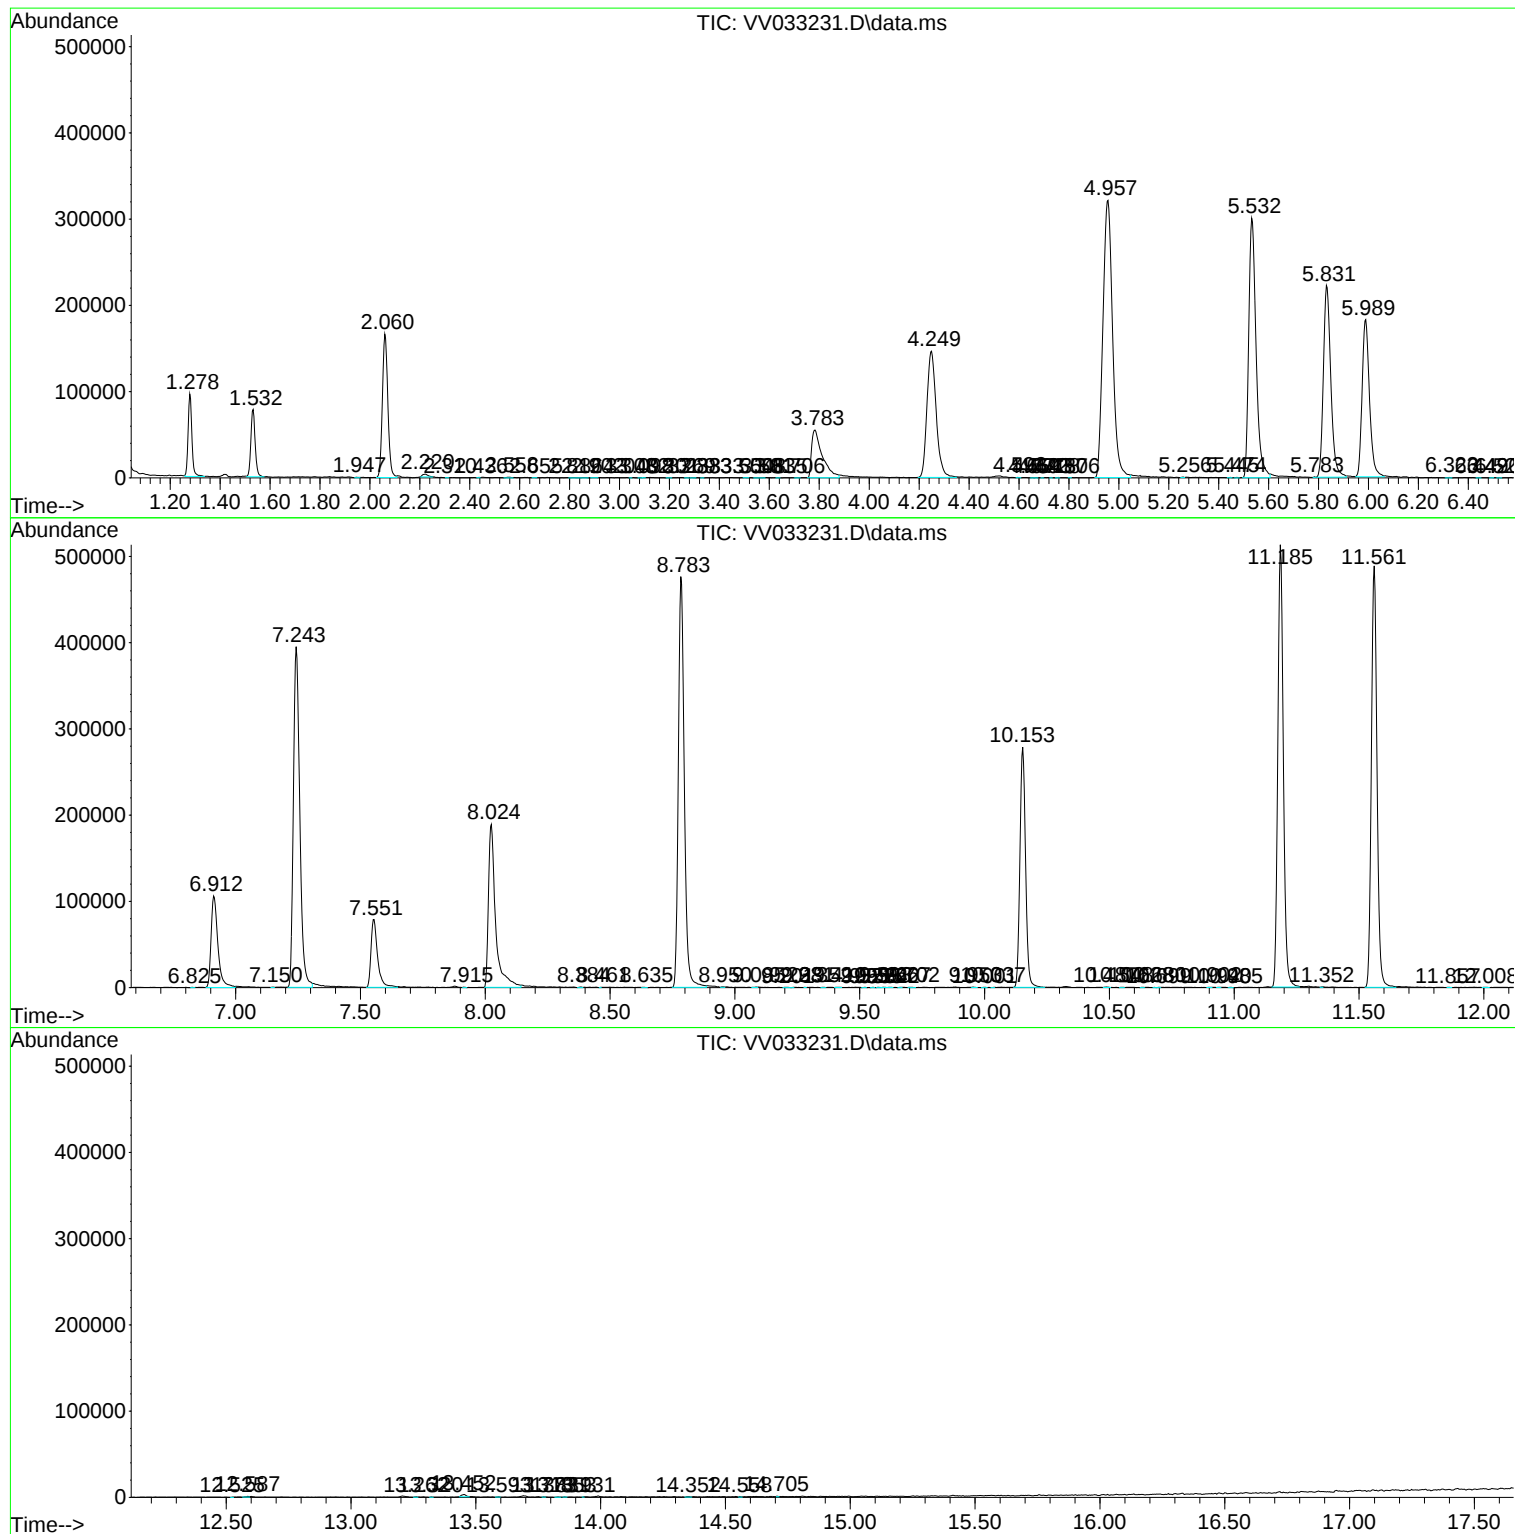

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033231.D
Acq On : 11 Dec 2023 22:42
Operator : SY/MD
Sample : 05730-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033231.D
Acq On : 11 Dec 2023 22:42
Operator : SY/MD
Sample : 05730-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc