

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033232.D
 Acq On : 11 Dec 2023 23:05
 Operator : SY/MD
 Sample : 05730-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	92406	95039	11.38%	1.382%
2	1.532	146	153	170	rVB	74660	89458	10.71%	1.301%
3	1.896	265	266	270	rVB2	723	304	0.04%	0.004%
4	2.060	305	317	335	rBV	154479	231344	27.70%	3.364%
5	2.220	352	367	376	rBV3	5107	9896	1.18%	0.144%
6	2.320	395	398	402	rBV3	323	256	0.03%	0.004%
7	2.433	430	433	435	rBV2	298	250	0.03%	0.004%
8	2.619	486	491	493	rBV2	267	249	0.03%	0.004%
9	2.667	503	506	508	rBV2	268	213	0.03%	0.003%
10	2.732	523	526	530	rBV2	303	220	0.03%	0.003%
11	2.934	586	589	593	rBV2	371	321	0.04%	0.005%
12	3.056	624	627	630	rBV2	355	204	0.02%	0.003%
13	3.130	646	650	652	rBV3	310	200	0.02%	0.003%
14	3.179	661	665	670	rBB2	366	368	0.04%	0.005%
15	3.220	674	678	682	rVV2	222	207	0.02%	0.003%
16	3.288	696	699	702	rVV	306	181	0.02%	0.003%
17	3.346	714	717	721	rVV2	404	363	0.04%	0.005%
18	3.372	723	725	728	rVV2	375	203	0.02%	0.003%
19	3.429	739	743	747	rVB	493	391	0.05%	0.006%
20	3.458	747	752	755	rBV2	330	363	0.04%	0.005%
21	3.532	772	775	782	rBV2	272	428	0.05%	0.006%
22	3.725	834	835	837	rBV	362	159	0.02%	0.002%
23	3.780	844	852	876	rBV	54419	142817	17.10%	2.076%
24	4.249	980	998	1023	rBV2	145259	370519	44.36%	5.387%
25	4.558	1089	1094	1096	rBV3	645	528	0.06%	0.008%
26	4.654	1120	1124	1127	rBV3	302	293	0.04%	0.004%
27	4.722	1143	1145	1149	rVB	299	161	0.02%	0.002%
28	4.754	1149	1155	1157	rBV2	312	306	0.04%	0.004%
29	4.957	1201	1218	1241	rBV3	316791	835285	100.00%	12.145%
30	5.240	1303	1306	1309	rBV3	573	478	0.06%	0.007%
31	5.462	1372	1375	1380	rBV2	339	216	0.03%	0.003%
32	5.532	1386	1397	1423	rBV2	290390	598873	71.70%	8.707%
33	5.825	1480	1488	1511	rVB5	12758	28484	3.41%	0.414%
34	5.989	1526	1539	1560	rBV2	178221	369998	44.30%	5.380%
35	6.310	1637	1639	1641	rBV2	242	162	0.02%	0.002%
36	6.378	1658	1660	1666	rBV2	234	229	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033232.D
 Acq On : 11 Dec 2023 23:05
 Operator : SY/MD
 Sample : 05730-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.458	1683	1685	1688	rBV2	505	236	0.03%	0.003%
38	6.506	1698	1700	1705	rVB2	214	162	0.02%	0.002%
39	6.635	1738	1740	1743	rBV	261	196	0.02%	0.003%
40	6.732	1766	1770	1775	rVB	229	207	0.02%	0.003%
41	6.912	1815	1826	1845	rBV	100091	189493	22.69%	2.755%
42	7.137	1893	1896	1897	rBV	339	176	0.02%	0.003%
43	7.243	1918	1929	1954	rBV	378031	671435	80.38%	9.762%
44	7.551	2016	2025	2050	rBV3	74524	137254	16.43%	1.996%
45	7.844	2112	2116	2118	rBV	317	219	0.03%	0.003%
46	7.873	2120	2125	2128	rBV3	770	785	0.09%	0.011%
47	7.908	2134	2136	2139	rVB2	634	296	0.04%	0.004%
48	8.024	2163	2172	2209	rBV	187746	370579	44.37%	5.388%
49	8.349	2270	2273	2275	rVB2	488	203	0.02%	0.003%
50	8.365	2275	2278	2287	rVB2	628	656	0.08%	0.010%
51	8.404	2287	2290	2295	rBV2	266	235	0.03%	0.003%
52	8.603	2348	2352	2355	rBV	193	204	0.02%	0.003%
53	8.783	2397	2408	2437	rBV	462860	770092	92.20%	11.197%
54	9.079	2495	2500	2502	rBV2	520	456	0.05%	0.007%
55	9.121	2510	2513	2515	rVB2	400	236	0.03%	0.003%
56	9.358	2585	2587	2593	rBV2	403	387	0.05%	0.006%
57	9.397	2596	2599	2602	rBV	250	224	0.03%	0.003%
58	9.574	2651	2654	2657	rBV2	297	161	0.02%	0.002%
59	9.709	2691	2696	2698	rBV2	194	178	0.02%	0.003%
60	9.748	2705	2708	2711	rBV	452	348	0.04%	0.005%
61	9.866	2742	2745	2750	rBV2	417	500	0.06%	0.007%
62	9.934	2761	2766	2769	rBV3	282	222	0.03%	0.003%
63	10.008	2786	2789	2795	rVB2	233	195	0.02%	0.003%
64	10.037	2795	2798	2802	rBV2	271	249	0.03%	0.004%
65	10.069	2805	2808	2812	rBV2	242	215	0.03%	0.003%
66	10.153	2822	2834	2858	rBV	273547	429475	51.42%	6.244%
67	10.426	2915	2919	2923	rVB2	447	269	0.03%	0.004%
68	10.448	2923	2926	2934	rBV	372	389	0.05%	0.006%
69	10.484	2934	2937	2940	rBV2	401	295	0.04%	0.004%
70	10.590	2964	2970	2973	rBV2	337	456	0.05%	0.007%
71	10.764	3021	3024	3030	rVB2	208	234	0.03%	0.003%
72	10.828	3040	3044	3047	rBV2	253	203	0.02%	0.003%
73	10.892	3062	3064	3069	rBV2	295	223	0.03%	0.003%
74	10.979	3087	3091	3094	rBV	348	352	0.04%	0.005%
75	11.127	3134	3137	3142	rBV	582	492	0.06%	0.007%
76	11.185	3144	3155	3182	rVV	507669	775281	92.82%	11.272%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033232.D
 Acq On : 11 Dec 2023 23:05
 Operator : SY/MD
 Sample : 05730-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.368	3209	3212	3215	rBV2	442	282	0.03%	0.004%
78	11.413	3224	3226	3229	rBV2	247	170	0.02%	0.002%
79	11.561	3259	3272	3296	rBV	473897	737788	88.33%	10.727%
80	11.834	3355	3357	3360	rBV	232	181	0.02%	0.003%
81	11.963	3393	3397	3401	rBV2	237	239	0.03%	0.003%
82	11.989	3401	3405	3408	rBV	275	193	0.02%	0.003%
83	12.008	3408	3411	3412	rBV	277	183	0.02%	0.003%
84	12.310	3502	3505	3506	rBV	320	165	0.02%	0.002%
85	12.329	3506	3511	3512	rBV2	428	289	0.03%	0.004%
86	12.368	3520	3523	3528	rBV	322	303	0.04%	0.004%
87	12.432	3539	3543	3546	rBV	274	273	0.03%	0.004%
88	12.664	3612	3615	3617	rBV	274	164	0.02%	0.002%
89	12.850	3669	3673	3678	rBV2	413	541	0.06%	0.008%
90	12.889	3683	3685	3689	rVB	307	186	0.02%	0.003%
91	12.905	3689	3690	3694	rBV	257	165	0.02%	0.002%
92	13.082	3743	3745	3750	rVB3	299	154	0.02%	0.002%
93	13.284	3805	3808	3817	rVB2	542	653	0.08%	0.009%
94	13.606	3905	3908	3911	rBV2	295	180	0.02%	0.003%
95	13.693	3927	3935	3939	rBV4	1032	1403	0.17%	0.020%
96	13.731	3944	3947	3949	rBV	522	373	0.04%	0.005%
97	14.043	4040	4044	4045	rBV	701	439	0.05%	0.006%
98	14.079	4052	4055	4056	rBV	377	205	0.02%	0.003%
99	14.696	4245	4247	4249	rBV2	509	240	0.03%	0.003%
100	14.757	4264	4266	4273	rBV5	712	628	0.08%	0.009%




Sum of corrected areas: 6877831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033232.D
Acq On : 11 Dec 2023 23:05
Operator : SY/MD
Sample : 05730-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

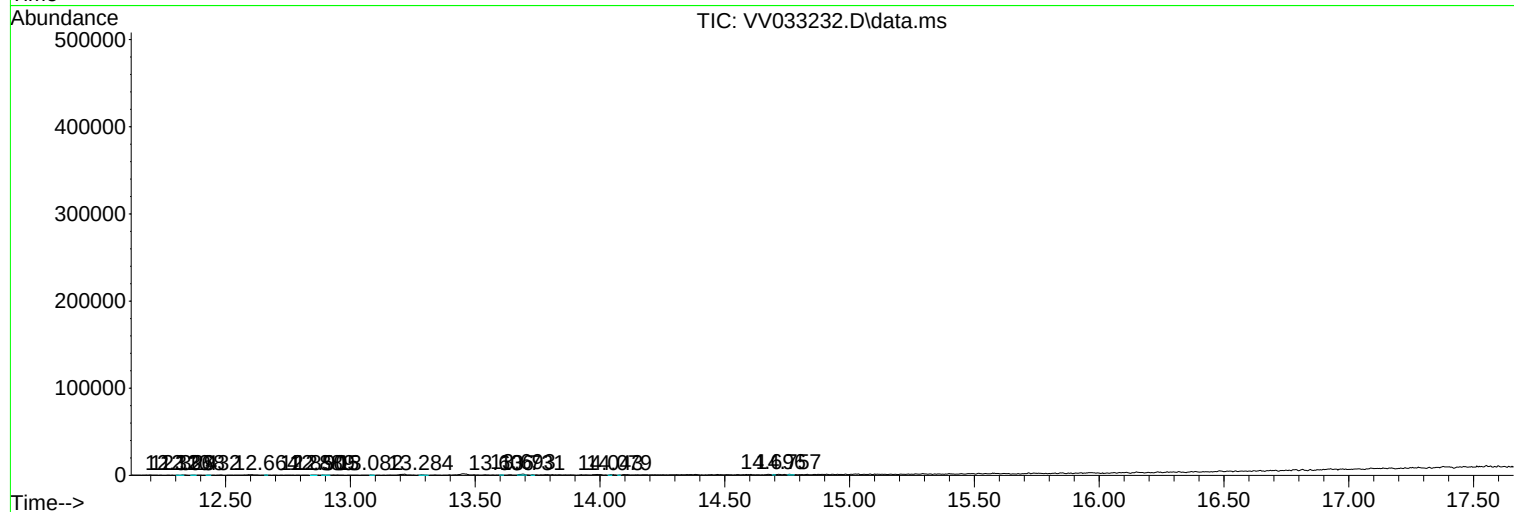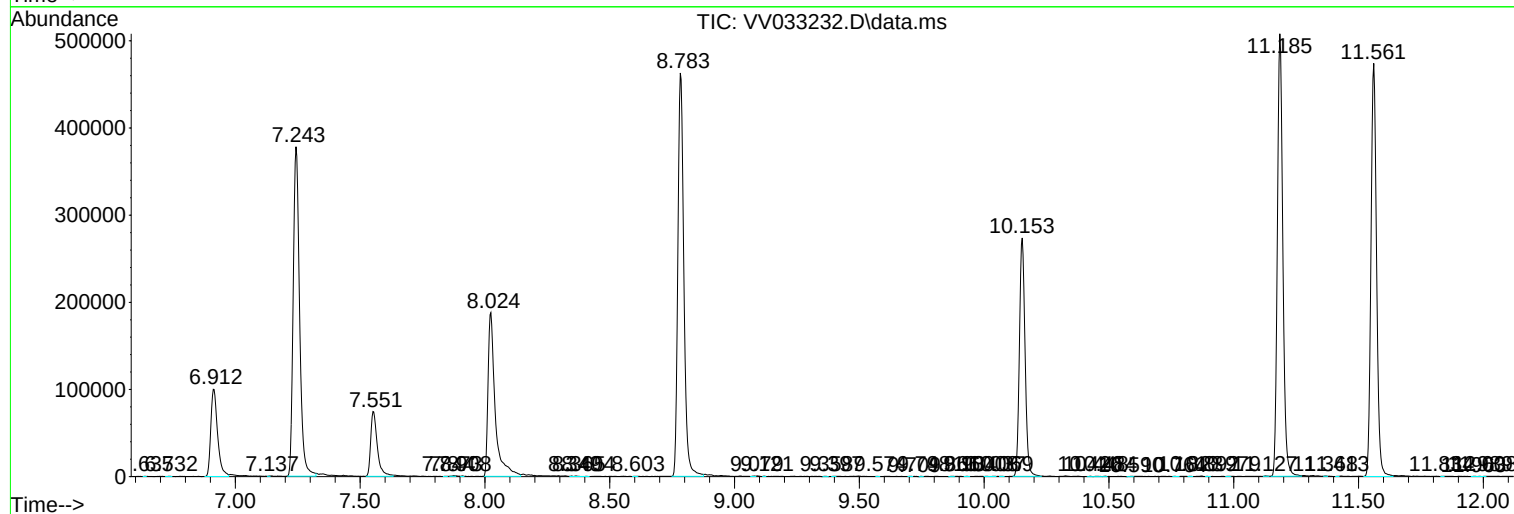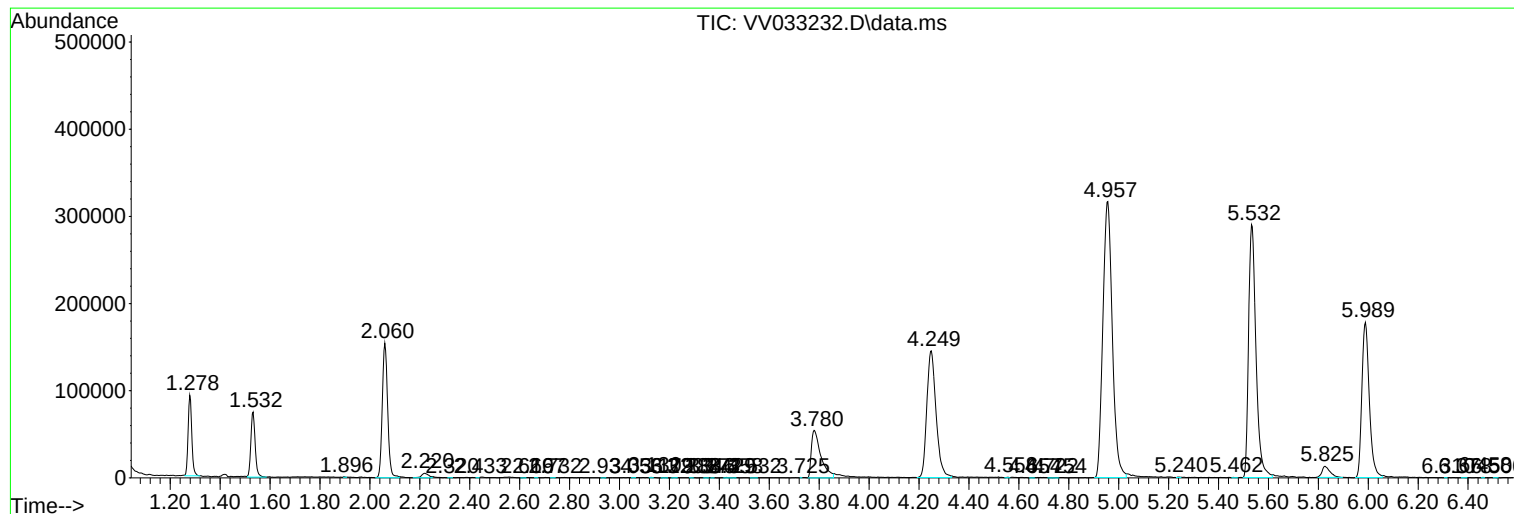

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033232.D
Acq On : 11 Dec 2023 23:05
Operator : SY/MD
Sample : 05730-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033232.D
Acq On : 11 Dec 2023 23:05
Operator : SY/MD
Sample : 05730-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc