

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033233.D
 Acq On : 11 Dec 2023 23:28
 Operator : SY/MD
 Sample : 05730-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	90748	93819	10.38%	1.207%
2	1.532	145	153	169	rVB	73764	88113	9.75%	1.134%
3	2.060	306	317	338	rBV2	168159	265870	29.41%	3.421%
4	2.217	360	366	383	rVB2	3842	7920	0.88%	0.102%
5	2.436	431	434	435	rBV2	635	359	0.04%	0.005%
6	2.561	466	473	476	rBV3	792	1047	0.12%	0.013%
7	2.606	484	487	492	rBV	338	276	0.03%	0.004%
8	2.754	530	533	539	rBV2	286	205	0.02%	0.003%
9	2.796	544	546	550	rVB	382	226	0.02%	0.003%
10	2.838	555	559	562	rBV	262	269	0.03%	0.003%
11	2.915	580	583	585	rBV	294	197	0.02%	0.003%
12	2.986	602	605	609	rVB2	249	234	0.03%	0.003%
13	3.047	620	624	627	rBV2	299	281	0.03%	0.004%
14	3.101	635	641	642	rBV	667	477	0.05%	0.006%
15	3.269	691	693	697	rBV	400	247	0.03%	0.003%
16	3.381	723	728	731	rBV2	380	344	0.04%	0.004%
17	3.433	739	744	747	rBV2	292	219	0.02%	0.003%
18	3.523	768	772	774	rVV2	244	193	0.02%	0.002%
19	3.783	843	853	879	rBV3	52555	179336	19.83%	2.308%
20	4.246	983	997	1026	rBV	142340	357112	39.50%	4.595%
21	4.474	1065	1068	1070	rBV2	601	427	0.05%	0.005%
22	4.513	1073	1080	1084	rBV5	4676	7238	0.80%	0.093%
23	4.603	1105	1108	1112	rBV2	490	399	0.04%	0.005%
24	4.709	1139	1141	1145	rVB2	367	229	0.03%	0.003%
25	4.957	1201	1218	1245	rBV2	313461	834923	92.34%	10.744%
26	5.532	1386	1397	1429	rVV	290145	603058	66.70%	7.760%
27	5.831	1477	1490	1522	rBV	446108	904163	100.00%	11.635%
28	5.989	1527	1539	1568	rVB2	179160	371756	41.12%	4.784%
29	6.236	1610	1616	1617	rBV	420	402	0.04%	0.005%
30	6.278	1624	1629	1632	rBV2	552	429	0.05%	0.006%
31	6.336	1641	1647	1649	rBV2	260	295	0.03%	0.004%
32	6.439	1674	1679	1682	rBV	166	195	0.02%	0.003%
33	6.510	1697	1701	1704	rBV2	485	357	0.04%	0.005%
34	6.551	1712	1714	1719	rBV2	273	237	0.03%	0.003%
35	6.738	1770	1772	1777	rBV	334	197	0.02%	0.003%
36	6.863	1806	1811	1815	rBV2	344	451	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033233.D
 Acq On : 11 Dec 2023 23:28
 Operator : SY/MD
 Sample : 05730-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.912	1816	1826	1850	rVV	100768	189424	20.95%	2.438%
38	7.088	1878	1881	1887	rVB2	372	294	0.03%	0.004%
39	7.175	1906	1908	1915	rVB4	377	353	0.04%	0.005%
40	7.243	1918	1929	1950	rBV	388919	670524	74.16%	8.629%
41	7.503	2008	2010	2011	rBV	480	211	0.02%	0.003%
42	7.551	2017	2025	2045	rBV2	73205	131497	14.54%	1.692%
43	7.805	2102	2104	2107	rBV	314	214	0.02%	0.003%
44	7.831	2107	2112	2114	rVB3	329	213	0.02%	0.003%
45	7.873	2118	2125	2133	rBV4	1496	2057	0.23%	0.026%
46	7.950	2144	2149	2151	rBV2	432	318	0.04%	0.004%
47	8.024	2163	2172	2189	rBV	177917	326898	36.15%	4.207%
48	8.355	2272	2275	2280	rBV3	487	583	0.06%	0.008%
49	8.445	2301	2303	2307	rBV2	415	377	0.04%	0.005%
50	8.529	2325	2329	2331	rBV2	465	268	0.03%	0.003%
51	8.571	2339	2342	2345	rBV2	363	303	0.03%	0.004%
52	8.712	2381	2386	2387	rBB3	350	198	0.02%	0.003%
53	8.731	2387	2392	2397	rBV2	415	556	0.06%	0.007%
54	8.783	2397	2408	2435	rBV	463841	771023	85.27%	9.922%
55	9.088	2499	2503	2506	rBV3	319	212	0.02%	0.003%
56	9.204	2535	2539	2540	rBV	323	204	0.02%	0.003%
57	9.291	2563	2566	2571	rBV2	260	277	0.03%	0.004%
58	9.339	2578	2581	2585	rBV2	252	205	0.02%	0.003%
59	9.368	2585	2590	2592	rBV	332	279	0.03%	0.004%
60	9.407	2599	2602	2606	rVB2	371	296	0.03%	0.004%
61	9.432	2606	2610	2615	rBB2	387	470	0.05%	0.006%
62	9.461	2616	2619	2621	rBV	329	247	0.03%	0.003%
63	9.516	2634	2636	2640	rBV2	222	196	0.02%	0.003%
64	9.567	2646	2652	2656	rBV	422	354	0.04%	0.005%
65	9.593	2656	2660	2666	rVB2	347	500	0.06%	0.006%
66	9.622	2666	2669	2674	rBV2	299	333	0.04%	0.004%
67	9.870	2743	2746	2752	rBV2	575	642	0.07%	0.008%
68	10.153	2822	2834	2860	rBV	262625	421010	46.56%	5.418%
69	10.255	2864	2866	2867	rBV	424	200	0.02%	0.003%
70	10.284	2872	2875	2877	rBV	419	292	0.03%	0.004%
71	10.326	2881	2888	2896	rVB2	1516	2220	0.25%	0.029%
72	10.410	2911	2914	2919	rBV2	247	288	0.03%	0.004%
73	10.532	2949	2952	2955	rVV	254	233	0.03%	0.003%
74	10.921	3070	3073	3076	rBV	292	317	0.04%	0.004%
75	11.130	3133	3138	3139	rBV2	667	546	0.06%	0.007%
76	11.185	3144	3155	3179	rBV	506286	776665	85.90%	9.994%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033233.D
 Acq On : 11 Dec 2023 23:28
 Operator : SY/MD
 Sample : 05730-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.407	3221	3224	3227	rBV3	316	263	0.03%	0.003%
78	11.561	3260	3272	3298	rBV	468528	736366	81.44%	9.476%
79	12.130	3445	3449	3452	rBV3	434	353	0.04%	0.005%
80	12.387	3526	3529	3532	rBV	344	284	0.03%	0.004%
81	12.455	3547	3550	3553	rBV	329	266	0.03%	0.003%
82	12.593	3591	3593	3596	rBV2	521	332	0.04%	0.004%
83	12.638	3604	3607	3614	rVB	506	399	0.04%	0.005%
84	12.673	3614	3618	3621	rBV2	429	325	0.04%	0.004%
85	12.734	3631	3637	3641	rBV3	387	447	0.05%	0.006%
86	12.972	3706	3711	3716	rVB2	359	410	0.05%	0.005%
87	13.046	3730	3734	3736	rBV2	288	193	0.02%	0.002%
88	13.104	3748	3752	3761	rBV3	458	661	0.07%	0.009%
89	13.149	3763	3766	3772	rBV2	315	349	0.04%	0.004%
90	13.178	3772	3775	3777	rBV	271	201	0.02%	0.003%
91	13.214	3780	3786	3794	rVB4	1328	1974	0.22%	0.025%
92	13.252	3794	3798	3800	rBV2	233	202	0.02%	0.003%
93	13.307	3810	3815	3817	rBV2	496	390	0.04%	0.005%
94	13.342	3824	3826	3829	rBV	299	228	0.03%	0.003%
95	13.410	3843	3847	3851	rBV	236	241	0.03%	0.003%
96	13.455	3851	3861	3868	rBV3	1697	2851	0.32%	0.037%
97	13.889	3992	3996	3999	rBV3	585	519	0.06%	0.007%
98	14.432	4163	4165	4168	rBV	605	321	0.04%	0.004%
99	14.509	4184	4189	4191	rBV	517	455	0.05%	0.006%
100	14.561	4203	4205	4207	rBV	469	209	0.02%	0.003%


Sum of corrected areas: 7771036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033233.D
Acq On : 11 Dec 2023 23:28
Operator : SY/MD
Sample : 05730-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

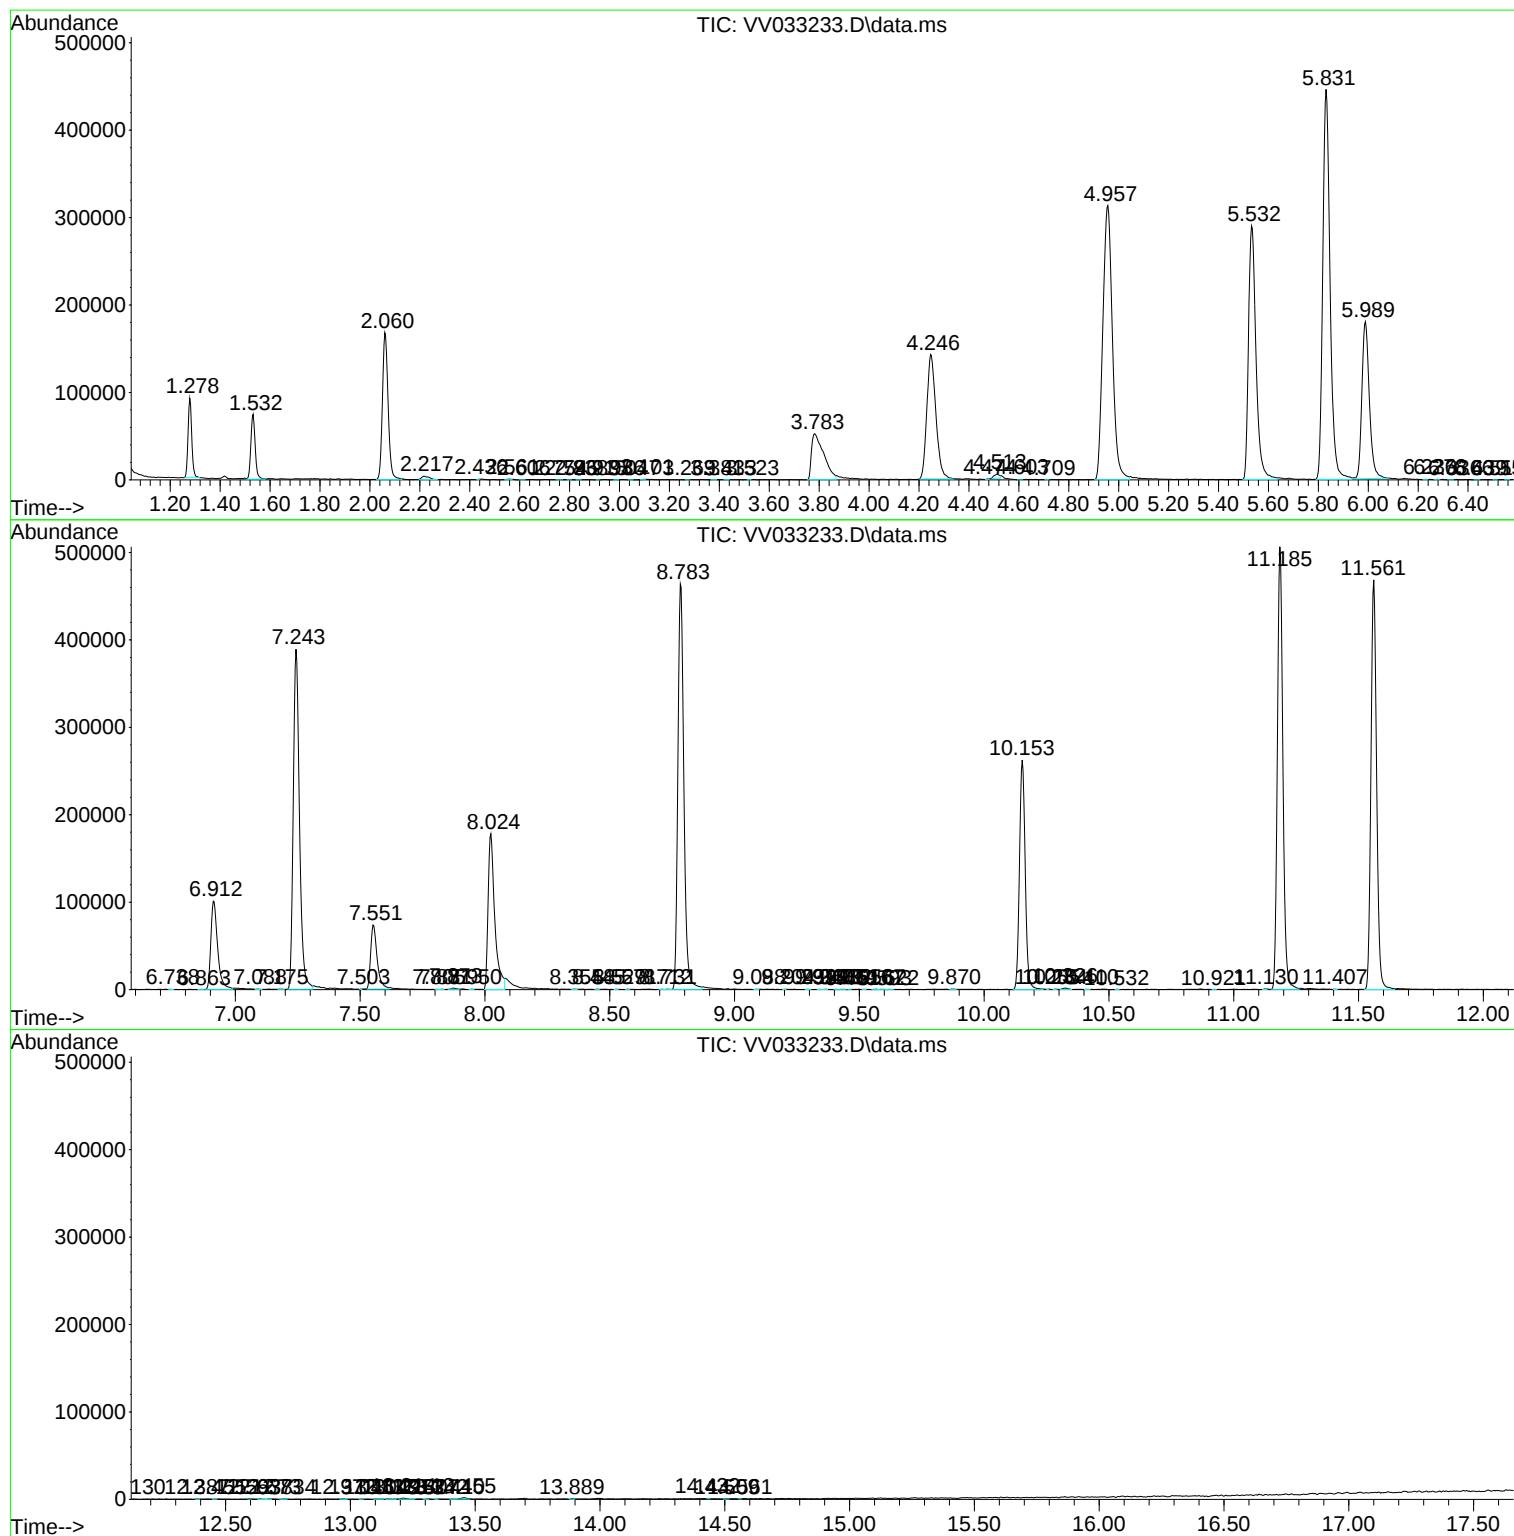

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033233.D
Acq On : 11 Dec 2023 23:28
Operator : SY/MD
Sample : 05730-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033233.D
Acq On : 11 Dec 2023 23:28
Operator : SY/MD
Sample : 05730-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------