

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033249.D
 Acq On : 12 Dec 2023 05:39
 Operator : SY/MD
 Sample : 05751-13MS
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHF6MS

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	14	20	33	rVB	258671	253487	11.90%	0.693%
2	1.166	33	39	49	rBV	54222	69467	3.26%	0.190%
3	1.214	49	54	67	rVB	149624	153706	7.21%	0.420%
4	1.281	67	75	102	rBV2	278542	314914	14.78%	0.861%
5	1.423	112	119	127	rVB7	6825	8893	0.42%	0.024%
6	1.484	130	138	146	rBV	129478	151571	7.11%	0.414%
7	1.532	146	153	155	rBV	98075	104998	4.93%	0.287%
8	1.712	200	209	227	rBV	279673	379172	17.79%	1.037%
9	1.976	288	291	295	rBV2	742	572	0.03%	0.002%
10	2.069	307	320	328	rBV4	769140	1303473	61.17%	3.563%
11	2.240	356	373	392	rVB2	202520	388688	18.24%	1.063%
12	2.368	405	413	426	rBV	49607	84000	3.94%	0.230%
13	2.445	427	437	456	rVB	203252	335490	15.74%	0.917%
14	2.561	467	473	483	rVB6	2944	4898	0.23%	0.013%
15	2.696	501	515	543	rVV2	482408	969339	45.49%	2.650%
16	2.834	556	558	563	rBV4	640	508	0.02%	0.001%
17	2.867	565	568	571	rBV3	726	493	0.02%	0.001%
18	2.889	572	575	579	rVB3	518	341	0.02%	0.001%
19	2.982	601	604	608	rBV3	610	504	0.02%	0.001%
20	3.111	630	644	670	rVV2	168973	355769	16.70%	0.973%
21	3.310	703	706	710	rVB2	570	477	0.02%	0.001%
22	3.503	762	766	768	rVB2	425	328	0.02%	0.001%
23	3.812	841	862	872	rBV2	220210	635547	29.83%	1.737%
24	4.146	948	966	983	rBV2	144094	374126	17.56%	1.023%
25	4.262	986	1002	1030	rVB4	244449	883996	41.49%	2.417%
26	4.510	1061	1079	1091	rBV	223287	577794	27.12%	1.579%
27	4.583	1093	1102	1126	rVV2	228103	559193	26.24%	1.529%
28	4.735	1130	1149	1172	rBV2	215280	529057	24.83%	1.446%
29	4.860	1186	1188	1194	rVB4	553	519	0.02%	0.001%
30	4.956	1201	1218	1227	rBV2	383832	1000578	46.96%	2.735%
31	5.297	1320	1324	1327	rVB3	730	503	0.02%	0.001%
32	5.368	1343	1346	1349	rBV3	448	369	0.02%	0.001%
33	5.474	1377	1379	1386	rVB3	403	399	0.02%	0.001%
34	5.532	1386	1397	1424	rBV	297959	610281	28.64%	1.668%
35	5.831	1477	1490	1525	rBV	608361	1221933	57.35%	3.340%
36	5.989	1526	1539	1548	rBV	202989	406627	19.08%	1.112%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033249.D
 Acq On : 12 Dec 2023 05:39
 Operator : SY/MD
 Sample : 05751-13MS
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHF6MS

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.050	1549	1558	1565	rBV	282932	511313	24.00%	1.398%
38	6.239	1610	1617	1627	rVB	2738	5152	0.24%	0.014%
39	6.320	1638	1642	1644	rVB4	460	363	0.02%	0.001%
40	6.378	1655	1660	1662	rBV4	636	627	0.03%	0.002%
41	6.432	1663	1677	1701	rBV	209397	404131	18.97%	1.105%
42	6.542	1708	1711	1716	rVV4	499	476	0.02%	0.001%
43	6.763	1776	1780	1782	rVB	547	331	0.02%	0.001%
44	6.911	1816	1826	1832	rBV	130767	215894	10.13%	0.590%
45	6.953	1832	1839	1863	rVB	247850	445662	20.91%	1.218%
46	7.153	1890	1901	1918	rBV	330032	577027	27.08%	1.577%
47	7.243	1918	1929	1941	rVV	510056	891452	41.84%	2.437%
48	7.313	1942	1951	1975	rVB	584001	993816	46.64%	2.717%
49	7.554	2016	2026	2027	rBV	110591	128198	6.02%	0.350%
50	7.580	2029	2034	2060	rVB	263454	435261	20.43%	1.190%
51	7.767	2081	2092	2115	rBV	330147	564282	26.48%	1.543%
52	7.905	2123	2135	2157	rVB	409694	685378	32.16%	1.874%
53	8.021	2163	2171	2180	rBV	214894	352183	16.53%	0.963%
54	8.072	2180	2187	2207	rVV	266211	451104	21.17%	1.233%
55	8.175	2209	2219	2240	rVV	239465	412440	19.36%	1.127%
56	8.281	2240	2252	2281	rVB	173603	312649	14.67%	0.855%
57	8.426	2295	2297	2302	rVB4	561	472	0.02%	0.001%
58	8.471	2306	2311	2314	rVB3	646	540	0.03%	0.001%
59	8.786	2397	2409	2413	rBV	509799	805317	37.79%	2.201%
60	8.947	2448	2459	2486	rVB	695392	1079311	50.65%	2.950%
61	9.072	2487	2498	2524	rVB	673408	1081460	50.75%	2.956%
62	9.291	2564	2566	2572	rVB3	758	584	0.03%	0.002%
63	9.397	2593	2599	2601	rBV2	420	348	0.02%	0.001%
64	9.487	2612	2627	2657	rBV4	933076	2130838	100.00%	5.825%
65	9.664	2671	2682	2701	rBV	221603	361739	16.98%	0.989%
66	9.866	2732	2745	2769	rBV	819267	1245373	58.45%	3.404%
67	10.008	2787	2789	2795	rVB5	591	380	0.02%	0.001%
68	10.082	2807	2812	2815	rBV4	500	423	0.02%	0.001%
69	10.152	2822	2834	2838	rBV	342820	536916	25.20%	1.468%
70	10.284	2873	2875	2880	rVV4	742	553	0.03%	0.002%
71	10.323	2882	2887	2897	rVB4	3224	4358	0.20%	0.012%
72	10.387	2902	2907	2911	rBV3	1292	1492	0.07%	0.004%
73	10.477	2923	2935	2956	rBV	785547	1161979	54.53%	3.176%
74	10.683	2988	2999	3008	rVB4	3407	5606	0.26%	0.015%
75	10.805	3029	3037	3041	rBV6	9525	13115	0.62%	0.036%
76	10.850	3041	3051	3074	rVB	822710	1204386	56.52%	3.292%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033249.D
 Acq On : 12 Dec 2023 05:39
 Operator : SY/MD
 Sample : 05751-13MS
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHF6MS

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.985	3089	3093	3095	rBV3	657	397	0.02%	0.001%
78	11.117	3122	3134	3145	rBV	642468	989460	46.44%	2.705%
79	11.188	3145	3156	3158	rBV	677887	908267	42.62%	2.483%
80	11.567	3260	3274	3299	rBV2	829705	1972337	92.56%	5.392%
81	11.741	3324	3328	3332	rVB4	652	632	0.03%	0.002%
82	12.117	3439	3445	3448	rBV	288	341	0.02%	0.001%
83	12.201	3467	3471	3477	rVB3	772	812	0.04%	0.002%
84	12.365	3511	3522	3543	rVB	151574	240141	11.27%	0.656%
85	12.580	3576	3589	3616	rBV	633296	972202	45.63%	2.658%
86	12.975	3709	3712	3719	rVB3	383	499	0.02%	0.001%
87	13.020	3719	3726	3728	rBV2	616	656	0.03%	0.002%
88	13.197	3768	3781	3805	rBV	597004	906250	42.53%	2.477%
89	13.281	3805	3807	3810	rBV3	573	332	0.02%	0.001%
90	13.438	3843	3856	3880	rBV	589169	919398	43.15%	2.513%
91	13.680	3919	3931	3949	rBV	620712	959526	45.03%	2.623%
92	13.943	4009	4013	4014	rBV2	664	421	0.02%	0.001%
93	14.265	4109	4113	4118	rBV2	508	609	0.03%	0.002%
94	14.377	4143	4148	4150	rBV2	483	455	0.02%	0.001%
95	14.454	4168	4172	4181	rVB4	1014	1119	0.05%	0.003%
96	14.532	4194	4196	4200	rBV3	529	491	0.02%	0.001%
97	14.564	4204	4206	4211	rVB5	736	551	0.03%	0.002%
98	15.040	4352	4354	4357	rBV2	656	452	0.02%	0.001%
99	15.239	4412	4416	4418	rBV3	512	359	0.02%	0.001%
100	15.406	4466	4468	4473	rBV4	506	412	0.02%	0.001%




Sum of corrected areas: 36581058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033249.D
Acq On : 12 Dec 2023 05:39
Operator : SY/MD
Sample : 05751-13MS
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHF6MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

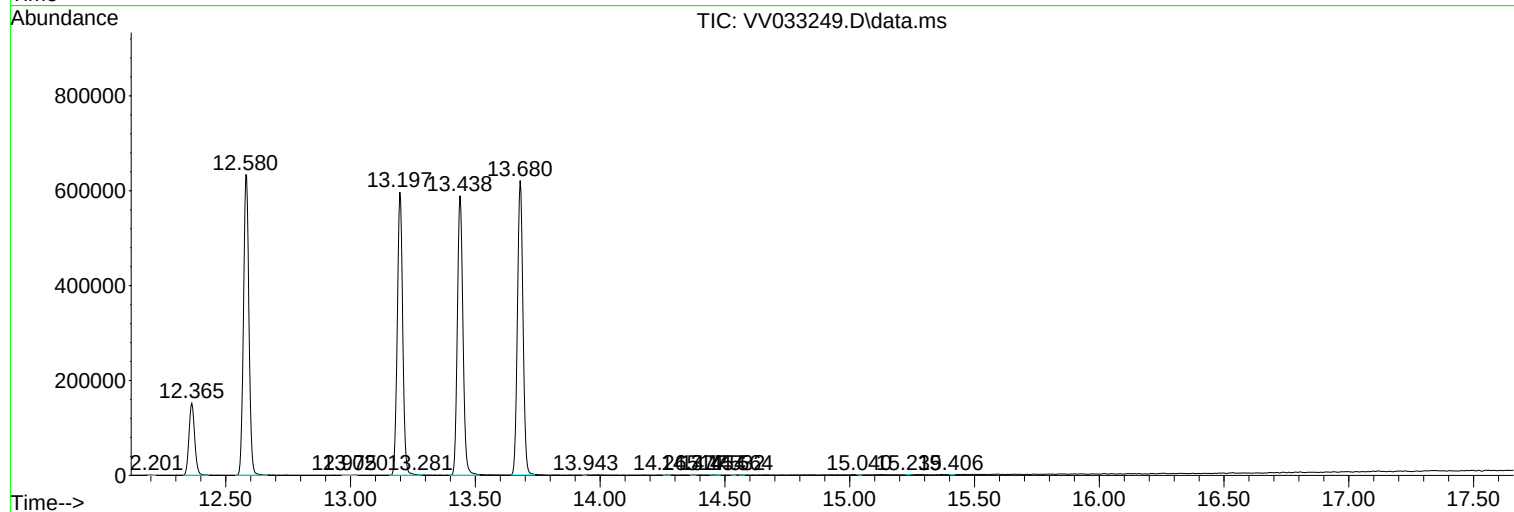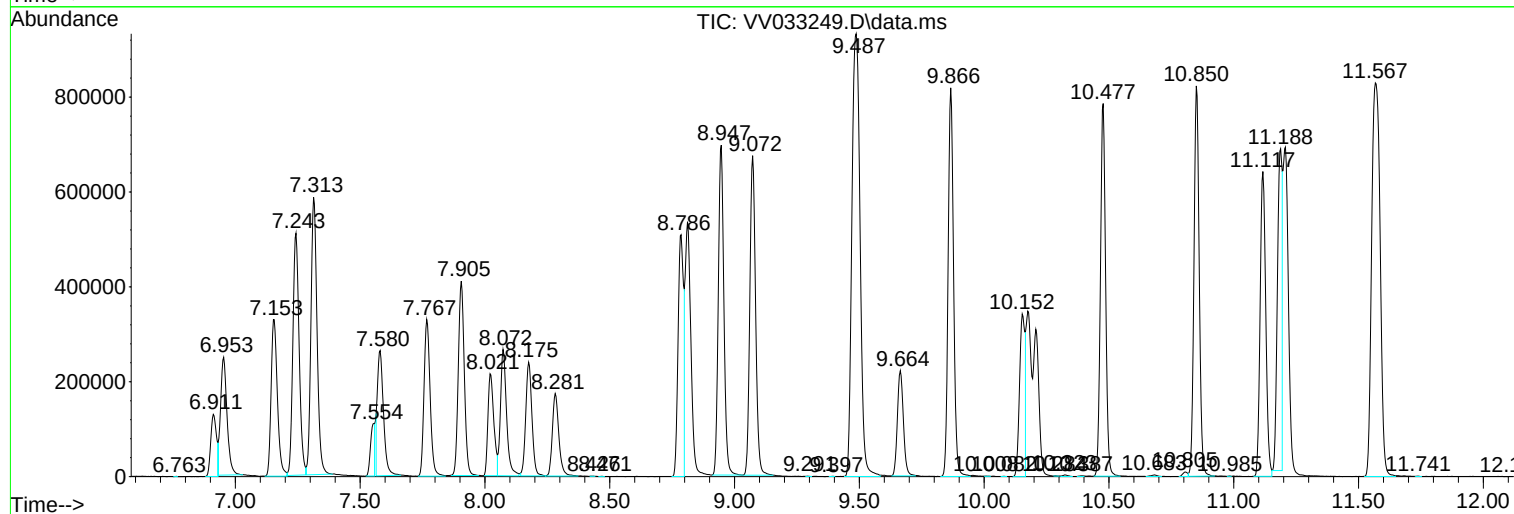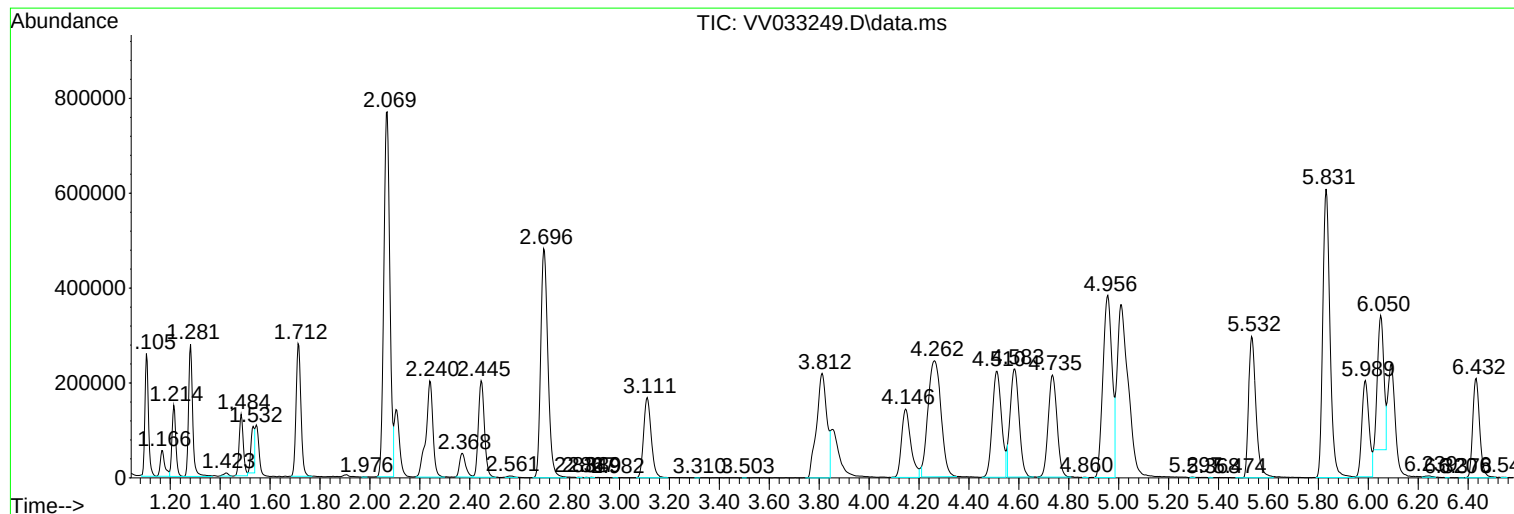

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033249.D
Acq On : 12 Dec 2023 05:39
Operator : SY/MD
Sample : 05751-13MS
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHF6MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033249.D
Acq On : 12 Dec 2023 05:39
Operator : SY/MD
Sample : 05751-13MS
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHF6MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------