

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121125\
 Data File : VV039539.D
 Acq On : 11 Dec 2025 14:08
 Operator : SY/MD
 Sample : Q3828-04
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 OWBR-06-219-120925-SIM

Quant Time: Dec 12 00:48:46 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5608	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5701	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	2982	0.500	ug/L	0.02

System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3112	0.565	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	114.000%
4) 1,2-Dichloroethane-d4	4.993	65	1748	0.468	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
7) 1,2-Dichloropropane-d6	5.996	67	2012	0.418	ug/L	-0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	=	84.000%
8) Toluene-d8	7.254	98	3786	0.467	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1504	0.555	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121125\
Data File : VV039539.D
Acq On : 11 Dec 2025 14:08
Operator : SY/MD
Sample : Q3828-04
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OWBR-06-219-120925-SIM

Quant Time: Dec 12 00:48:46 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration




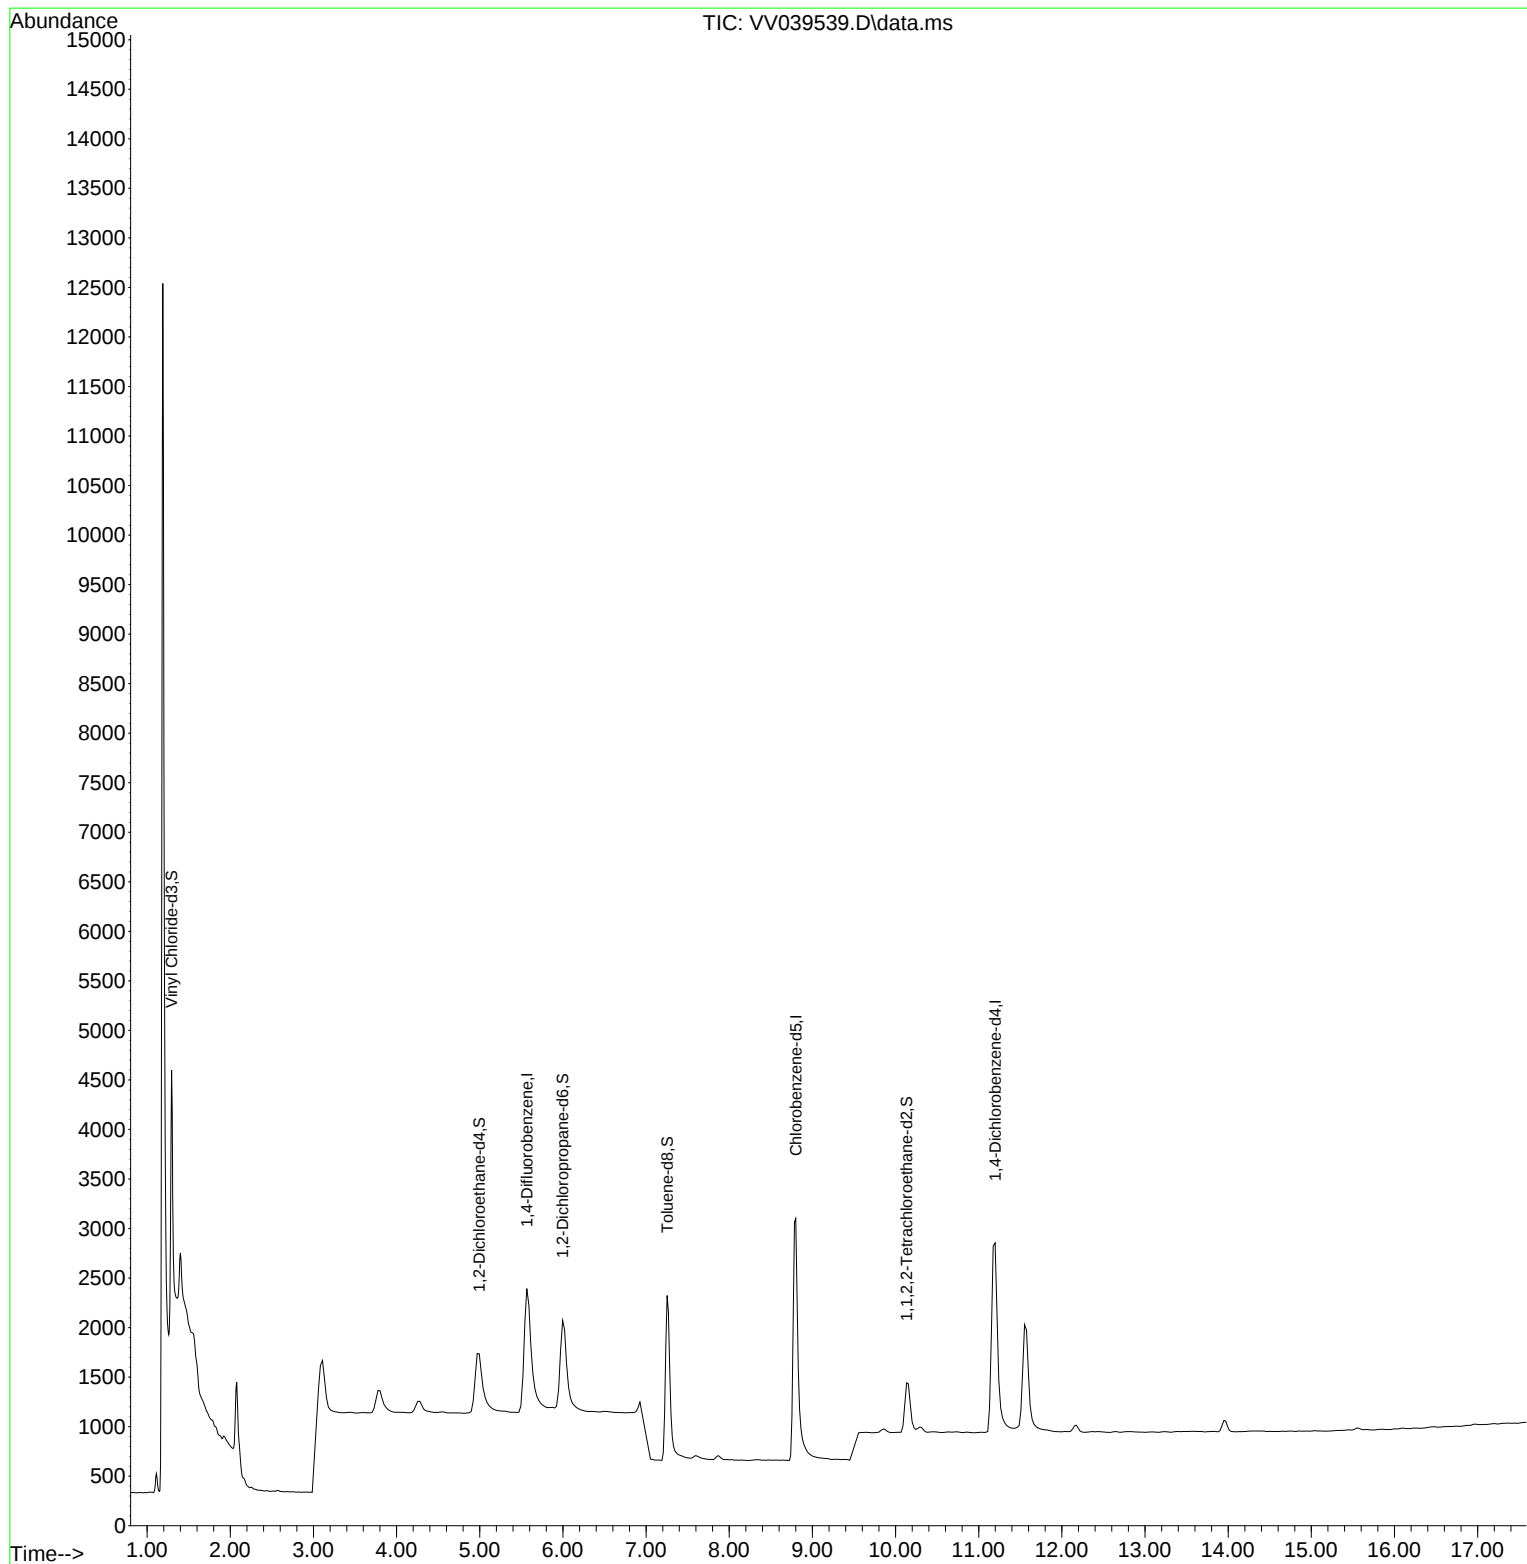


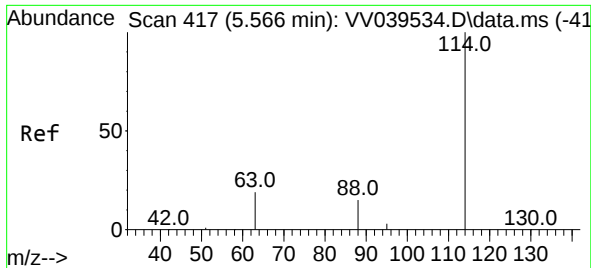

#1
1,4-Difluorobenzene
Concen: 0.500 ug/L
RT: 5.566 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV039539.D
Acq: 11 Dec 2025 14:08




Instrument :
MSVOA_V
ClientSampleId :
OWBR-06-219-120925-SIM


Tgt Ion:	114	Resp:	5608
Ion	Ratio	Lower	Upper
114	100		
63	21.0	15.0	22.4
88	16.4	12.0	18.0

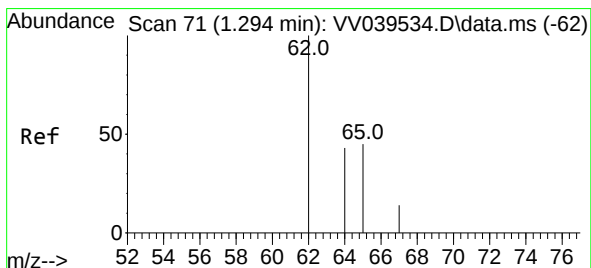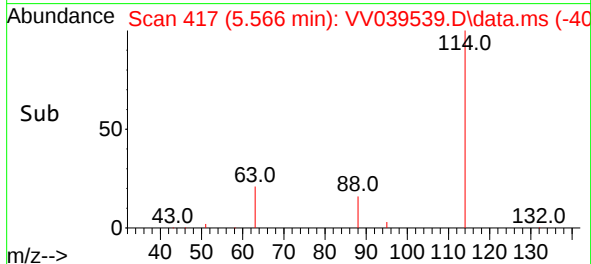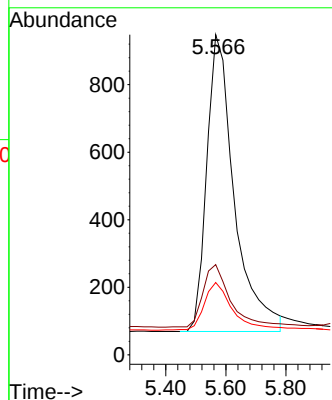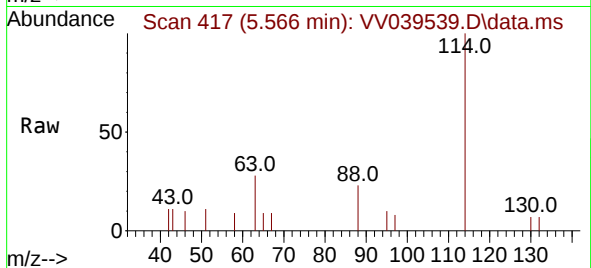

#2
Vinyl Chloride-d3
Concen: 0.565 ug/L
RT: 1.294 min Scan# 71
Delta R.T. 0.000 min
Lab File: VV039539.D
Acq: 11 Dec 2025 14:08

Tgt Ion:	65	Resp:	3112
Ion	Ratio	Lower	Upper
65	100		
67	33.1	22.3	41.5


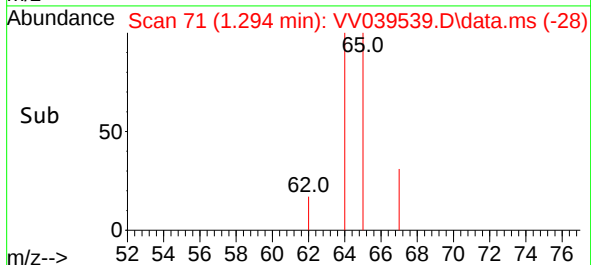
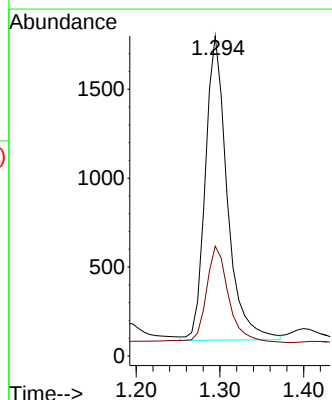
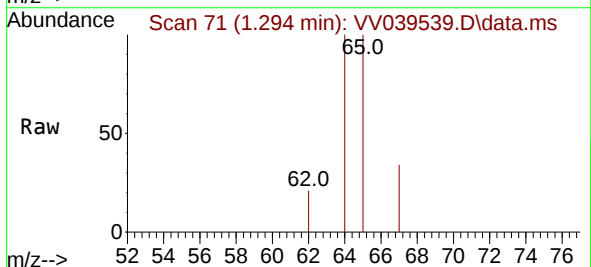


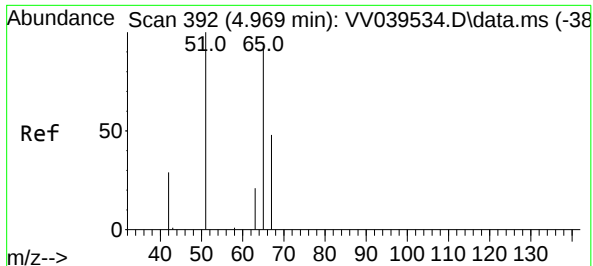

#4
1,2-Dichloroethane-d4
Concen: 0.468 ug/L
RT: 4.993 min Scan# 392
Delta R.T. 0.024 min
Lab File: VV039539.D
Acq: 11 Dec 2025 14:08




Instrument :
MSVOA_V
ClientSampleId :
OWBR-06-219-120925-SIM


Tgt Ion: 65 Resp: 1748
Ion Ratio Lower Upper
65 100
67 51.5 32.5 60.3
51 42.6 121.4 225.6#

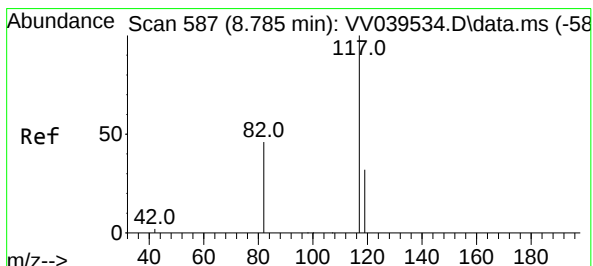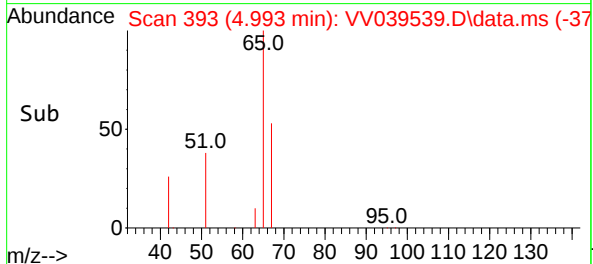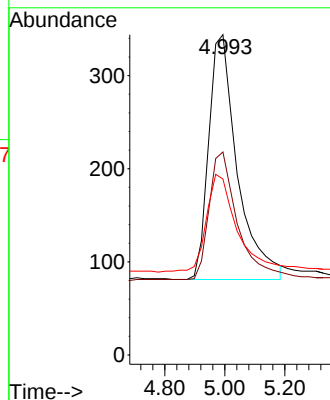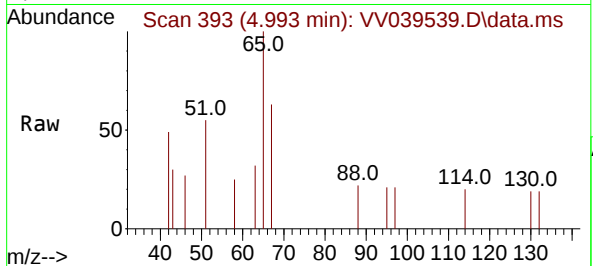

#5
Chlorobenzene-d5
Concen: 0.500 ug/L
RT: 8.800 min Scan# 588
Delta R.T. 0.015 min
Lab File: VV039539.D
Acq: 11 Dec 2025 14:08

Tgt Ion:117 Resp: 5701
Ion Ratio Lower Upper
117 100
82 47.4 39.4 59.2
119 32.8 26.2 39.2


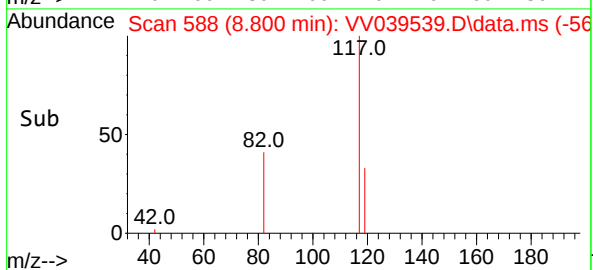
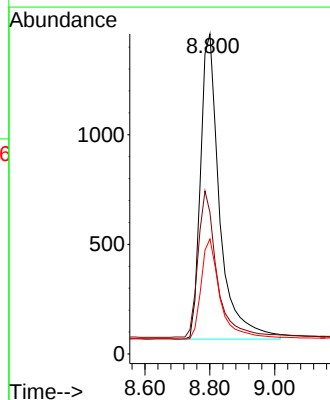
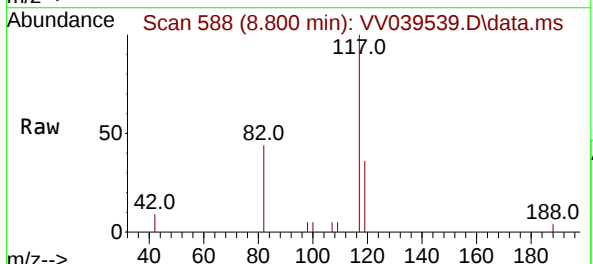


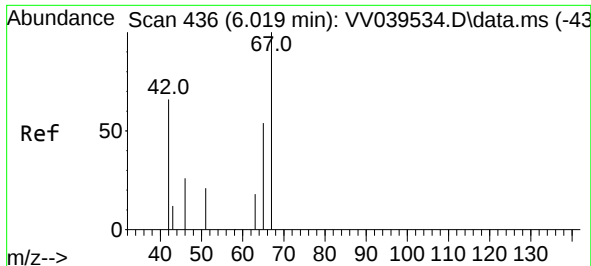

#7
1,2-Dichloropropane-d6
Concen: 0.418 ug/L
RT: 5.996 min Scan# 41
Delta R.T. -0.023 min
Lab File: VV039539.D
Acq: 11 Dec 2025 14:08




Instrument :
MSVOA_V
ClientSampleId :
OWBR-06-219-120925-SIM


Tgt Ion:	67	Resp:	2012
Ion	Ratio	Lower	Upper
67	100		
65	63.6	37.9	56.9#
46	43.1	27.4	41.0#
42	30.2	51.2	76.8#

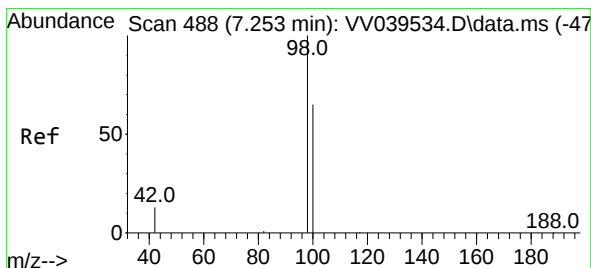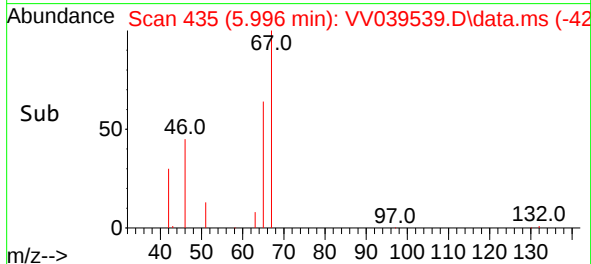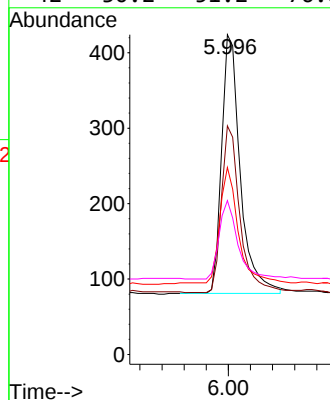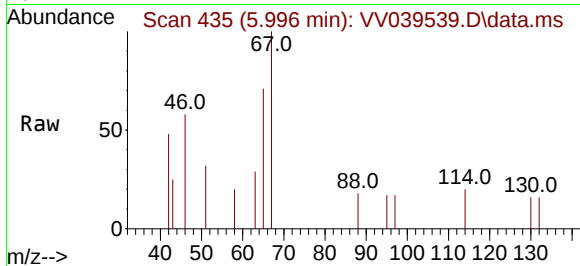

#8
Toluene-d8
Concen: 0.467 ug/L
RT: 7.254 min Scan# 488
Delta R.T. 0.016 min
Lab File: VV039539.D
Acq: 11 Dec 2025 14:08

Tgt Ion:	98	Resp:	3786
Ion	Ratio	Lower	Upper
98	100		
100	62.2	44.5	82.7
42	10.9	10.1	18.7


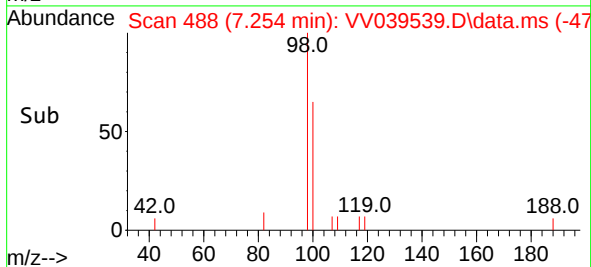
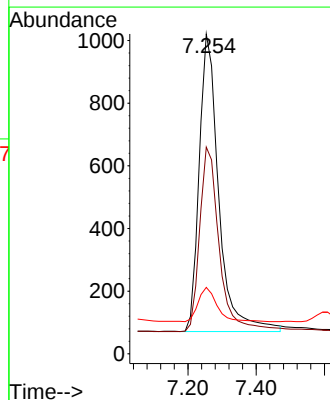
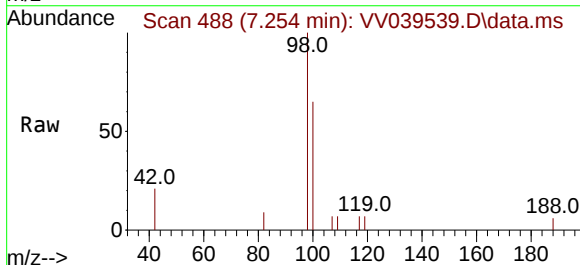


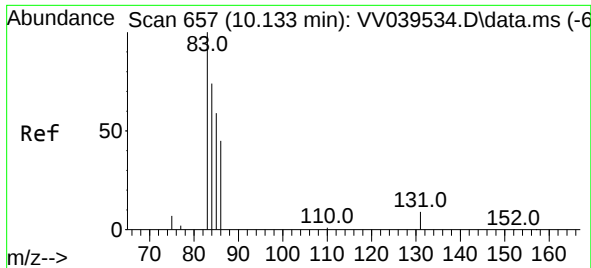

#10
1,1,2,2-Tetrachloroethane-d2
Concen: 0.555 ug/L
RT: 10.133 min Scan# 610
Delta R.T. -0.000 min
Lab File: VV039539.D
Acq: 11 Dec 2025 14:08

Instrument :
MSVOA_V
ClientSampleId :
OWBR-06-219-120925-SIM

Tgt Ion: 84 Resp: 1504
Ion Ratio Lower Upper
84 100
86 61.2 44.4 82.5

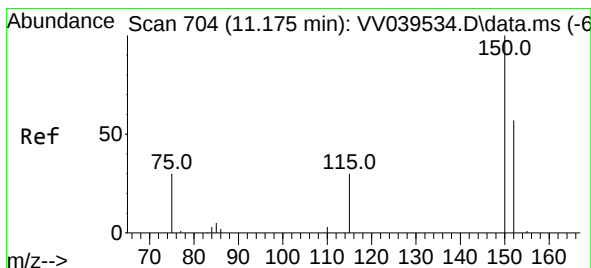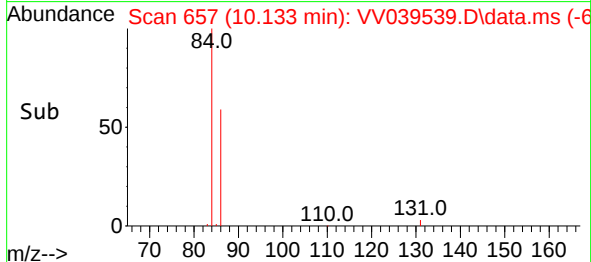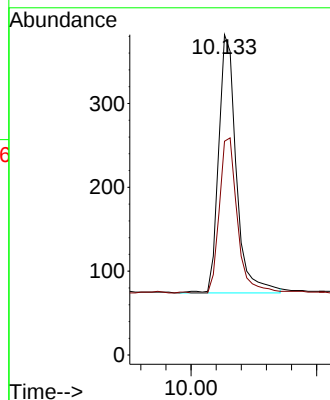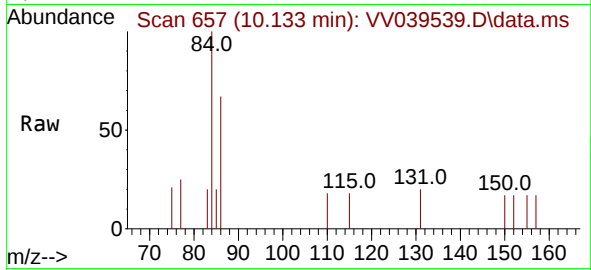

#12
1,4-Dichlorobenzene-d4
Concen: 0.500 ug/L
RT: 11.197 min Scan# 705
Delta R.T. 0.022 min
Lab File: VV039539.D
Acq: 11 Dec 2025 14:08

Tgt Ion: 152 Resp: 2982
Ion Ratio Lower Upper
152 100
115 54.5 0.0 101.6
150 160.6 0.0 396.2

