
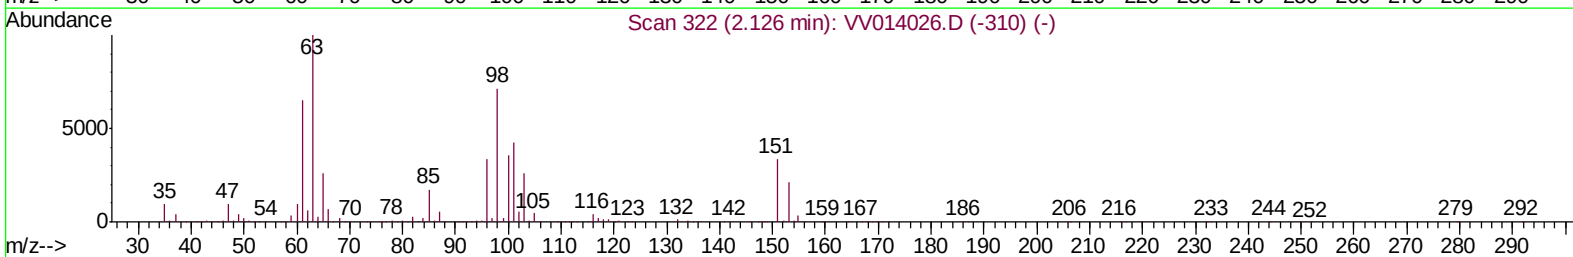
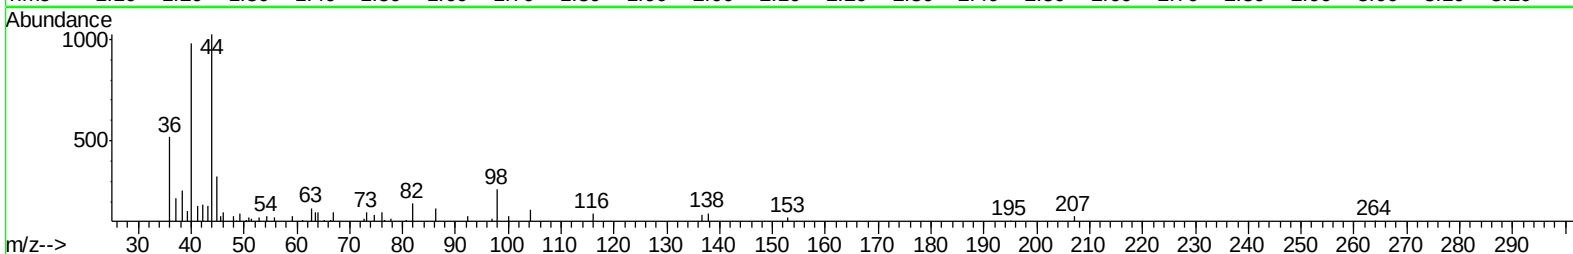


Data File : VV014041.D
Acq On : 12 Dec 2019 19:05
Operator : SY/MD
Sample : K6276-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Dec 13 06:18:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:14:07 2019
Response via : Initial Calibration

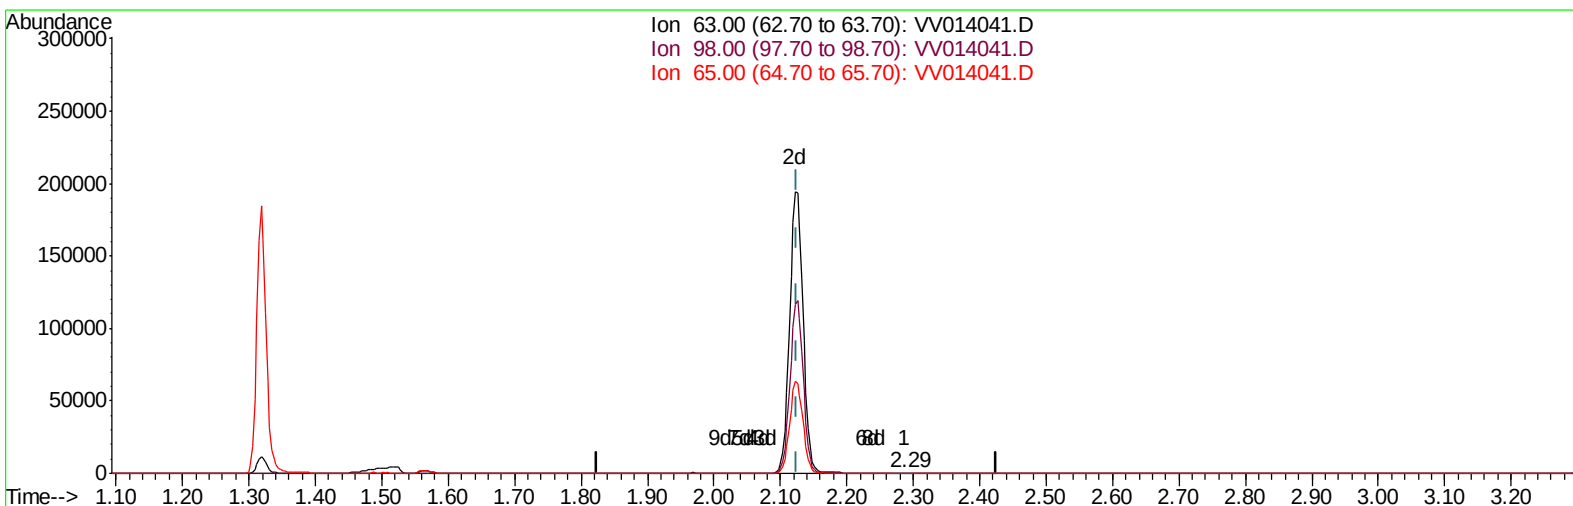

TIC: VV014041.D

(11) 1,1-Dichloroethene-d2 (S)

2.286min (+0.161) 0.02ug/L

response 176

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	98.86
65.00	23.60	23.86
0.00	0.00	0.00