
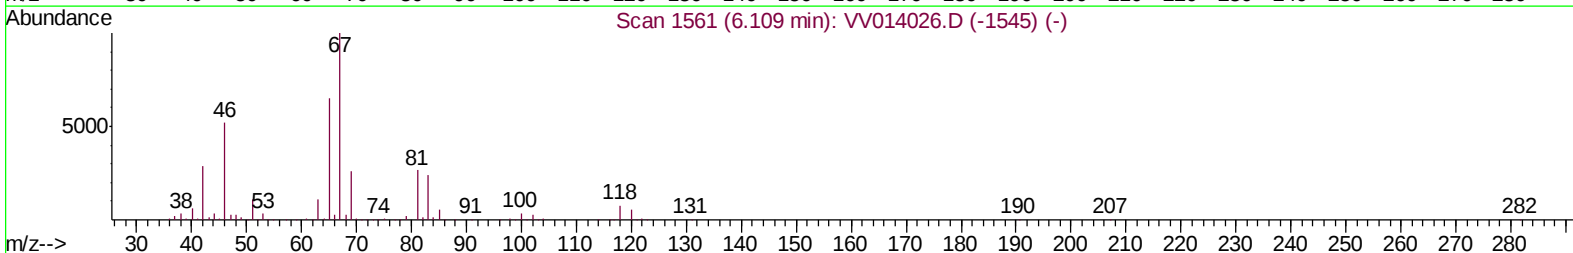
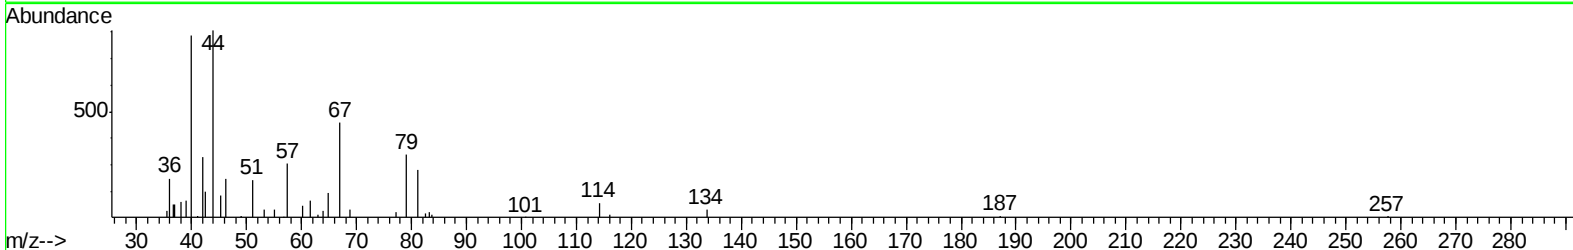


Data File : VV014043.D
Acq On : 12 Dec 2019 19:54
Operator : SY/MD
Sample : K6276-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 13 06:18:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:14:07 2019
Response via : Initial Calibration

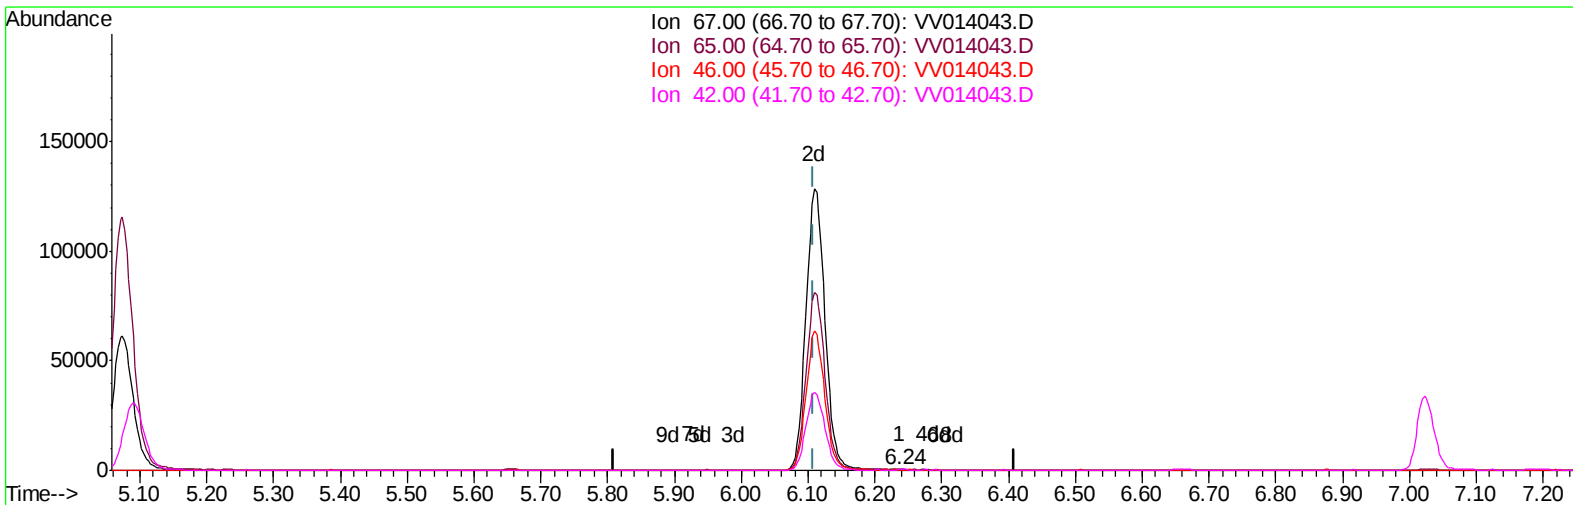

TIC: VV014043.D

(36) 1,2-Dichloropropane-d6 (S)

6.238min (+0.129) 0.06ug/L

response 289

Ion	Exp%	Act%
67.00	100	100
65.00	64.70	81.31
46.00	49.60	48.44
42.00	28.10	19.72