

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014029.D
 Acq On : 12 Dec 2019 11:21
 Operator : SY/MD
 Sample : K6200-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF43

Quant Time: Dec 13 06:30:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:14:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	697022	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	676539	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	269629	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	202226	50.16	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.32%
7) Chloroethane-d5	1.56	69	196690	46.74	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.48%
11) 1,1-Dichloroethene-d2	2.12	63	291717	32.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.44%
21) 2-Butanone-d5	3.92	46	254813	89.80	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.80%
24) Chloroform-d	4.39	84	411177	48.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.14%
26) 1,2-Dichloroethane-d4	5.07	65	263906	49.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.38%
32) Benzene-d6	5.09	84	838244	47.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.64%
36) 1,2-Dichloropropane-d6	6.11	67	268446	51.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.02%
41) Toluene-d8	7.35	98	721011	45.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.22%
43) trans-1,3-Dichloropropene-	7.66	79	109607	42.80	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.60%
47) 2-Hexanone-d5	8.13	63	132621	67.49	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.49%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	319578	41.94	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.88%
64) 1,2-Dichlorobenzene-d4	11.67	152	280223	52.92	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.84%


Target Compounds					Ovalue
13) Acetone	2.18	43	9009	2.167 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
Data File : VV014029.D
Acq On : 12 Dec 2019 11:21
Operator : SY/MD
Sample : K6200-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF43

Quant Time: Dec 13 06:30:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:14:07 2019
Response via : Initial Calibration

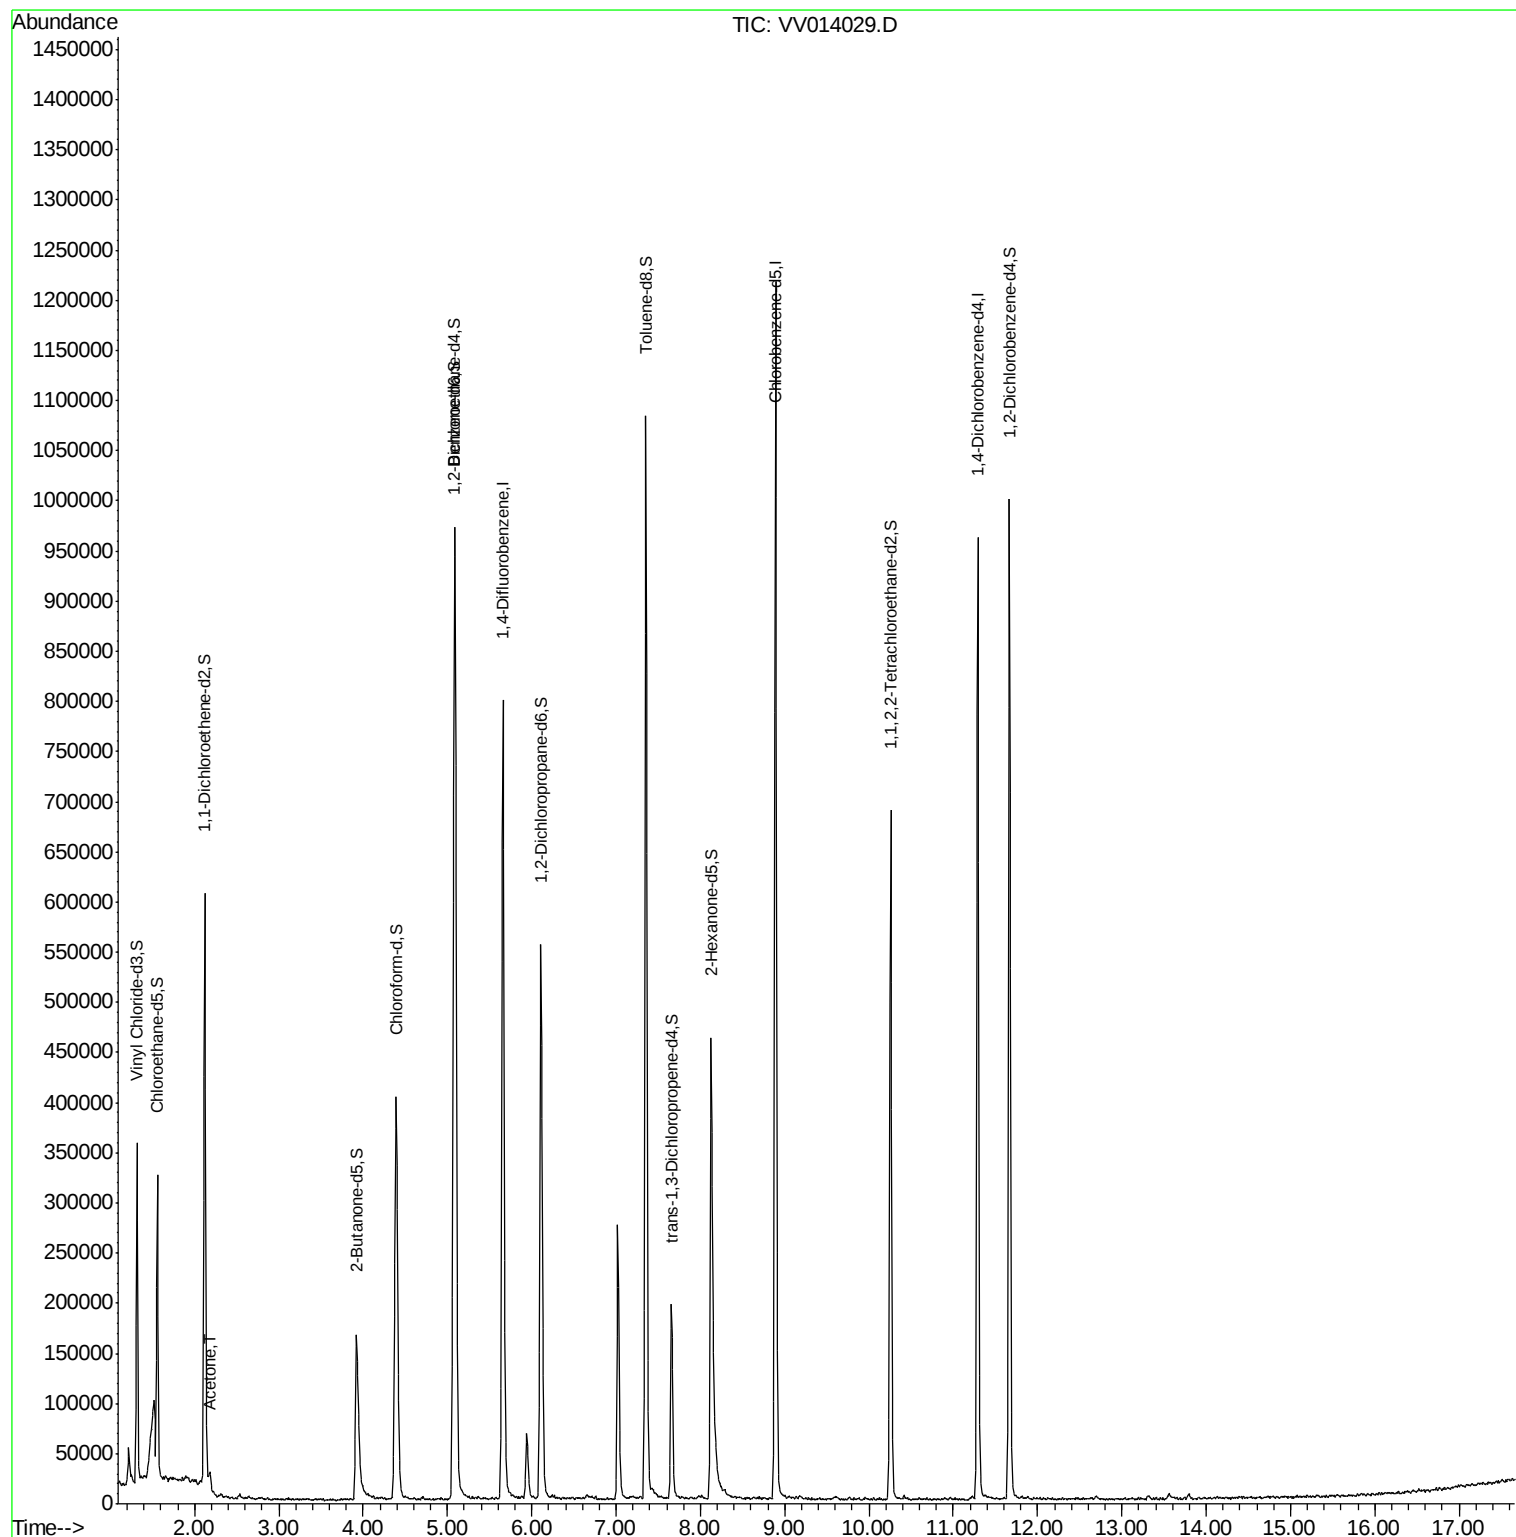

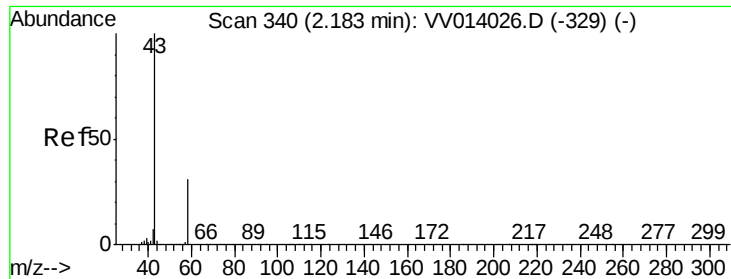

#13
 Acetone
 Concen: 2.167 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. 0.00 min
 Lab File: VV014029.D
 Acq: 12 Dec 2019 11:21

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF43

Tot Ion: 43 Resp: 9009
 Ion Ratio Lower Upper
 43 100
 58 36.3 0.0 60.8

