

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014036.D
 Acq On : 12 Dec 2019 17:02
 Operator : SY/MD
 Sample : K6280-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF29

Quant Time: Dec 13 07:30:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:14:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	648760	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	629839	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	244290	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	184900	49.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.56%
7) Chloroethane-d5	1.56	69	182800	46.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.34%
11) 1,1-Dichloroethene-d2	2.12	63	271898	32.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.54%
21) 2-Butanone-d5	3.92	46	263793	99.88	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.88%
24) Chloroform-d	4.39	84	392234	49.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.56%
26) 1,2-Dichloroethane-d4	5.07	65	253847	50.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.68%
32) Benzene-d6	5.09	84	804812	49.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.62%
36) 1,2-Dichloropropane-d6	6.11	67	258248	52.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.42%
41) Toluene-d8	7.35	98	693360	46.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.20%
43) trans-1,3-Dichloropropene-	7.66	79	103102	43.25	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.50%
47) 2-Hexanone-d5	8.13	63	145439	79.51	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.51%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	312237	44.02	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.04%
64) 1,2-Dichlorobenzene-d4	11.67	152	267109	55.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.34%


Target Compounds				Ovalue
13) Acetone	2.19	43	7070	1.827 ug/L 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
Data File : VV014036.D
Acq On : 12 Dec 2019 17:02
Operator : SY/MD
Sample : K6280-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF29

Quant Time: Dec 13 07:30:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:14:07 2019
Response via : Initial Calibration

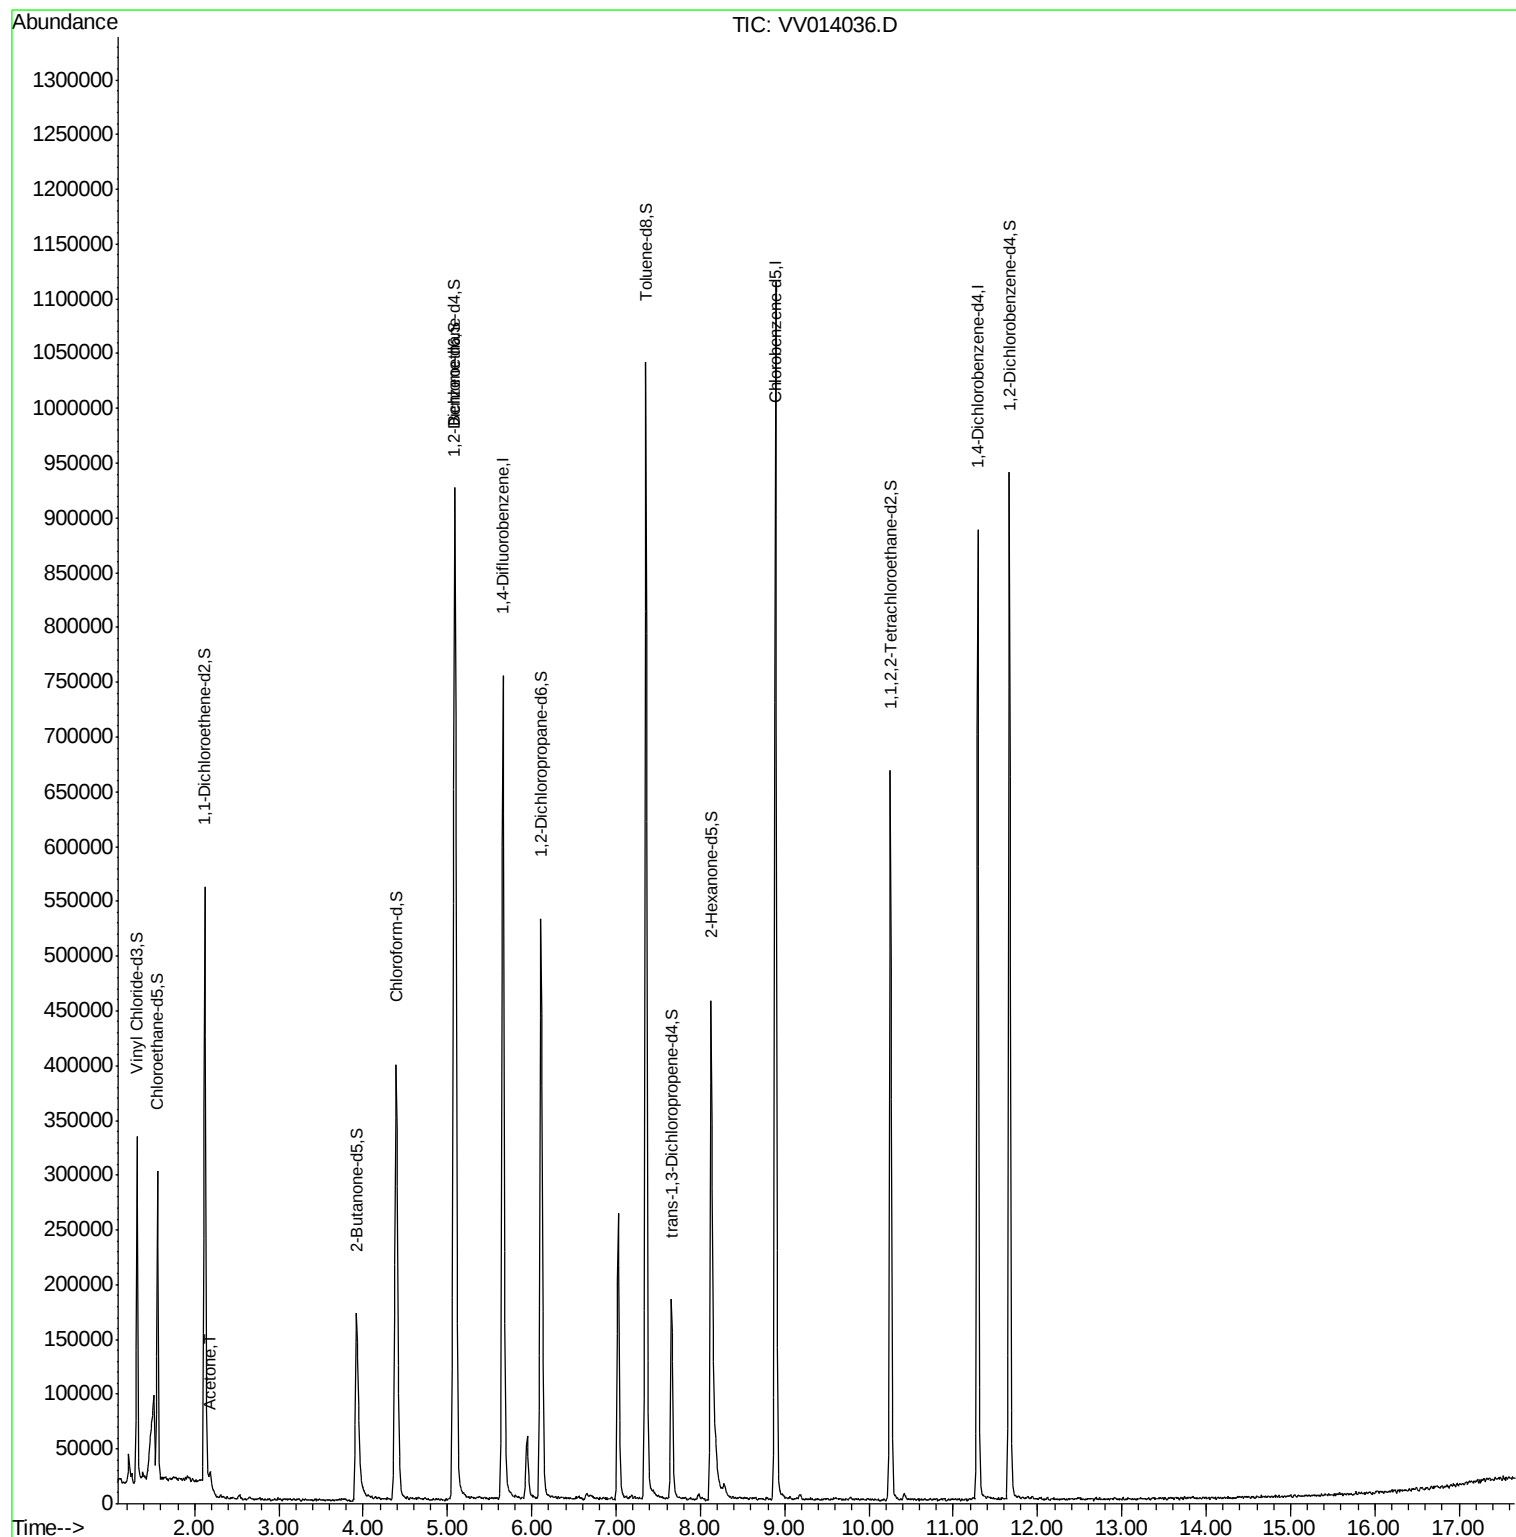

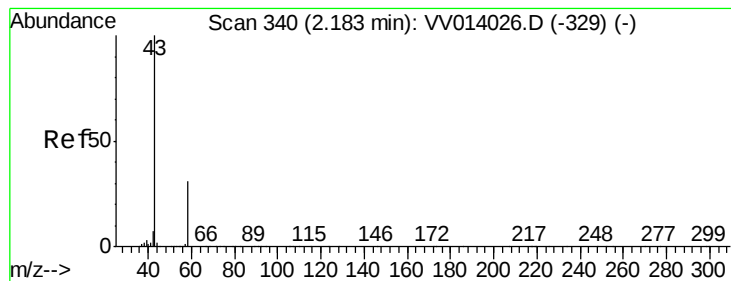

#13
 Acetone
 Concen: 1.827 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. 0.00 min
 Lab File: VV014036.D
 Acq: 12 Dec 2019 17:02

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF29

Tot Ion: 43 Resp: 7070
 Ion Ratio Lower Upper
 43 100
 58 41.0 0.0 60.8

