

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014038.D
 Acq On : 12 Dec 2019 17:51
 Operator : SY/MD
 Sample : K6276-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C49

Quant Time: Dec 13 07:35:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:14:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	652040	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	617352	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	233078	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	178918	47.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.88%
7) Chloroethane-d5	1.56	69	179203	45.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.06%
11) 1,1-Dichloroethene-d2	2.12	63	271277	32.53	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.06%
21) 2-Butanone-d5	3.92	46	267941	100.94	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.94%
24) Chloroform-d	4.39	84	379702	47.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.90%
26) 1,2-Dichloroethane-d4	5.07	65	243825	48.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.18%
32) Benzene-d6	5.09	84	775517	48.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.96%
36) 1,2-Dichloropropane-d6	6.11	67	252930	52.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.34%
41) Toluene-d8	7.35	98	675964	46.35	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.70%
43) trans-1,3-Dichloropropene-	7.66	79	105983	45.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.72%
47) 2-Hexanone-d5	8.13	63	161333	89.98	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.98%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	315153	45.33	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.66%
64) 1,2-Dichlorobenzene-d4	11.67	152	253758	55.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.86%


Target Compounds					Ovalue
13) Acetone	2.19	43	7063	1.816 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121219\
Data File : VV014038.D
Acq On : 12 Dec 2019 17:51
Operator : SY/MD
Sample : K6276-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C49

Quant Time: Dec 13 07:35:04 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:14:07 2019
Response via : Initial Calibration

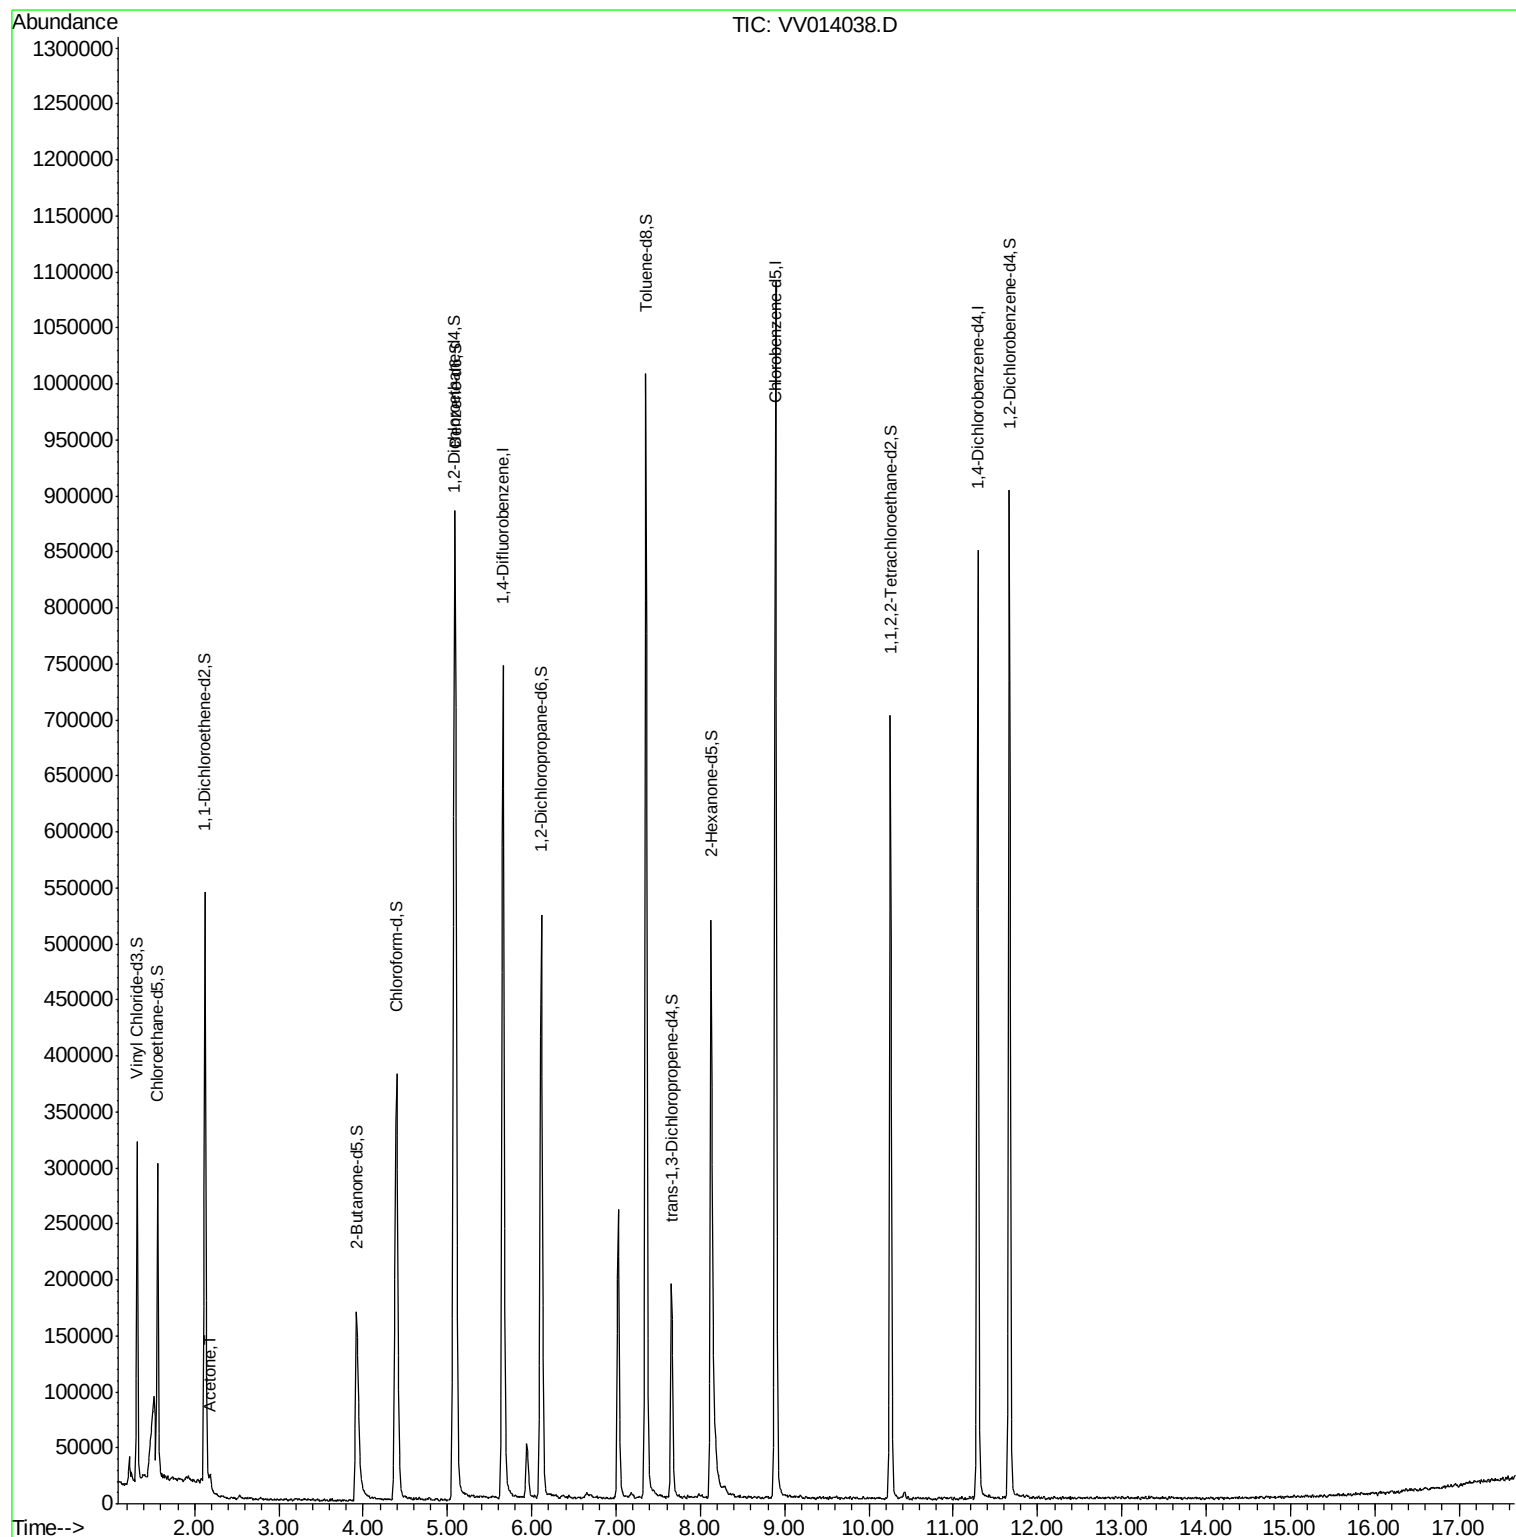

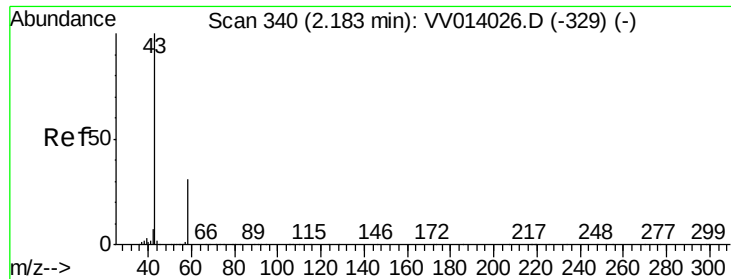

#13
 Acetone
 Concen: 1.816 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. 0.00 min
 Lab File: VV014038.D
 Acq: 12 Dec 2019 17:51

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C49

Tot Ion: 43 Resp: 7063
 Ion Ratio Lower Upper
 43 100
 58 39.9 0.0 60.8

