

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014039.D
 Acq On : 12 Dec 2019 18:16
 Operator : SY/MD
 Sample : K6276-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C51

Quant Time: Dec 13 07:37:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 13 06:14:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	625590	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	605199	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	246412	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	174024	48.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.20%
7) Chloroethane-d5	1.56	69	175127	46.37	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.74%
11) 1,1-Dichloroethene-d2	2.12	63	259009	32.37	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.74%
21) 2-Butanone-d5	3.92	46	265803	104.37	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.37%
24) Chloroform-d	4.39	84	379291	49.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.84%
26) 1,2-Dichloroethane-d4	5.07	65	241366	50.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.26%
32) Benzene-d6	5.09	84	765168	48.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.58%
36) 1,2-Dichloropropane-d6	6.11	67	247711	52.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.24%
41) Toluene-d8	7.35	98	676144	47.29	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.58%
43) trans-1,3-Dichloropropene-	7.66	79	103728	45.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.56%
47) 2-Hexanone-d5	8.13	63	152840	86.95	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.95%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	310536	45.56	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.12%
64) 1,2-Dichlorobenzene-d4	11.67	152	266090	54.98	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.96%


Target Compounds					Ovalue
13) Acetone	2.19	43	8459	2.267 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121219\
Data File : VV014039.D
Acq On : 12 Dec 2019 18:16
Operator : SY/MD
Sample : K6276-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C51

Quant Time: Dec 13 07:37:22 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 13 06:14:07 2019
Response via : Initial Calibration

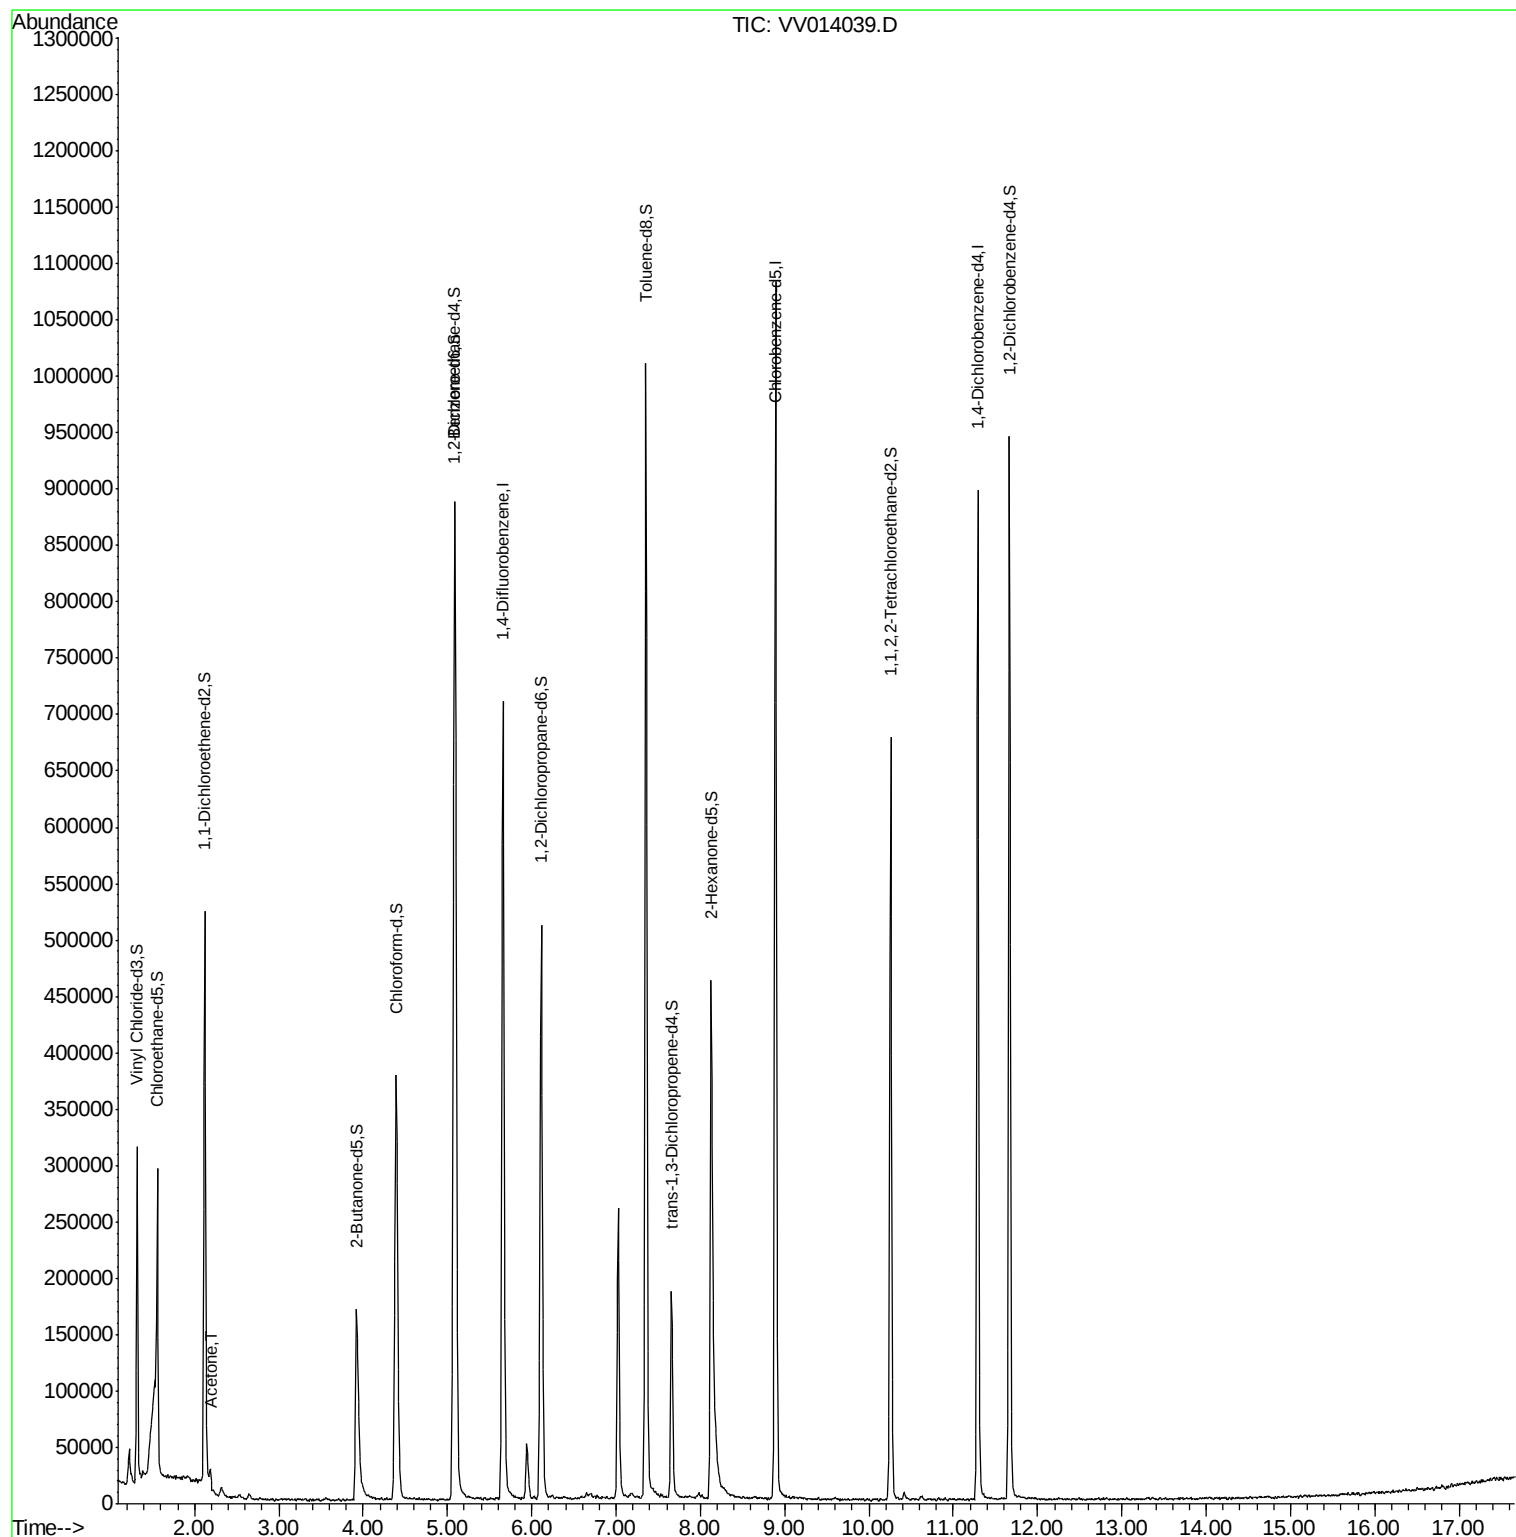

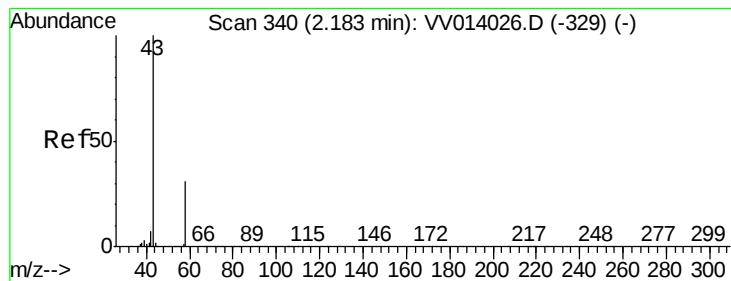

#13

Acetone

Concen: 2.267 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.00 min

Lab File: VV014039.D

Acq: 12 Dec 2019 18:16

Instrument :
MSVOA_V
ClientSampleId :
C0C51

Tot Ion: 43 Resp: 8459

Ion Ratio Lower Upper

43 100

58 34.8 0.0 60.8

