

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014032.D
 Acq On : 12 Dec 2019 15:24
 Operator : SY/MD
 Sample : K6276-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	66	71	85	rVB	325335	331155	13.09%	1.758%
2	1.576	144	151	159	rVB	324805	363554	14.38%	1.930%
3	2.126	314	322	336	rVB	622963	872178	34.49%	4.631%
4	2.727	507	509	513	rBV4	1921	1262	0.05%	0.007%
5	2.910	563	566	571	rBV8	2369	2003	0.08%	0.011%
6	2.958	579	581	583	rVB3	1939	822	0.03%	0.004%
7	3.151	637	641	643	rBV4	1422	1271	0.05%	0.007%
8	3.254	671	673	678	rVB4	1565	935	0.04%	0.005%
9	3.277	678	680	684	rVB5	1887	1138	0.04%	0.006%
10	3.302	684	688	693	rBV8	2115	1821	0.07%	0.010%
11	3.328	693	696	702	rBV6	2370	1993	0.08%	0.011%
12	3.389	713	715	716	rBV2	1058	565	0.02%	0.003%
13	3.479	741	743	745	rBV3	1018	353	0.01%	0.002%
14	3.528	755	758	761	rVB5	970	486	0.02%	0.003%
15	3.560	764	768	770	rVB4	1184	772	0.03%	0.004%
16	3.576	770	773	776	rBV4	1354	1107	0.04%	0.006%
17	3.640	791	793	795	rBV3	1179	592	0.02%	0.003%
18	3.698	810	811	814	rBV3	879	383	0.02%	0.002%
19	3.730	817	821	822	rBV3	989	571	0.02%	0.003%
20	3.765	830	832	837	rVB6	1408	920	0.04%	0.005%
21	3.788	837	839	842	rBV2	1036	455	0.02%	0.002%
22	3.801	842	843	847	rVB4	1536	598	0.02%	0.003%
23	3.820	847	849	853	rBV5	1989	1349	0.05%	0.007%
24	3.920	869	880	906	rBV	165192	443482	17.54%	2.355%
25	4.389	1012	1026	1051	rBV	424945	1013706	40.08%	5.382%
26	4.595	1088	1090	1092	rBV3	1645	787	0.03%	0.004%
27	4.801	1151	1154	1158	rVB4	1900	1169	0.05%	0.006%
28	4.868	1172	1175	1176	rBV2	1618	878	0.03%	0.005%
29	4.958	1201	1203	1204	rBV	1096	432	0.02%	0.002%
30	4.974	1205	1208	1210	rVV3	1806	1304	0.05%	0.007%
31	5.087	1225	1243	1269	rBV2	1000115	2528974	100.00%	13.427%
32	5.421	1344	1347	1349	rBV3	2154	1604	0.06%	0.009%
33	5.656	1403	1420	1447	rBV	918935	1833829	72.51%	9.736%
34	6.109	1548	1561	1591	rBV	561035	1139428	45.05%	6.049%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014032.D
 Acq On : 12 Dec 2019 15:24
 Operator : SY/MD
 Sample : K6276-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.325	1626	1628	1633	rBV5	2180	2236	0.09%	0.012%
36	6.550	1695	1698	1701	rBV4	1673	1317	0.05%	0.007%
37	7.023	1833	1845	1866	rBV	282688	510689	20.19%	2.711%
38	7.254	1915	1917	1919	rBV3	2133	1078	0.04%	0.006%
39	7.354	1934	1948	1968	rBV	1120592	1944388	76.88%	10.323%
40	7.656	2033	2042	2064	rBV	199820	340178	13.45%	1.806%
41	8.125	2178	2188	2224	rBV3	440597	967859	38.27%	5.139%
42	8.640	2345	2348	2349	rBV3	1669	1081	0.04%	0.006%
43	8.804	2397	2399	2403	rBV5	1291	1015	0.04%	0.005%
44	8.887	2412	2425	2450	rBV	1339202	2179625	86.19%	11.572%
45	9.302	2551	2554	2556	rBV3	1050	680	0.03%	0.004%
46	9.334	2562	2564	2569	rBV6	1638	1071	0.04%	0.006%
47	9.537	2624	2627	2628	rBV3	809	521	0.02%	0.003%
48	9.576	2635	2639	2641	rBV4	2515	1975	0.08%	0.010%
49	9.756	2691	2695	2697	rBV3	1195	787	0.03%	0.004%
50	9.791	2702	2706	2708	rVV5	949	555	0.02%	0.003%
51	9.884	2733	2735	2736	rBV	916	391	0.02%	0.002%
52	9.942	2750	2753	2756	rVB3	1248	599	0.02%	0.003%
53	10.006	2771	2773	2775	rBV3	1007	421	0.02%	0.002%
54	10.042	2781	2784	2787	rBV4	1631	1324	0.05%	0.007%
55	10.071	2791	2793	2794	rBV2	946	397	0.02%	0.002%
56	10.109	2803	2805	2807	rBV3	1059	611	0.02%	0.003%
57	10.170	2821	2824	2825	rBV2	1546	819	0.03%	0.004%
58	10.254	2838	2850	2868	rBV	663349	1020913	40.37%	5.420%
59	10.563	2942	2946	2949	rBV4	1832	1601	0.06%	0.008%
60	10.630	2965	2967	2970	rVB4	1678	730	0.03%	0.004%
61	10.669	2977	2979	2983	rVB4	1460	865	0.03%	0.005%
62	10.691	2984	2986	2988	rBV3	954	544	0.02%	0.003%
63	10.723	2993	2996	3001	rVB5	2188	1487	0.06%	0.008%
64	10.752	3001	3005	3008	rBV5	1640	1219	0.05%	0.006%
65	10.778	3010	3013	3016	rBV4	1028	718	0.03%	0.004%
66	10.817	3022	3025	3027	rBV4	1283	811	0.03%	0.004%
67	10.900	3049	3051	3053	rBV2	1144	579	0.02%	0.003%
68	11.010	3081	3085	3088	rBV3	1799	1612	0.06%	0.009%
69	11.026	3088	3090	3095	rVB4	1736	1361	0.05%	0.007%
70	11.055	3096	3099	3101	rBV3	1018	519	0.02%	0.003%
71	11.096	3108	3112	3114	rBV4	810	630	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014032.D
 Acq On : 12 Dec 2019 15:24
 Operator : SY/MD
 Sample : K6276-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.206	3140	3146	3147	rBV4	2253	1679	0.07%	0.009%
73	11.289	3159	3172	3192	rBV	1105682	1699210	67.19%	9.021%
74	11.527	3244	3246	3248	rBV3	1115	482	0.02%	0.003%
75	11.665	3276	3289	3305	rBV	986886	1561870	61.76%	8.292%
76	11.855	3346	3348	3352	rBV5	1753	906	0.04%	0.005%
77	12.000	3391	3393	3396	rBV3	1113	870	0.03%	0.005%
78	12.241	3465	3468	3470	rBV4	1063	620	0.02%	0.003%
79	12.267	3474	3476	3477	rBV2	1236	400	0.02%	0.002%
80	12.444	3529	3531	3534	rBV4	1729	1037	0.04%	0.006%
81	12.485	3542	3544	3545	rBV2	1527	759	0.03%	0.004%
82	12.563	3565	3568	3573	rBV7	1542	1575	0.06%	0.008%
83	12.585	3573	3575	3579	rVB4	2445	1431	0.06%	0.008%
84	12.608	3579	3582	3584	rBV2	1328	847	0.03%	0.004%
85	12.620	3584	3586	3587	rBV	1193	471	0.02%	0.003%
86	12.656	3595	3597	3603	rVB7	2279	1490	0.06%	0.008%
87	12.685	3603	3606	3607	rBV3	1952	971	0.04%	0.005%
88	12.775	3631	3634	3636	rBV4	1736	1082	0.04%	0.006%
89	12.981	3694	3698	3700	rBV3	1083	939	0.04%	0.005%
90	13.071	3723	3726	3728	rBV3	1883	1362	0.05%	0.007%
91	13.167	3754	3756	3757	rBV	993	362	0.01%	0.002%
92	13.318	3795	3803	3807	rBV10	2705	4163	0.16%	0.022%
93	13.778	3943	3946	3947	rBV3	2197	1063	0.04%	0.006%
94	13.791	3947	3950	3952	rBV4	2250	1484	0.06%	0.008%
95	14.019	4018	4021	4024	rBV5	1599	1389	0.05%	0.007%
96	14.215	4080	4082	4084	rVB2	1543	623	0.02%	0.003%
97	14.228	4084	4086	4089	rBV3	1014	701	0.03%	0.004%
98	14.363	4124	4128	4130	rBV4	938	770	0.03%	0.004%
99	14.399	4137	4139	4142	rBV3	1835	794	0.03%	0.004%
100	14.681	4225	4227	4229	rBV2	2102	925	0.04%	0.005%


Sum of corrected areas: 18835357

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121219\
Data File : VV014032.D
Acq On : 12 Dec 2019 15:24
Operator : SY/MD
Sample : K6276-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C47

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

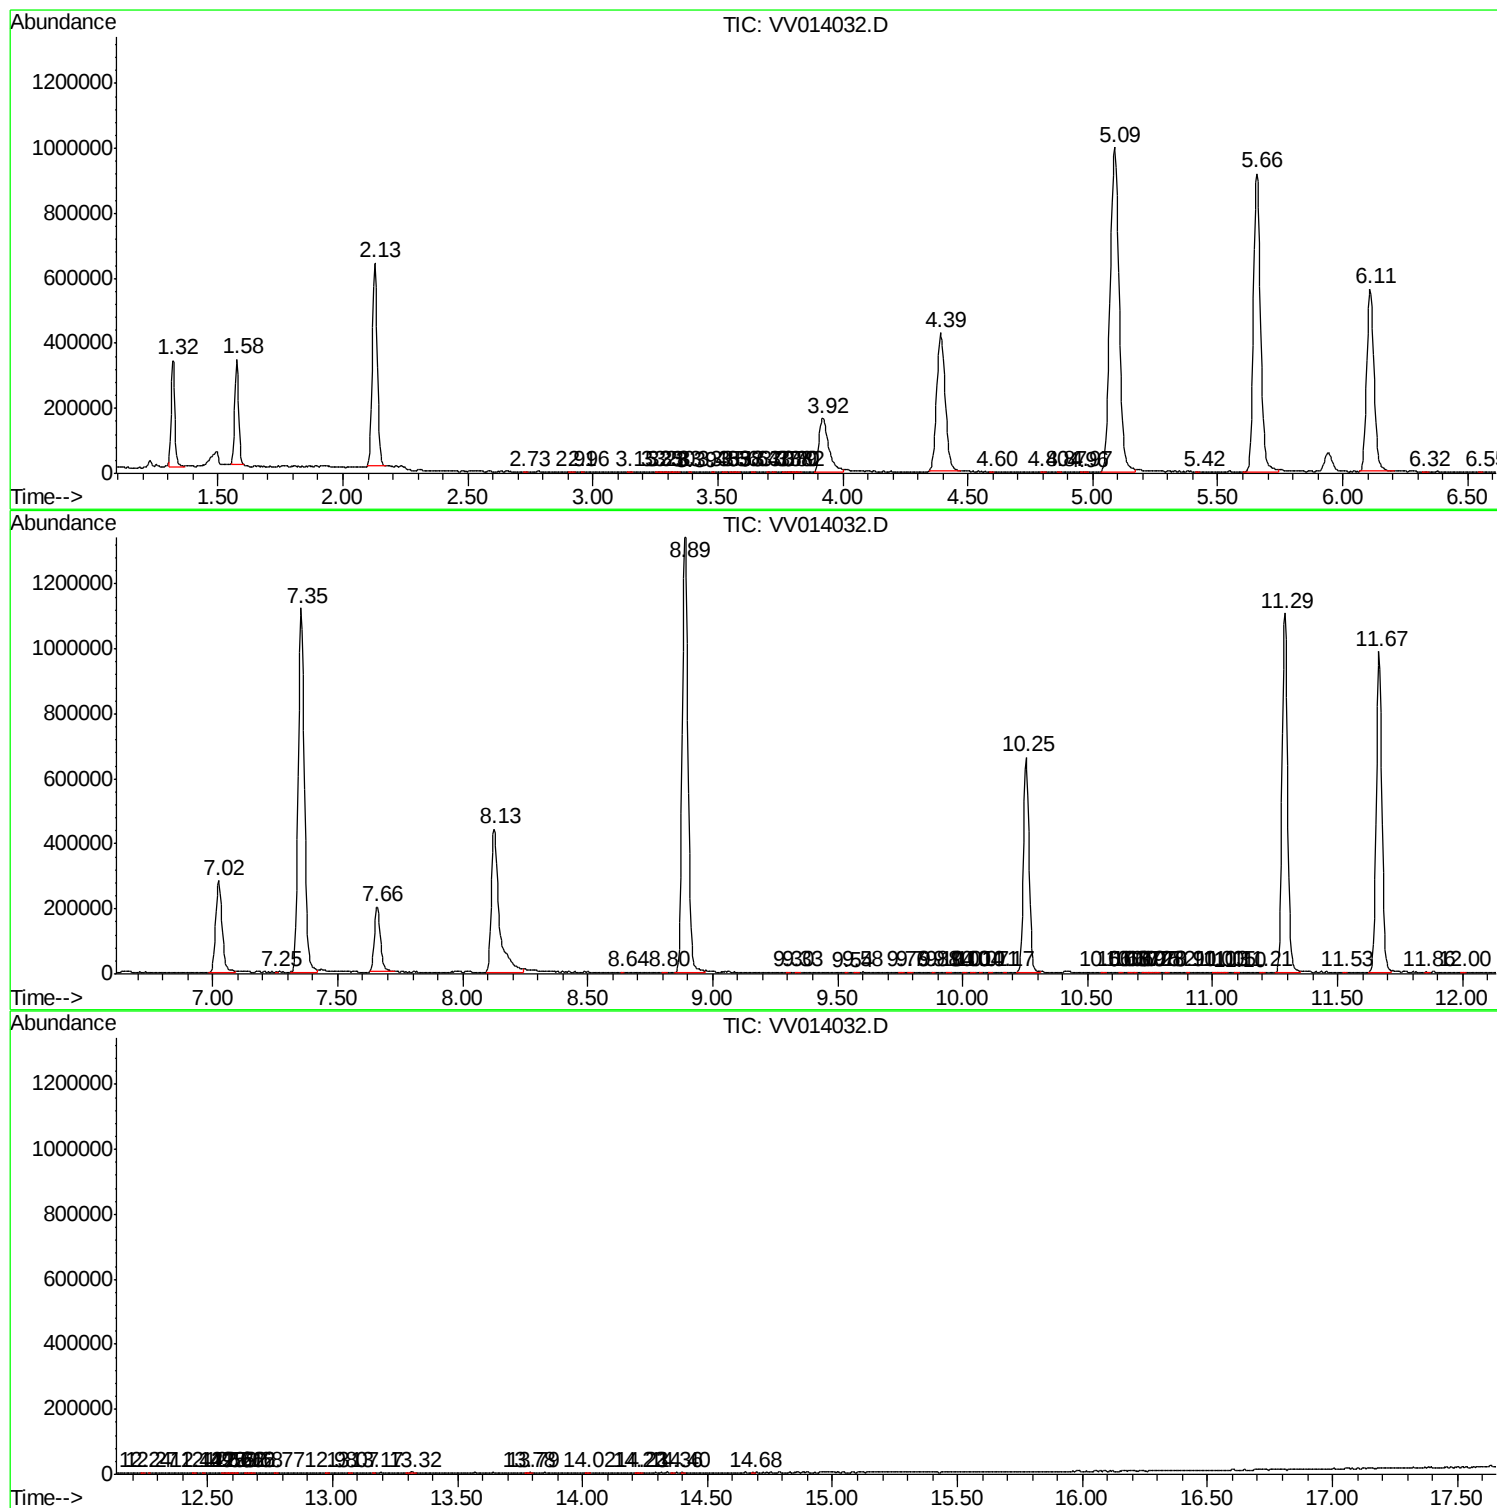

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121219\
Data File : VV014032.D
Acq On : 12 Dec 2019 15:24
Operator : SY/MD
Sample : K6276-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C47

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121219\
Data File : VV014032.D
Acq On : 12 Dec 2019 15:24
Operator : SY/MD
Sample : K6276-09
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0C47

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc