

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014034.D
 Acq On : 12 Dec 2019 16:13
 Operator : SY/MD
 Sample : K6280-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF20

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	266857	265116	12.87%	1.715%
2	2.123	313	321	333	rVB	502406	695021	33.75%	4.496%
3	2.727	507	509	511	rBV2	1116	334	0.02%	0.002%
4	3.042	605	607	608	rBV	524	199	0.01%	0.001%
5	3.068	613	615	619	rBV5	1525	878	0.04%	0.006%
6	3.161	640	644	648	rBV6	1284	1420	0.07%	0.009%
7	3.187	651	652	654	rVB2	1171	421	0.02%	0.003%
8	3.213	658	660	662	rBV3	847	407	0.02%	0.003%
9	3.290	682	684	685	rBV2	808	206	0.01%	0.001%
10	3.306	687	689	692	rVB2	922	404	0.02%	0.003%
11	3.351	701	703	705	rVB3	1196	372	0.02%	0.002%
12	3.418	722	724	727	rBV4	1051	822	0.04%	0.005%
13	3.486	743	745	746	rBV2	609	289	0.01%	0.002%
14	3.495	746	748	750	rVB3	979	374	0.02%	0.002%
15	3.512	750	753	755	rBV2	1460	797	0.04%	0.005%
16	3.550	763	765	767	rBV3	1282	661	0.03%	0.004%
17	3.598	776	780	786	rBV8	968	1070	0.05%	0.007%
18	3.695	808	810	812	rVB2	676	303	0.01%	0.002%
19	3.708	812	814	815	rBV2	1036	552	0.03%	0.004%
20	3.782	834	837	838	rBV2	756	360	0.02%	0.002%
21	3.862	860	862	864	rBV2	694	258	0.01%	0.002%
22	3.881	864	868	870	rBV3	1013	889	0.04%	0.006%
23	3.920	870	880	903	rBV	149070	408242	19.82%	2.641%
24	4.216	970	972	973	rBV2	1199	455	0.02%	0.003%
25	4.393	1013	1027	1046	rBV	353284	838554	40.72%	5.424%
26	4.602	1090	1092	1093	rBV2	970	412	0.02%	0.003%
27	4.711	1124	1126	1127	rBV2	1121	320	0.02%	0.002%
28	4.827	1160	1162	1164	rBV3	909	367	0.02%	0.002%
29	4.897	1181	1184	1186	rBV3	2095	1127	0.05%	0.007%
30	4.936	1193	1196	1198	rBV4	909	617	0.03%	0.004%
31	4.997	1213	1215	1216	rVB2	789	231	0.01%	0.001%
32	5.013	1218	1220	1222	rBV3	1060	543	0.03%	0.004%
33	5.087	1226	1243	1271	rBV2	813940	2059397	100.00%	13.321%
34	5.589	1397	1399	1400	rBV2	1249	549	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014034.D
 Acq On : 12 Dec 2019 16:13
 Operator : SY/MD
 Sample : K6280-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF20

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.605	1402	1404	1406	rBV4	1071	546	0.03%	0.004%
36	5.656	1407	1420	1455	rVV	737240	1472990	71.53%	9.528%
37	6.110	1548	1561	1585	rBV2	484355	983964	47.78%	6.364%
38	6.534	1691	1693	1694	rBV2	1750	773	0.04%	0.005%
39	7.026	1835	1846	1862	rBV	239052	423517	20.57%	2.739%
40	7.354	1937	1948	1965	rBV	942582	1615388	78.44%	10.449%
41	7.659	2034	2043	2058	rBV	167101	275101	13.36%	1.779%
42	7.933	2126	2128	2131	rBV4	2211	1171	0.06%	0.008%
43	8.129	2179	2189	2226	rBV3	443026	986276	47.89%	6.379%
44	8.891	2414	2426	2448	rBV	1094973	1750090	84.98%	11.320%
45	9.527	2622	2624	2627	rBV4	2081	1333	0.06%	0.009%
46	9.807	2709	2711	2712	rBV2	1433	736	0.04%	0.005%
47	10.000	2768	2771	2774	rBV4	1944	1564	0.08%	0.010%
48	10.196	2829	2832	2833	rBV2	2289	1167	0.06%	0.008%
49	10.254	2839	2850	2871	rBV	609162	965336	46.87%	6.244%
50	10.344	2876	2878	2881	rVB3	2119	841	0.04%	0.005%
51	10.543	2936	2940	2943	rBV4	2439	2257	0.11%	0.015%
52	10.707	2990	2991	2992	rBV2	1266	427	0.02%	0.003%
53	10.775	3010	3012	3016	rBV3	1561	1097	0.05%	0.007%
54	10.859	3035	3038	3040	rBV2	1452	893	0.04%	0.006%
55	11.289	3161	3172	3188	rBV	858812	1346599	65.39%	8.710%
56	11.666	3278	3289	3306	rBV	839067	1336293	64.89%	8.643%
57	12.260	3472	3474	3476	rBV3	1244	592	0.03%	0.004%
58	12.640	3590	3592	3595	rBV3	984	690	0.03%	0.004%
59	12.955	3688	3690	3694	rBV4	1799	866	0.04%	0.006%
60	13.157	3749	3753	3755	rBV3	1842	1505	0.07%	0.010%
61	13.395	3825	3827	3831	rBV4	1963	1177	0.06%	0.008%
62	13.781	3944	3947	3949	rBV3	1767	1033	0.05%	0.007%
63	13.794	3949	3951	3956	rVV4	2726	1947	0.09%	0.013%
64	14.456	4152	4157	4159	rBV5	2137	2211	0.11%	0.014%


Sum of corrected areas: 15460347

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121219\
Data File : VV014034.D
Acq On : 12 Dec 2019 16:13
Operator : SY/MD
Sample : K6280-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF20

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

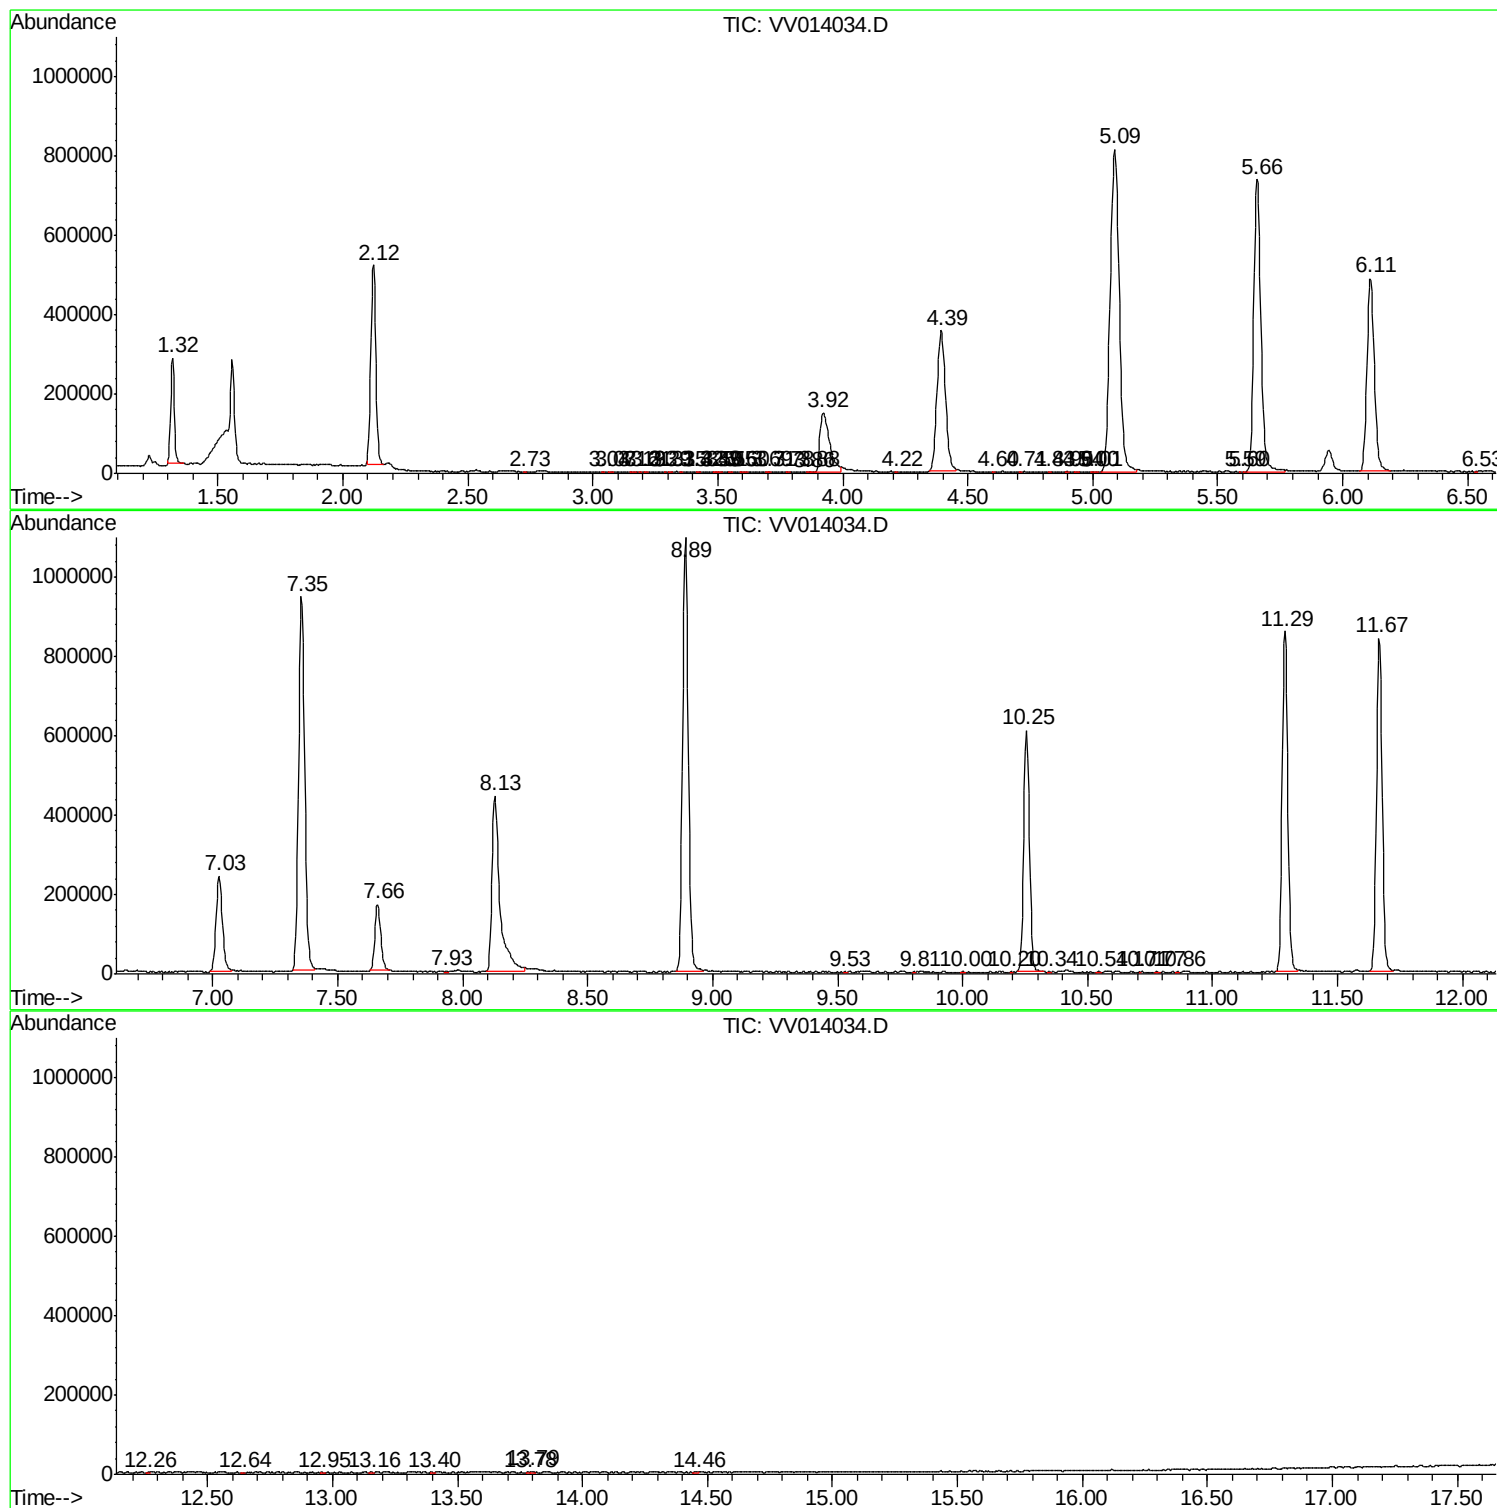

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121219\
Data File : VV014034.D
Acq On : 12 Dec 2019 16:13
Operator : SY/MD
Sample : K6280-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF20

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121219\
Data File : VV014034.D
Acq On : 12 Dec 2019 16:13
Operator : SY/MD
Sample : K6280-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF20

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc