

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014040.D
 Acq On : 12 Dec 2019 18:40
 Operator : SY/MD
 Sample : K6276-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	82	rVB	301216	292733	13.39%	1.774%
2	1.557	140	145	155	rVB	262502	306755	14.03%	1.859%
3	2.123	313	321	335	rVB	513889	719315	32.90%	4.359%
4	2.576	460	462	464	rBV2	1488	617	0.03%	0.004%
5	2.692	496	498	500	rBV3	1154	672	0.03%	0.004%
6	2.843	543	545	550	rVB4	1474	981	0.04%	0.006%
7	2.872	550	554	557	rBV6	1760	1858	0.08%	0.011%
8	2.952	577	579	581	rBV2	1291	666	0.03%	0.004%
9	3.132	634	635	640	rVB3	1801	1175	0.05%	0.007%
10	3.167	640	646	648	rBV6	1318	1313	0.06%	0.008%
11	3.306	686	689	694	rBV6	1264	1127	0.05%	0.007%
12	3.344	699	701	702	rVB2	605	212	0.01%	0.001%
13	3.399	715	718	720	rVB4	1267	614	0.03%	0.004%
14	3.415	720	723	727	rVB3	1153	846	0.04%	0.005%
15	3.444	730	732	737	rBV6	870	465	0.02%	0.003%
16	3.486	742	745	748	rVB4	1565	950	0.04%	0.006%
17	3.502	748	750	753	rBV4	744	354	0.02%	0.002%
18	3.524	753	757	762	rVB6	1526	1275	0.06%	0.008%
19	3.579	772	774	779	rVB4	1216	701	0.03%	0.004%
20	3.624	785	788	789	rBV2	1411	723	0.03%	0.004%
21	3.724	817	819	822	rVB5	1365	671	0.03%	0.004%
22	3.749	822	827	829	rBV5	2069	1517	0.07%	0.009%
23	3.804	843	844	846	rBV2	1228	407	0.02%	0.002%
24	3.823	846	850	853	rBV4	1323	1030	0.05%	0.006%
25	3.852	858	859	861	rBV	754	284	0.01%	0.002%
26	3.862	861	862	863	rBV	1512	541	0.02%	0.003%
27	3.885	868	869	870	rBV	664	164	0.01%	0.001%
28	3.923	870	881	910	rBV	161748	446688	20.43%	2.707%
29	4.264	983	987	989	rBV4	1624	1231	0.06%	0.007%
30	4.393	1012	1027	1054	rBV	356954	884557	40.46%	5.361%
31	4.830	1160	1163	1164	rBV3	813	543	0.02%	0.003%
32	4.865	1172	1174	1178	rVB3	1247	657	0.03%	0.004%
33	4.884	1178	1180	1183	rBV4	1040	474	0.02%	0.003%
34	4.949	1197	1200	1202	rBV3	1172	832	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014040.D
 Acq On : 12 Dec 2019 18:40
 Operator : SY/MD
 Sample : K6276-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.974	1205	1208	1211	rBV5	1282	929	0.04%	0.006%
36	5.087	1225	1243	1273	rBV2	858924	2186234	100.00%	13.250%
37	5.499	1370	1371	1373	rBV2	1072	387	0.02%	0.002%
38	5.659	1407	1421	1444	rBV	756746	1506208	68.90%	9.129%
39	6.113	1550	1562	1585	rVB	530946	1062239	48.59%	6.438%
40	7.026	1835	1846	1875	rVB	258417	458978	20.99%	2.782%
41	7.354	1936	1948	1969	rBV	1003341	1720393	78.69%	10.427%
42	7.659	2033	2043	2061	rBV	180578	294988	13.49%	1.788%
43	8.129	2178	2189	2233	rBV2	439527	1043052	47.71%	6.322%
44	8.569	2323	2326	2329	rBV5	1556	1166	0.05%	0.007%
45	8.646	2342	2350	2353	rBV9	2576	3178	0.15%	0.019%
46	8.820	2402	2404	2406	rBV3	1079	378	0.02%	0.002%
47	8.891	2414	2426	2450	rBV	1114147	1787293	81.75%	10.832%
48	9.347	2566	2568	2570	rBV3	1132	616	0.03%	0.004%
49	9.434	2593	2595	2599	rBV3	1031	487	0.02%	0.003%
50	9.463	2602	2604	2606	rVV3	1312	442	0.02%	0.003%
51	9.614	2649	2651	2652	rBV2	1151	447	0.02%	0.003%
52	9.730	2684	2687	2691	rBV4	1082	670	0.03%	0.004%
53	9.804	2708	2710	2713	rBV3	1377	761	0.03%	0.005%
54	9.939	2750	2752	2754	rBV2	1251	692	0.03%	0.004%
55	10.000	2770	2771	2772	rBV	556	119	0.01%	0.001%
56	10.013	2772	2775	2776	rBV2	1695	842	0.04%	0.005%
57	10.039	2781	2783	2785	rVV3	1091	683	0.03%	0.004%
58	10.077	2789	2795	2797	rBV7	2063	1817	0.08%	0.011%
59	10.116	2805	2807	2810	rBV4	1233	899	0.04%	0.005%
60	10.135	2811	2813	2816	rVB5	1369	684	0.03%	0.004%
61	10.180	2825	2827	2828	rBV2	692	201	0.01%	0.001%
62	10.254	2838	2850	2873	rBV	656043	1026501	46.95%	6.221%
63	10.611	2958	2961	2965	rBV5	1134	962	0.04%	0.006%
64	10.646	2970	2972	2975	rVB4	1005	464	0.02%	0.003%
65	10.662	2975	2977	2978	rBV2	841	381	0.02%	0.002%
66	10.801	3019	3020	3021	rBV	726	160	0.01%	0.001%
67	10.836	3028	3031	3033	rBV4	1165	721	0.03%	0.004%
68	10.849	3033	3035	3038	rVV4	1038	613	0.03%	0.004%
69	10.887	3041	3047	3048	rBV4	1961	1639	0.07%	0.010%
70	11.039	3091	3094	3096	rBV5	1598	847	0.04%	0.005%
71	11.074	3101	3105	3106	rBV3	842	517	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014040.D
 Acq On : 12 Dec 2019 18:40
 Operator : SY/MD
 Sample : K6276-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.180	3136	3138	3140	rBV2	1372	615	0.03%	0.004%
73	11.193	3140	3142	3145	rVB2	1980	1028	0.05%	0.006%
74	11.289	3160	3172	3188	rBV	872569	1335707	61.10%	8.095%
75	11.621	3274	3275	3277	rBV3	1459	747	0.03%	0.005%
76	11.666	3278	3289	3307	rVV	868731	1370032	62.67%	8.303%
77	12.125	3431	3432	3435	rBV3	1273	626	0.03%	0.004%
78	12.228	3461	3464	3467	rBV3	1903	1194	0.05%	0.007%
79	12.360	3503	3505	3508	rBV3	1338	649	0.03%	0.004%
80	12.666	3598	3600	3603	rVB4	1227	439	0.02%	0.003%
81	12.910	3674	3676	3678	rVB2	1114	408	0.02%	0.002%
82	13.083	3726	3730	3732	rBV4	1012	771	0.04%	0.005%
83	13.273	3785	3789	3791	rBV3	1929	1487	0.07%	0.009%
84	13.341	3808	3810	3813	rBV4	1158	647	0.03%	0.004%
85	13.588	3885	3887	3888	rBV2	967	289	0.01%	0.002%
86	13.640	3898	3903	3904	rBV4	2578	1631	0.07%	0.010%
87	13.665	3908	3911	3914	rBV4	1541	1184	0.05%	0.007%
88	14.164	4063	4066	4068	rBV3	1769	1365	0.06%	0.008%
89	14.318	4112	4114	4115	rBV	1679	664	0.03%	0.004%


Sum of corrected areas: 16500019

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
Data File : VV014040.D
Acq On : 12 Dec 2019 18:40
Operator : SY/MD
Sample : K6276-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C56

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

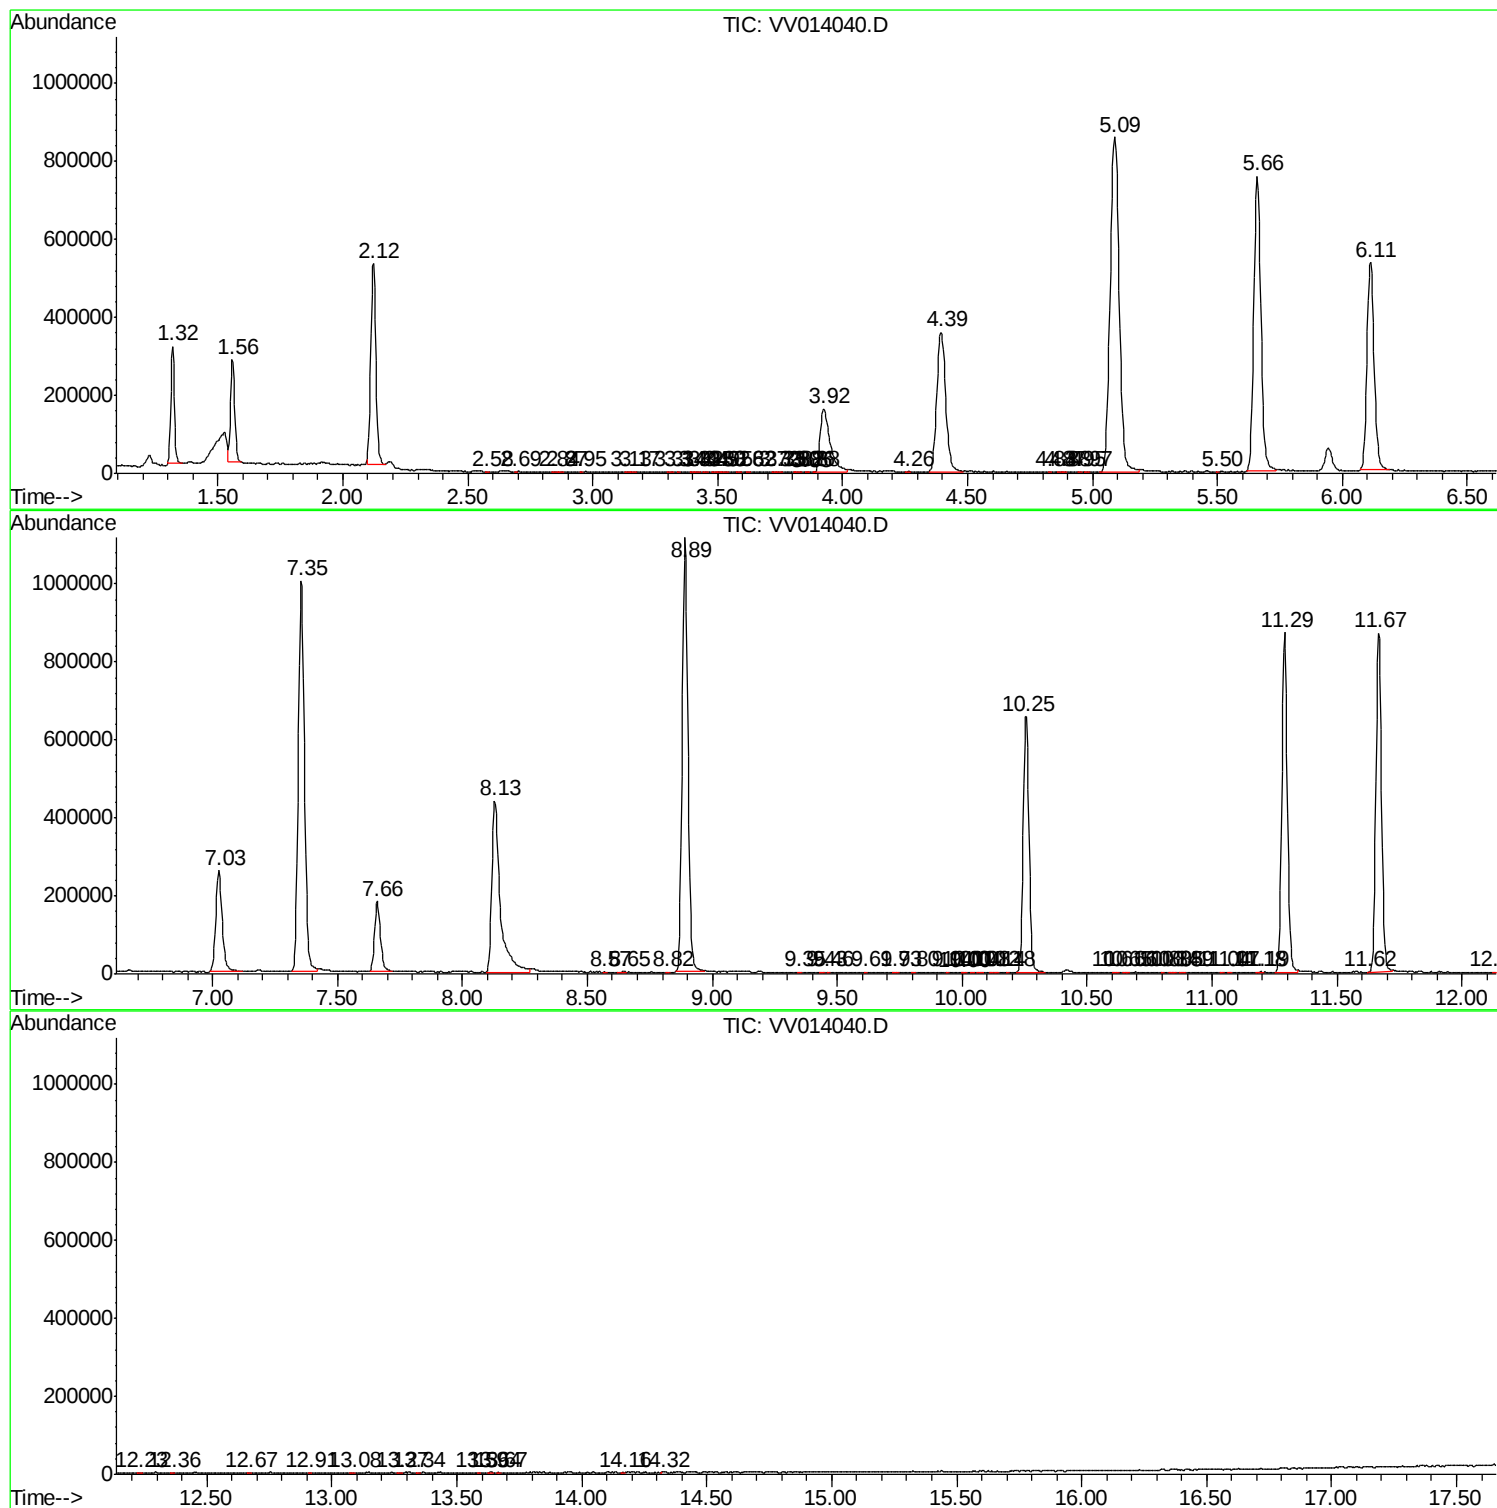

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121219\
Data File : VV014040.D
Acq On : 12 Dec 2019 18:40
Operator : SY/MD
Sample : K6276-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C56

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121219\
Data File : VV014040.D
Acq On : 12 Dec 2019 18:40
Operator : SY/MD
Sample : K6276-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C56

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc