

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014041.D
 Acq On : 12 Dec 2019 19:05
 Operator : SY/MD
 Sample : K6276-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	83	rVB	301072	289408	13.03%	1.743%
2	1.563	142	147	162	rVB	282441	330587	14.88%	1.991%
3	2.126	313	322	333	rVB	539244	753895	33.94%	4.540%
4	2.907	561	565	566	rBV4	1409	947	0.04%	0.006%
5	2.939	573	575	578	rBV2	1042	545	0.02%	0.003%
6	2.955	578	580	582	rVV3	1152	477	0.02%	0.003%
7	3.010	593	597	599	rVB4	1029	802	0.04%	0.005%
8	3.077	616	618	622	rVB3	2161	1085	0.05%	0.007%
9	3.093	622	623	625	rBV2	1089	383	0.02%	0.002%
10	3.106	625	627	629	rBV3	1093	569	0.03%	0.003%
11	3.155	637	642	644	rBV4	2614	1954	0.09%	0.012%
12	3.183	648	651	655	rVV5	1668	1193	0.05%	0.007%
13	3.267	671	677	682	rVB7	1745	2156	0.10%	0.013%
14	3.290	682	684	688	rBV3	1580	1044	0.05%	0.006%
15	3.338	697	699	700	rBV	999	389	0.02%	0.002%
16	3.412	720	722	723	rBV2	515	147	0.01%	0.001%
17	3.457	733	736	738	rBV3	734	464	0.02%	0.003%
18	3.476	740	742	745	rBV3	1094	758	0.03%	0.005%
19	3.524	755	757	759	rBV3	520	252	0.01%	0.002%
20	3.537	759	761	763	rVV3	1006	271	0.01%	0.002%
21	3.595	774	779	783	rBV7	1321	1427	0.06%	0.009%
22	3.618	783	786	788	rBV3	1613	730	0.03%	0.004%
23	3.630	788	790	793	rVV3	826	436	0.02%	0.003%
24	3.666	799	801	804	rVB4	869	448	0.02%	0.003%
25	3.688	805	808	809	rVB3	942	336	0.02%	0.002%
26	3.711	809	815	816	rBV6	1152	961	0.04%	0.006%
27	3.740	823	824	828	rBV2	879	378	0.02%	0.002%
28	3.756	828	829	830	rBV	541	159	0.01%	0.001%
29	3.788	835	839	841	rBV2	1111	763	0.03%	0.005%
30	3.804	841	844	850	rVB7	1425	1233	0.06%	0.007%
31	3.830	850	852	853	rBV2	703	335	0.02%	0.002%
32	3.839	853	855	856	rBV2	1494	579	0.03%	0.003%
33	3.881	866	868	870	rVB	1072	402	0.02%	0.002%
34	3.923	870	881	913	rBV	168993	461016	20.75%	2.776%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014041.D
 Acq On : 12 Dec 2019 19:05
 Operator : SY/MD
 Sample : K6276-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.286	990	994	995	rBV3	1311	839	0.04%	0.005%
36	4.392	1009	1027	1055	rBV	380494	919901	41.41%	5.539%
37	4.643	1102	1105	1110	rBV6	1872	1981	0.09%	0.012%
38	4.762	1140	1142	1145	rBV4	855	312	0.01%	0.002%
39	4.782	1145	1148	1149	rBV3	996	516	0.02%	0.003%
40	4.791	1149	1151	1153	rVB3	1246	433	0.02%	0.003%
41	4.820	1157	1160	1162	rBV4	1460	756	0.03%	0.005%
42	4.846	1165	1168	1172	rBV6	1179	750	0.03%	0.005%
43	4.923	1190	1192	1194	rBV3	1182	691	0.03%	0.004%
44	4.984	1207	1211	1212	rBV4	1422	924	0.04%	0.006%
45	5.090	1226	1244	1268	rBV2	884150	2221273	100.00%	13.376%
46	5.659	1408	1421	1443	rBV	732171	1450251	65.29%	8.733%
47	6.113	1548	1562	1585	rBV	501898	1013977	45.65%	6.106%
48	6.473	1672	1674	1676	rBV3	1200	533	0.02%	0.003%
49	6.498	1680	1682	1683	rBV2	900	426	0.02%	0.003%
50	6.624	1719	1721	1722	rBV	1409	577	0.03%	0.003%
51	6.823	1781	1783	1784	rBV2	859	289	0.01%	0.002%
52	6.913	1805	1811	1816	rBV8	1883	1622	0.07%	0.010%
53	6.933	1816	1817	1818	rBV	981	335	0.02%	0.002%
54	7.026	1830	1846	1863	rBV	245201	436978	19.67%	2.631%
55	7.296	1927	1930	1931	rBV3	1595	908	0.04%	0.005%
56	7.357	1936	1949	1965	rBV	980749	1693551	76.24%	10.198%
57	7.659	2032	2043	2064	rBV	175341	300753	13.54%	1.811%
58	7.842	2098	2100	2103	rBV3	1468	1116	0.05%	0.007%
59	7.907	2117	2120	2122	rBV4	1906	1069	0.05%	0.006%
60	7.974	2135	2141	2146	rBV10	3419	5149	0.23%	0.031%
61	8.129	2178	2189	2222	rBV2	476032	1027405	46.25%	6.187%
62	8.891	2414	2426	2446	rBV	1133737	1804761	81.25%	10.868%
63	9.505	2615	2617	2618	rBV2	1625	692	0.03%	0.004%
64	10.116	2804	2807	2808	rBV3	2249	1174	0.05%	0.007%
65	10.254	2840	2850	2865	rVB	674919	1047382	47.15%	6.307%
66	10.833	3027	3030	3031	rBV3	1526	757	0.03%	0.005%
67	10.961	3067	3070	3071	rBV3	1053	672	0.03%	0.004%
68	11.035	3089	3093	3097	rBV5	1216	948	0.04%	0.006%
69	11.093	3107	3111	3112	rBV4	1199	751	0.03%	0.005%
70	11.289	3160	3172	3190	rBV	883750	1364098	61.41%	8.214%
71	11.547	3250	3252	3254	rBV3	1463	713	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121219\
 Data File : VV014041.D
 Acq On : 12 Dec 2019 19:05
 Operator : SY/MD
 Sample : K6276-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.665	3278	3289	3312	rVB	913129	1431973	64.47%	8.623%
73	11.936	3369	3373	3376	rBV5	1834	1421	0.06%	0.009%
74	11.990	3388	3390	3396	rVB7	1877	1327	0.06%	0.008%
75	12.190	3450	3452	3454	rBV3	1162	502	0.02%	0.003%
76	12.235	3465	3466	3468	rBV2	1025	333	0.01%	0.002%
77	12.405	3516	3519	3524	rVB5	1642	1433	0.06%	0.009%
78	12.463	3535	3537	3538	rBV2	1471	611	0.03%	0.004%
79	12.575	3570	3572	3574	rBV3	1302	646	0.03%	0.004%
80	12.611	3582	3583	3585	rBV2	1208	551	0.02%	0.003%
81	12.685	3604	3606	3608	rBV3	929	436	0.02%	0.003%
82	12.717	3614	3616	3617	rVB2	992	272	0.01%	0.002%
83	12.784	3635	3637	3639	rBV3	1209	608	0.03%	0.004%
84	12.855	3657	3659	3662	rVB3	1228	534	0.02%	0.003%
85	13.054	3718	3721	3722	rBV3	1520	835	0.04%	0.005%
86	13.116	3737	3740	3741	rBV3	1751	933	0.04%	0.006%
87	13.145	3748	3749	3750	rBV	1007	356	0.02%	0.002%
88	13.273	3787	3789	3791	rBV3	1548	711	0.03%	0.004%
89	13.534	3868	3870	3873	rBV3	1386	700	0.03%	0.004%
90	13.878	3975	3977	3981	rBV4	1299	771	0.03%	0.005%


Sum of corrected areas: 16606745

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121219\
Data File : VV014041.D
Acq On : 12 Dec 2019 19:05
Operator : SY/MD
Sample : K6276-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C61

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

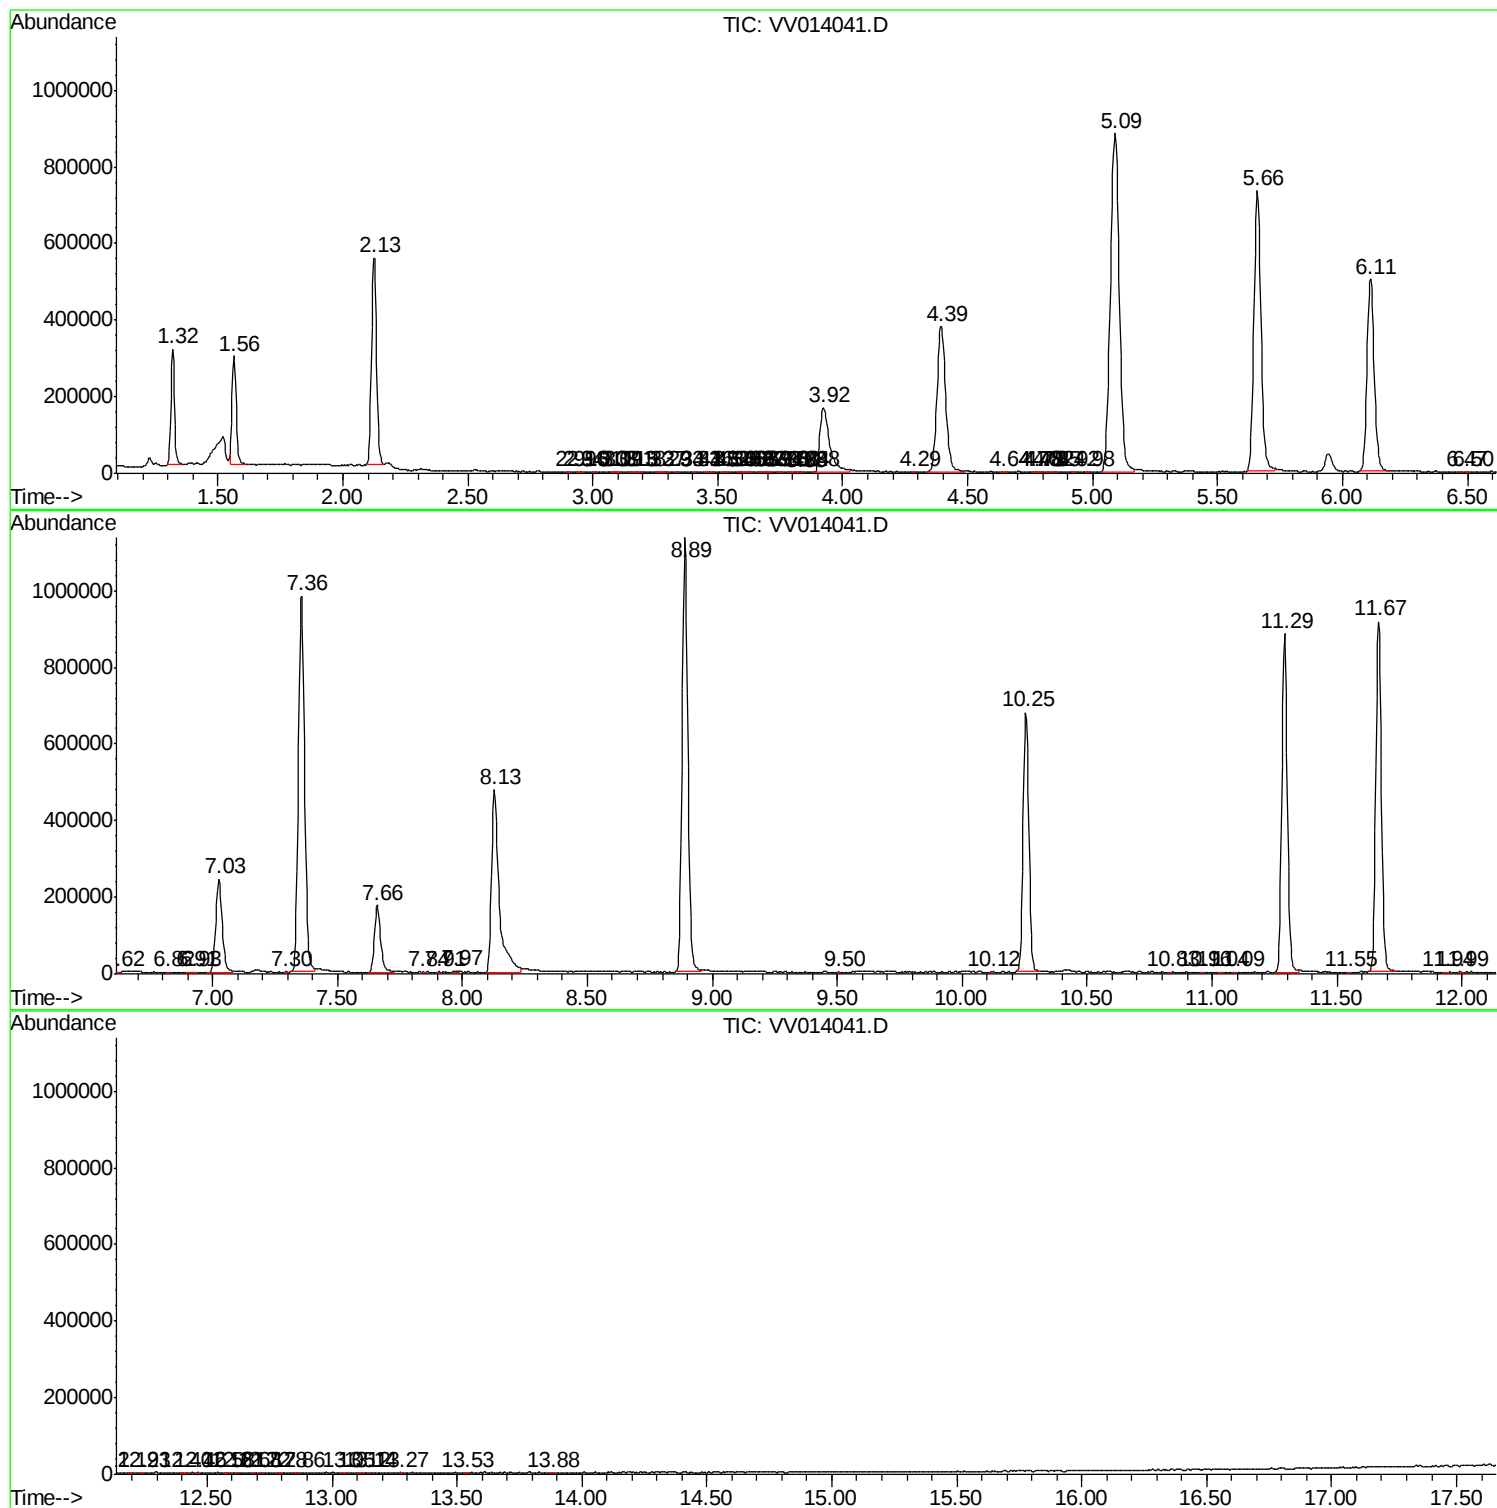

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121219\
Data File : VV014041.D
Acq On : 12 Dec 2019 19:05
Operator : SY/MD
Sample : K6276-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C61

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121219\
Data File : VV014041.D
Acq On : 12 Dec 2019 19:05
Operator : SY/MD
Sample : K6276-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C61

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
