


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121219\
Data File : VV014025.D
Acq On : 12 Dec 2019 09:00
Operator : SY/MD
Sample : BFB81
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis
Last Update : Fri Dec 13 06:14:07 2019

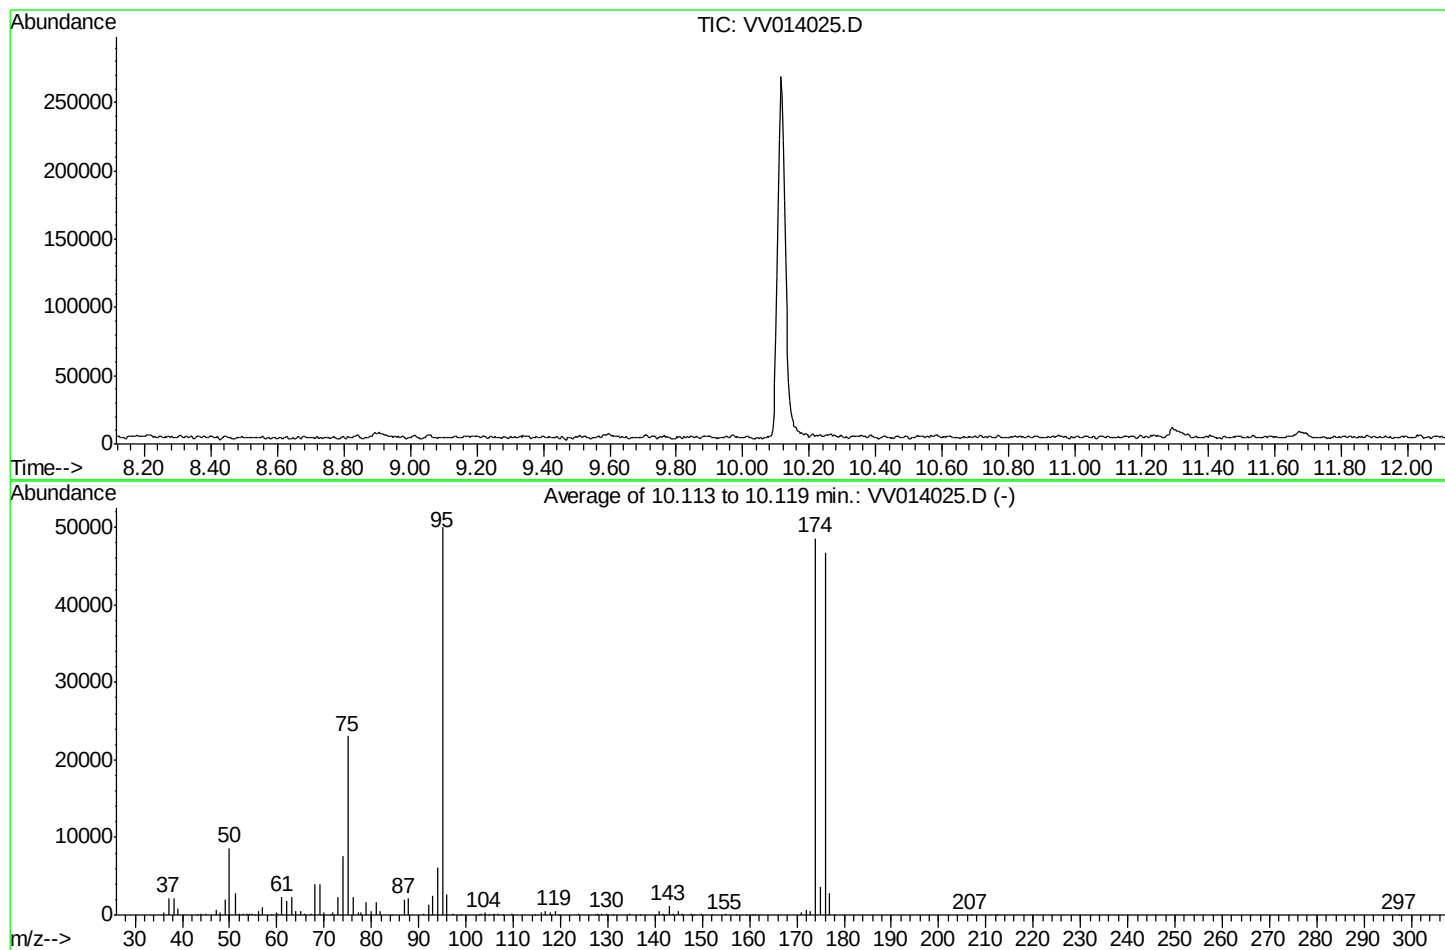

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	8621	PASS
75	95	30	80	46.2	23104	PASS
95	95	100	100	100.0	50013	PASS
96	95	5	9	5.4	2702	PASS
173	174	0.00	2	0.9	436	PASS
174	95	50	120	97.1	48554	PASS
175	174	5	9	7.4	3577	PASS
176	174	95	101	96.3	46760	PASS
177	176	5	9	6.0	2803	PASS

m/z	Abundance
36.00	588.0
37.10	2110.0
38.10	2450.0
39.00	886.0
40.00	952.0
44.00	1088.0
45.00	327.0
45.90	134.0
47.10	682.0
48.00	421.0
49.00	2097.0
50.00	8864.0
51.10	2981.0
52.20	226.0
52.90	153.0
54.20	104.0
54.90	186.0
56.00	604.0
57.00	1058.0
59.90	502.0
61.10	2578.0
62.00	1827.0
63.00	2417.0
64.00	751.0
65.00	459.0
65.90	148.0
67.10	178.0
68.00	3811.0
69.00	3923.0
70.00	368.0
71.90	336.0
73.00	2310.0
74.00	7614.0
75.00	23056.0
76.10	2404.0
77.20	485.0
77.80	346.0
78.90	1558.0
80.00	463.0
80.90	1825.0
81.90	541.0
86.90	2062.0
87.90	1863.0
90.90	233.0
92.00	1409.0
93.00	2371.0
94.00	5855.0
95.00	50536.0
96.00	2786.0
97.20	145.0
102.70	130.0
103.20	109.0
103.90	220.0
105.90	192.0
106.90	124.0
107.80	113.0
109.70	113.0
115.90	286.0
116.80	511.0
117.80	260.0
118.80	503.0
127.30	104.0
127.90	143.0
128.60	129.0
129.90	219.0
131.10	139.0
136.90	123.0
141.00	431.0
142.20	122.0
142.90	1274.0
143.90	151.0
144.90	616.0
145.80	144.0
147.70	240.0
149.80	116.0
151.90	105.0
154.90	181.0
160.70	119.0
161.30	125.0
170.90	342.0
172.00	585.0
172.70	614.0
174.00	47040.0
175.00	3503.0
176.00	44840.0
177.00	2702.0
177.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.00	492.0
37.00	2295.0
38.10	2355.0
39.00	885.0
40.00	901.0
44.00	1002.0
45.00	361.0
45.90	116.0
47.10	693.0
48.10	390.0
49.00	2080.0
50.00	8845.0
51.10	2990.0
52.10	245.0
52.90	162.0
53.70	124.0
54.20	106.0
54.80	184.0
56.00	522.0
57.00	1132.0
58.80	120.0
59.90	408.0
61.10	2453.0
62.00	1851.0
63.00	2389.0
64.00	745.0
65.00	591.0
65.80	158.0
67.10	183.0
68.00	4052.0
69.00	4160.0
70.00	448.0
71.20	105.0
72.00	376.0
73.00	2419.0
74.10	7869.0
75.00	23752.0
76.10	2380.0
77.20	441.0
77.80	261.0
79.00	1555.0
80.00	584.0
80.90	1777.0
81.90	568.0
84.20	136.0
86.90	2063.0
87.90	2231.0
90.90	215.0
92.00	1356.0
93.00	2612.0
94.00	6267.0
95.00	51704.0
96.00	2741.0
97.20	146.0
98.90	107.0
103.20	161.0
104.00	299.0
105.90	180.0
106.80	159.0
107.80	108.0
109.60	108.0
115.90	291.0
116.80	426.0
117.90	286.0
118.80	560.0
123.90	107.0
127.90	211.0
128.60	147.0
129.80	247.0
134.70	151.0
140.90	538.0
141.80	138.0
142.90	1223.0
143.90	156.0
144.90	624.0
145.70	140.0
147.70	256.0
148.30	120.0
149.80	122.0
154.90	143.0
157.00	108.0
159.20	110.0
160.70	123.0
161.30	124.0
170.80	356.0
172.00	760.0
172.70	694.0
174.00	50192.0
175.00	3681.0
176.00	48480.0
177.00	2845.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.10	410.0
37.00	2290.0
38.10	1919.0
39.00	806.0
40.00	823.0
42.60	104.0
43.20	139.0
44.00	948.0
45.00	374.0
47.00	658.0
48.10	397.0
49.00	1849.0
50.00	8154.0
51.10	2616.0
51.90	282.0
52.90	104.0
53.70	144.0
54.30	119.0
54.80	188.0
55.20	136.0
56.10	462.0
57.00	1026.0
58.80	134.0
60.10	355.0
61.10	2149.0
62.10	1851.0
63.10	2205.0
64.00	672.0
65.00	613.0
65.90	150.0
67.10	153.0
68.00	3943.0
69.00	3995.0
70.00	405.0
71.20	134.0
71.90	416.0
73.00	2127.0
74.10	7243.0
75.00	22504.0
76.10	2121.0
77.20	332.0
77.70	240.0
78.00	181.0
79.00	1640.0
80.00	653.0
81.00	1586.0
81.90	564.0
84.20	121.0
86.90	1866.0
87.90	2334.0
91.00	200.0
92.00	1229.0
93.00	2412.0
94.00	6116.0
95.00	47800.0
96.00	2581.0
97.10	115.0
98.90	123.0
103.20	146.0
103.90	314.0
104.90	117.0
105.80	246.0
106.80	127.0
109.60	116.0
114.70	103.0
115.90	237.0
116.80	384.0
117.90	236.0
118.80	541.0
119.80	116.0
123.90	163.0
127.80	286.0
128.60	121.0
129.80	231.0
134.70	178.0
140.10	142.0
140.90	558.0
141.80	129.0
143.00	1009.0
144.00	123.0
144.90	494.0
147.80	241.0
148.30	132.0
149.80	109.0
155.00	102.0
157.10	125.0
159.20	126.0
170.90	361.0
172.00	846.0
174.00	48432.0
175.00	3549.0
176.00	46960.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

177.00	2863.0
206.90	151.0
212.40	112.0
297.40	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.40	142.0
36.10	167.0
38.20	137.0
40.00	854.0
42.70	144.0
44.00	774.0
44.90	123.0
45.90	150.0
46.30	176.0
47.80	129.0
50.50	119.0
51.70	137.0
54.00	141.0
64.20	164.0
71.90	113.0
78.10	106.0
81.20	198.0
88.40	168.0
102.40	112.0
104.60	120.0
110.00	102.0
129.60	138.0
207.70	147.0
232.10	134.0
290.60	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81