

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019547.D
 Acq On : 12 Dec 2020 11:24
 Operator : SY/MD
 Sample : VV1212WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Quant Time: Dec 13 05:18:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 13 04:37:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	661632	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	608746	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.25	152	277587	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	198919	41.93	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.86%
7) Chloroethane-d5	1.57	69	169802	45.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.76%
11) 1,1-Dichloroethene-d2	2.11	63	294975	33.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.00%
21) 2-Butanone-d5	3.89	46	275027	106.65	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.65%
24) Chloroform-d	4.35	84	387613	45.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.66%
26) 1,2-Dichloroethane-d4	5.04	65	272660	48.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.58%
32) Benzene-d6	5.05	84	762463	46.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.92%
36) 1,2-Dichloropropane-d6	6.07	67	246627	48.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.98%
41) Toluene-d8	7.32	98	665206	45.51	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.02%
43) trans-1,3-Dichloropropene-	7.62	79	128313	44.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.72%
47) 2-Hexanone-d5	8.09	63	206342	103.37	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.37%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	334567	48.63	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.26%
64) 1,2-Dichlorobenzene-d4	11.63	152	248325	47.86	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.72%


Target Compounds					Ovalue
46) Tetrachloroethene	7.98	164	4871	1.498 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121220\
Data File : VV019547.D
Acq On : 12 Dec 2020 11:24
Operator : SY/MD
Sample : VV1212WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Time: Dec 13 05:18:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Sun Dec 13 04:37:51 2020
Response via : Initial Calibration

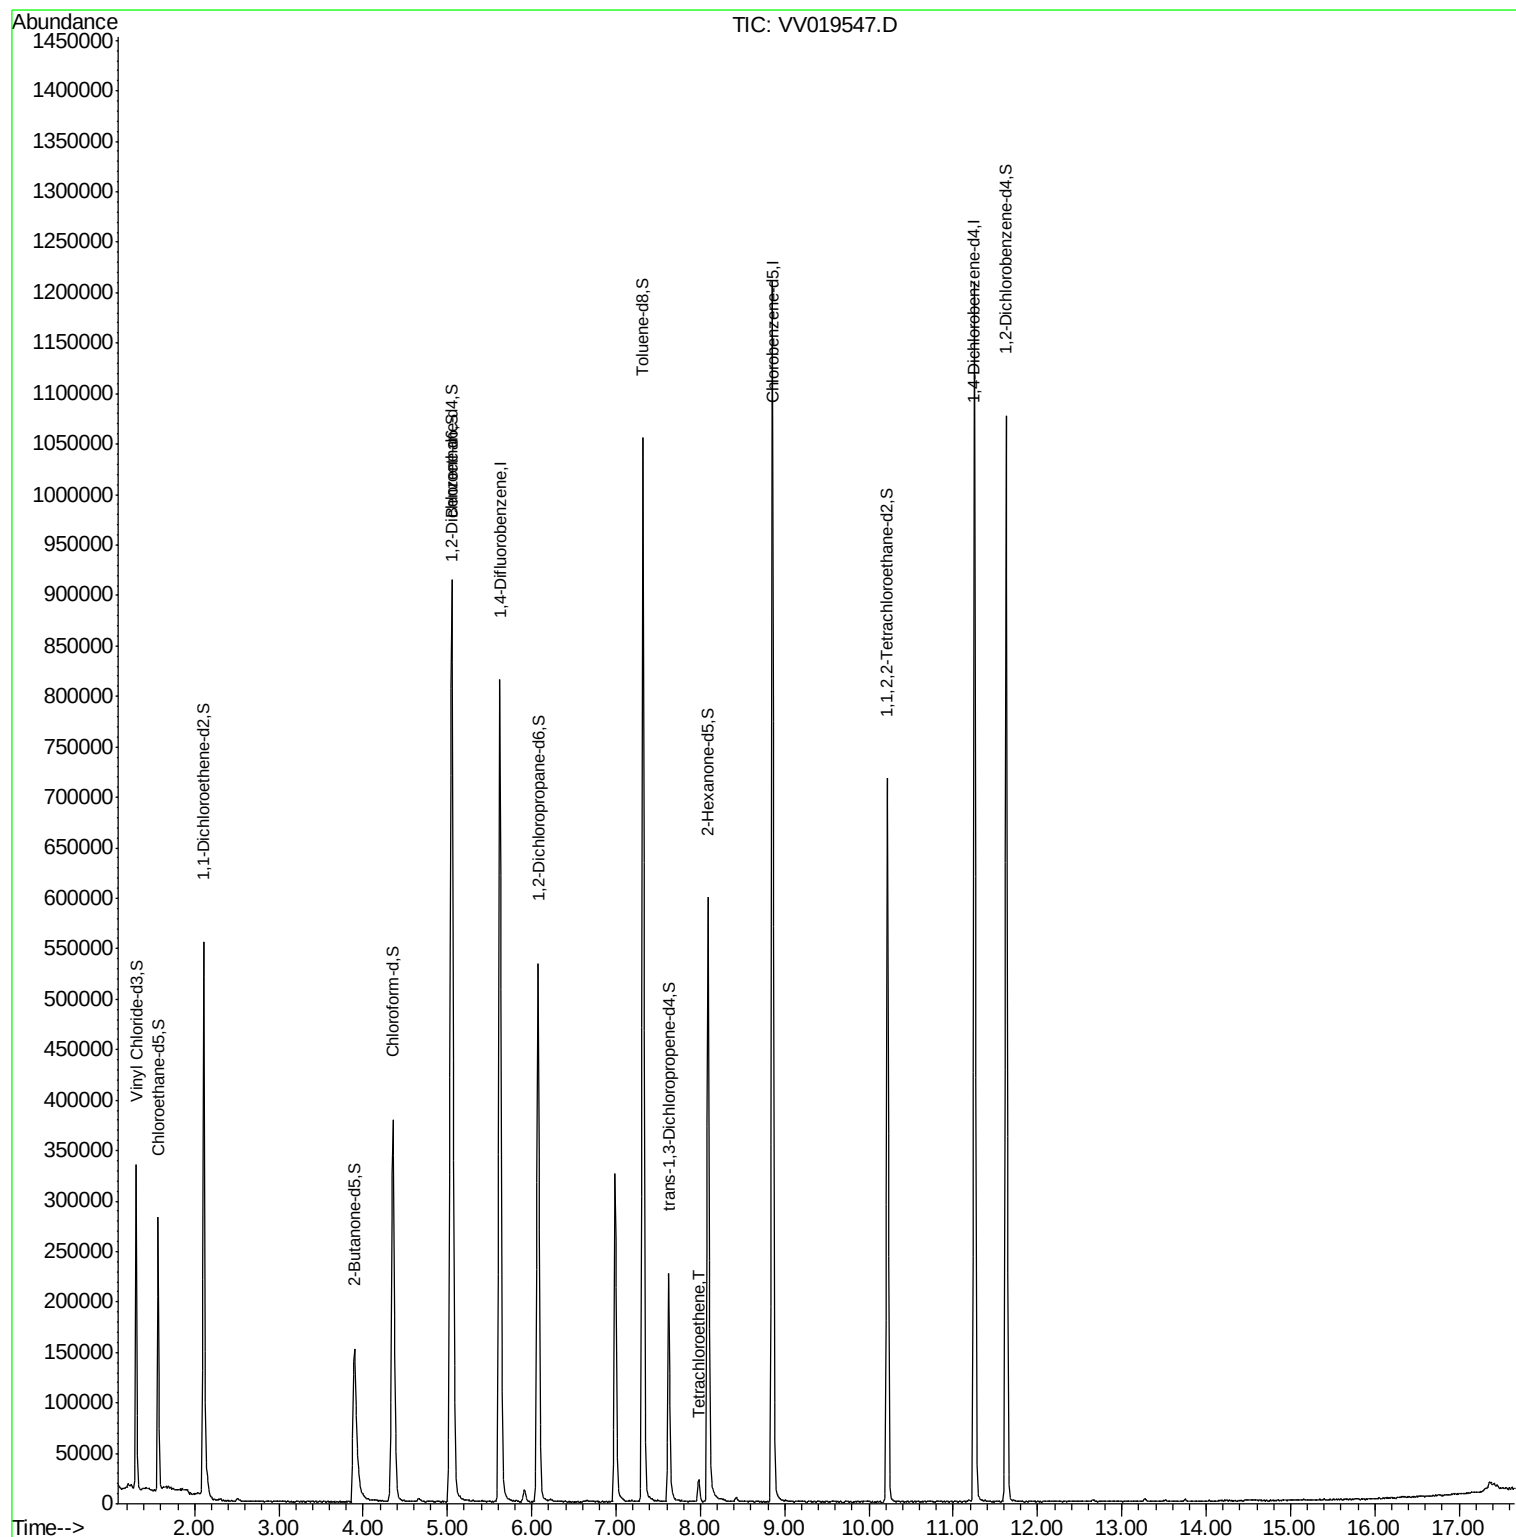

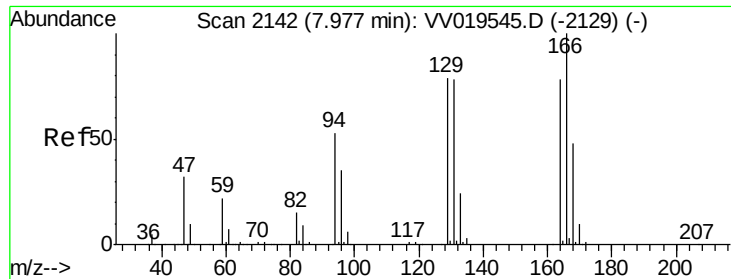

#46

Tetrachloroethene

Concen: 1.498 ug/L

RT: 7.98 min Scan# 2143

Delta R.T. 0.00 min

Lab File: VV019547.D


Acq: 12 Dec 2020 11:24

Instrument :

MSVOA_V

ClientSampleId :

VBLK63

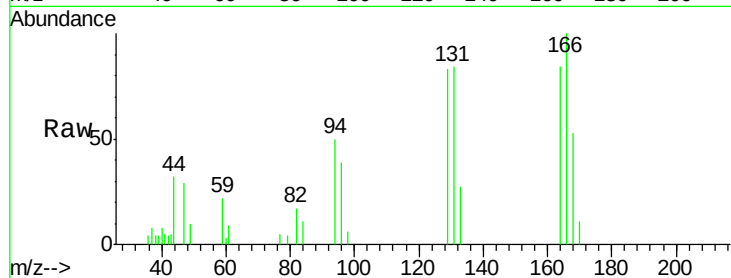

Tot Ion:164 Resp: 4871

Ion Ratio Lower Upper

164 100

129 98.9 70.6 131.0

131 100.6 68.0 126.4

166 119.3 86.9 161.5

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

