

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019586.D
 Acq On : 13 Dec 2020 04:04
 Operator : SY/MD
 Sample : L4998-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Quant Time: Dec 13 09:04:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 13 07:40:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	590959	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	546334	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.25	152	250430	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	233624	55.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	110.26%
7) Chloroethane-d5	1.57	69	194337	58.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	116.30%
11) 1,1-Dichloroethene-d2	2.11	63	336119	42.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.48%
21) 2-Butanone-d5	3.89	46	277537	120.50	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	120.50%
24) Chloroform-d	4.35	84	422769	55.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.72%
26) 1,2-Dichloroethane-d4	5.04	65	298529	59.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	119.62%
32) Benzene-d6	5.05	84	844459	57.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.90%
36) 1,2-Dichloropropane-d6	6.07	67	267351	58.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	117.14%
41) Toluene-d8	7.32	98	737715	56.23	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.46%
43) trans-1,3-Dichloropropene-	7.62	79	129492	49.88	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.76%
47) 2-Hexanone-d5	8.09	63	204174	113.97	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	113.97%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	349470	56.60	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	113.20%
64) 1,2-Dichlorobenzene-d4	11.63	152	266053	56.83	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.66%


Target Compounds					Ovalue
13) Acetone	2.19	43	5510	2.808 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121220\
Data File : VV019586.D
Acq On : 13 Dec 2020 04:04
Operator : SY/MD
Sample : L4998-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Time: Dec 13 09:04:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Sun Dec 13 07:40:15 2020
Response via : Initial Calibration

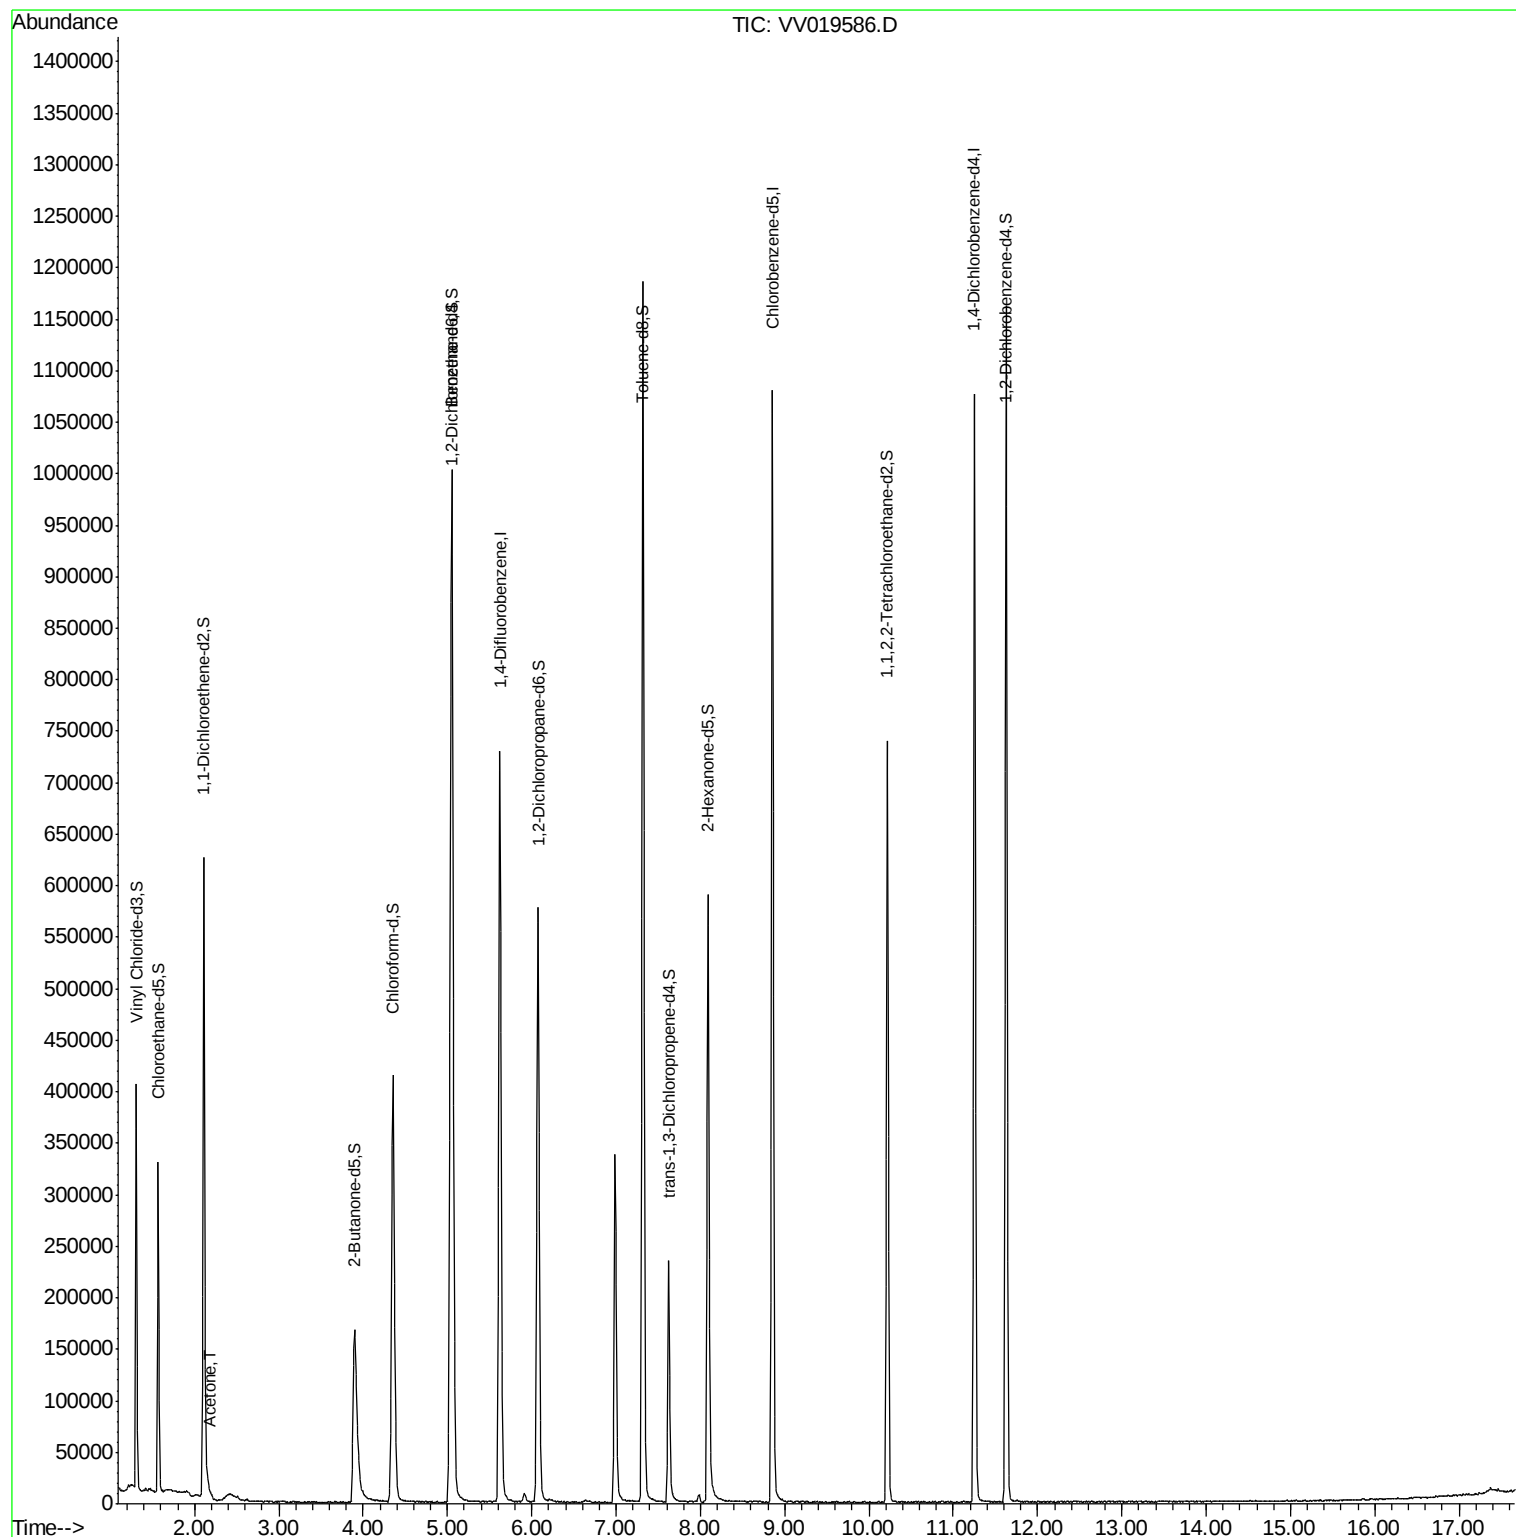

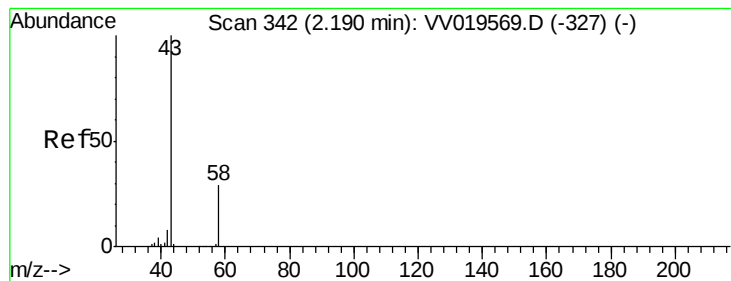

#13
 Acetone
 Concen: 2.808 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. -0.00 min
 Lab File: VV019586.D
 Acq: 13 Dec 2020 04:04

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Tot Ion: 43 Resp: 5510
 Ion Ratio Lower Upper
 43 100
 58 24.3 0.0 61.6

