

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019555.D
 Acq On : 12 Dec 2020 14:52
 Operator : SY/MD
 Sample : L5056-04DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4N1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	84	rVB	308979	305178	12.94%	1.497%
2	1.569	142	149	161	rBV	262857	293448	12.44%	1.439%
3	2.110	307	317	357	rVB	531412	850851	36.07%	4.173%
4	2.499	434	438	439	rBV3	2147	1216	0.05%	0.006%
5	2.868	549	553	555	rBV3	636	448	0.02%	0.002%
6	2.968	581	584	586	rBV3	577	406	0.02%	0.002%
7	3.048	599	609	624	rVV4	7978	17250	0.73%	0.085%
8	3.103	624	626	632	rVB4	907	643	0.03%	0.003%
9	3.155	638	642	647	rVB5	966	704	0.03%	0.003%
10	3.184	647	651	654	rBV3	661	604	0.03%	0.003%
11	3.286	681	683	686	rBV2	753	488	0.02%	0.002%
12	3.325	692	695	700	rBV3	1004	900	0.04%	0.004%
13	3.537	756	761	765	rBV3	511	416	0.02%	0.002%
14	3.589	771	777	781	rBV3	782	854	0.04%	0.004%
15	3.765	820	832	837	rBV7	2767	5664	0.24%	0.028%
16	3.897	862	873	906	rBV	142770	456604	19.36%	2.239%
17	4.235	975	978	981	rBV5	704	461	0.02%	0.002%
18	4.290	993	995	998	rBV3	840	584	0.02%	0.003%
19	4.354	998	1015	1049	rVV	380086	943869	40.02%	4.629%
20	4.949	1196	1200	1202	rVB4	754	504	0.02%	0.002%
21	5.052	1214	1232	1264	rBV2	920477	2358771	100.00%	11.568%
22	5.621	1394	1409	1441	rBV	834715	1661494	70.44%	8.148%
23	5.920	1490	1502	1522	rVB	13995	35799	1.52%	0.176%
24	6.000	1523	1527	1530	rBV4	644	520	0.02%	0.003%
25	6.074	1536	1550	1579	rBV	529927	1075079	45.58%	5.272%
26	6.370	1637	1642	1645	rBV4	730	726	0.03%	0.004%
27	6.415	1653	1656	1663	rVB4	797	589	0.02%	0.003%
28	6.482	1674	1677	1680	rBV3	733	493	0.02%	0.002%
29	6.569	1699	1704	1707	rBV4	584	571	0.02%	0.003%
30	6.634	1716	1724	1727	rBV7	1546	1993	0.08%	0.010%
31	6.781	1766	1770	1772	rBV3	691	469	0.02%	0.002%
32	6.990	1822	1835	1855	rBV	332004	591613	25.08%	2.901%
33	7.170	1888	1891	1896	rBV5	603	620	0.03%	0.003%
34	7.196	1896	1899	1902	rVB4	948	573	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019555.D
 Acq On : 12 Dec 2020 14:52
 Operator : SY/MD
 Sample : L5056-04DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4N1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	7.318	1925	1937	1964	rBV	1093877	1887512	80.02%	9.257%
36	7.624	2022	2032	2064	rVV	231182	401084	17.00%	1.967%
37	7.817	2089	2092	2096	rVB4	852	627	0.03%	0.003%
38	7.855	2100	2104	2106	rBV2	953	673	0.03%	0.003%
39	7.978	2126	2142	2162	rVV	1045288	1747124	74.07%	8.568%
40	8.090	2166	2177	2220	rVV	579492	993672	42.13%	4.873%
41	8.360	2257	2261	2262	rBV2	824	506	0.02%	0.002%
42	8.415	2272	2278	2279	rBV3	1284	1169	0.05%	0.006%
43	8.572	2322	2327	2329	rBV3	481	502	0.02%	0.002%
44	8.785	2390	2393	2399	rVB4	534	450	0.02%	0.002%
45	8.855	2400	2415	2440	rBV	1233983	1991605	84.43%	9.767%
46	9.196	2517	2521	2523	rVB3	899	430	0.02%	0.002%
47	9.277	2542	2546	2548	rBV3	515	416	0.02%	0.002%
48	9.305	2551	2555	2558	rBV4	836	629	0.03%	0.003%
49	9.325	2558	2561	2565	rVB4	701	582	0.02%	0.003%
50	9.932	2745	2750	2752	rBV2	691	708	0.03%	0.003%
51	9.945	2752	2754	2757	rVB3	1048	563	0.02%	0.003%
52	9.974	2757	2763	2765	rBV3	592	610	0.03%	0.003%
53	10.219	2827	2839	2861	rVV	716882	1114429	47.25%	5.465%
54	10.299	2861	2864	2868	rVB4	903	661	0.03%	0.003%
55	10.482	2917	2921	2926	rBV5	513	484	0.02%	0.002%
56	10.569	2945	2948	2950	rBV2	667	502	0.02%	0.002%
57	10.585	2950	2953	2958	rVV6	581	597	0.03%	0.003%
58	10.672	2975	2980	2982	rVV2	653	583	0.02%	0.003%
59	10.701	2987	2989	2992	rVB3	694	439	0.02%	0.002%
60	10.730	2992	2998	3001	rBV3	814	1000	0.04%	0.005%
61	11.016	3082	3087	3090	rBV5	983	809	0.03%	0.004%
62	11.112	3114	3117	3120	rBV4	535	435	0.02%	0.002%
63	11.161	3129	3132	3139	rBV5	943	643	0.03%	0.003%
64	11.186	3139	3140	3144	rVB3	743	474	0.02%	0.002%
65	11.251	3144	3160	3188	rBV	1231428	1908137	80.90%	9.358%
66	11.360	3191	3194	3196	rBV3	973	530	0.02%	0.003%
67	11.553	3249	3254	3259	rBV5	1063	1136	0.05%	0.006%
68	11.627	3261	3277	3294	rBV	1095644	1696326	71.92%	8.319%
69	11.813	3331	3335	3337	rBV3	532	464	0.02%	0.002%
70	11.878	3353	3355	3362	rVV4	1102	900	0.04%	0.004%
71	12.157	3437	3442	3445	rVV3	495	559	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019555.D
 Acq On : 12 Dec 2020 14:52
 Operator : SY/MD
 Sample : L5056-04DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4N1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	12.225	3458	3463	3464	rBV2	575	535	0.02%	0.003%
73	12.244	3464	3469	3471	rBV2	587	571	0.02%	0.003%
74	12.431	3525	3527	3534	rVV4	476	561	0.02%	0.003%
75	12.649	3591	3595	3600	rVB5	1633	1568	0.07%	0.008%
76	12.733	3617	3621	3626	rBV5	782	660	0.03%	0.003%
77	12.810	3640	3645	3646	rBV4	745	601	0.03%	0.003%
78	12.884	3664	3668	3671	rVB4	806	544	0.02%	0.003%
79	12.916	3672	3678	3683	rBV8	1043	984	0.04%	0.005%
80	13.022	3705	3711	3714	rBV5	815	1023	0.04%	0.005%
81	13.064	3722	3724	3728	rBV2	813	432	0.02%	0.002%
82	13.212	3767	3770	3773	rBV3	760	586	0.02%	0.003%
83	13.276	3785	3790	3793	rVV4	1286	1169	0.05%	0.006%
84	13.492	3853	3857	3859	rBV3	1211	856	0.04%	0.004%
85	13.585	3884	3886	3893	rVB3	703	755	0.03%	0.004%
86	13.649	3902	3906	3909	rBV3	868	805	0.03%	0.004%
87	13.691	3916	3919	3921	rBV2	645	434	0.02%	0.002%
88	13.723	3926	3929	3932	rVB2	726	522	0.02%	0.003%
89	13.833	3960	3963	3967	rVB4	781	491	0.02%	0.002%
90	13.862	3967	3972	3978	rBV4	733	911	0.04%	0.004%
91	13.910	3984	3987	3992	rBV4	909	798	0.03%	0.004%
92	14.019	4017	4021	4025	rBV3	908	1000	0.04%	0.005%
93	14.042	4025	4028	4032	rVB4	1108	833	0.04%	0.004%
94	14.067	4032	4036	4039	rVB4	1002	825	0.03%	0.004%
95	14.087	4039	4042	4045	rBV3	823	667	0.03%	0.003%
96	14.472	4159	4162	4165	rBV4	660	407	0.02%	0.002%
97	14.550	4181	4186	4189	rBV7	1454	1661	0.07%	0.008%
98	14.672	4220	4224	4226	rBV4	859	719	0.03%	0.004%
99	14.900	4292	4295	4299	rBV6	1536	1295	0.05%	0.006%
100	15.254	4403	4405	4410	rVB4	818	494	0.02%	0.002%


Sum of corrected areas: 20391079

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121220\
Data File : VV019555.D
Acq On : 12 Dec 2020 14:52
Operator : SY/MD
Sample : L5056-04DL 1000X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4N1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

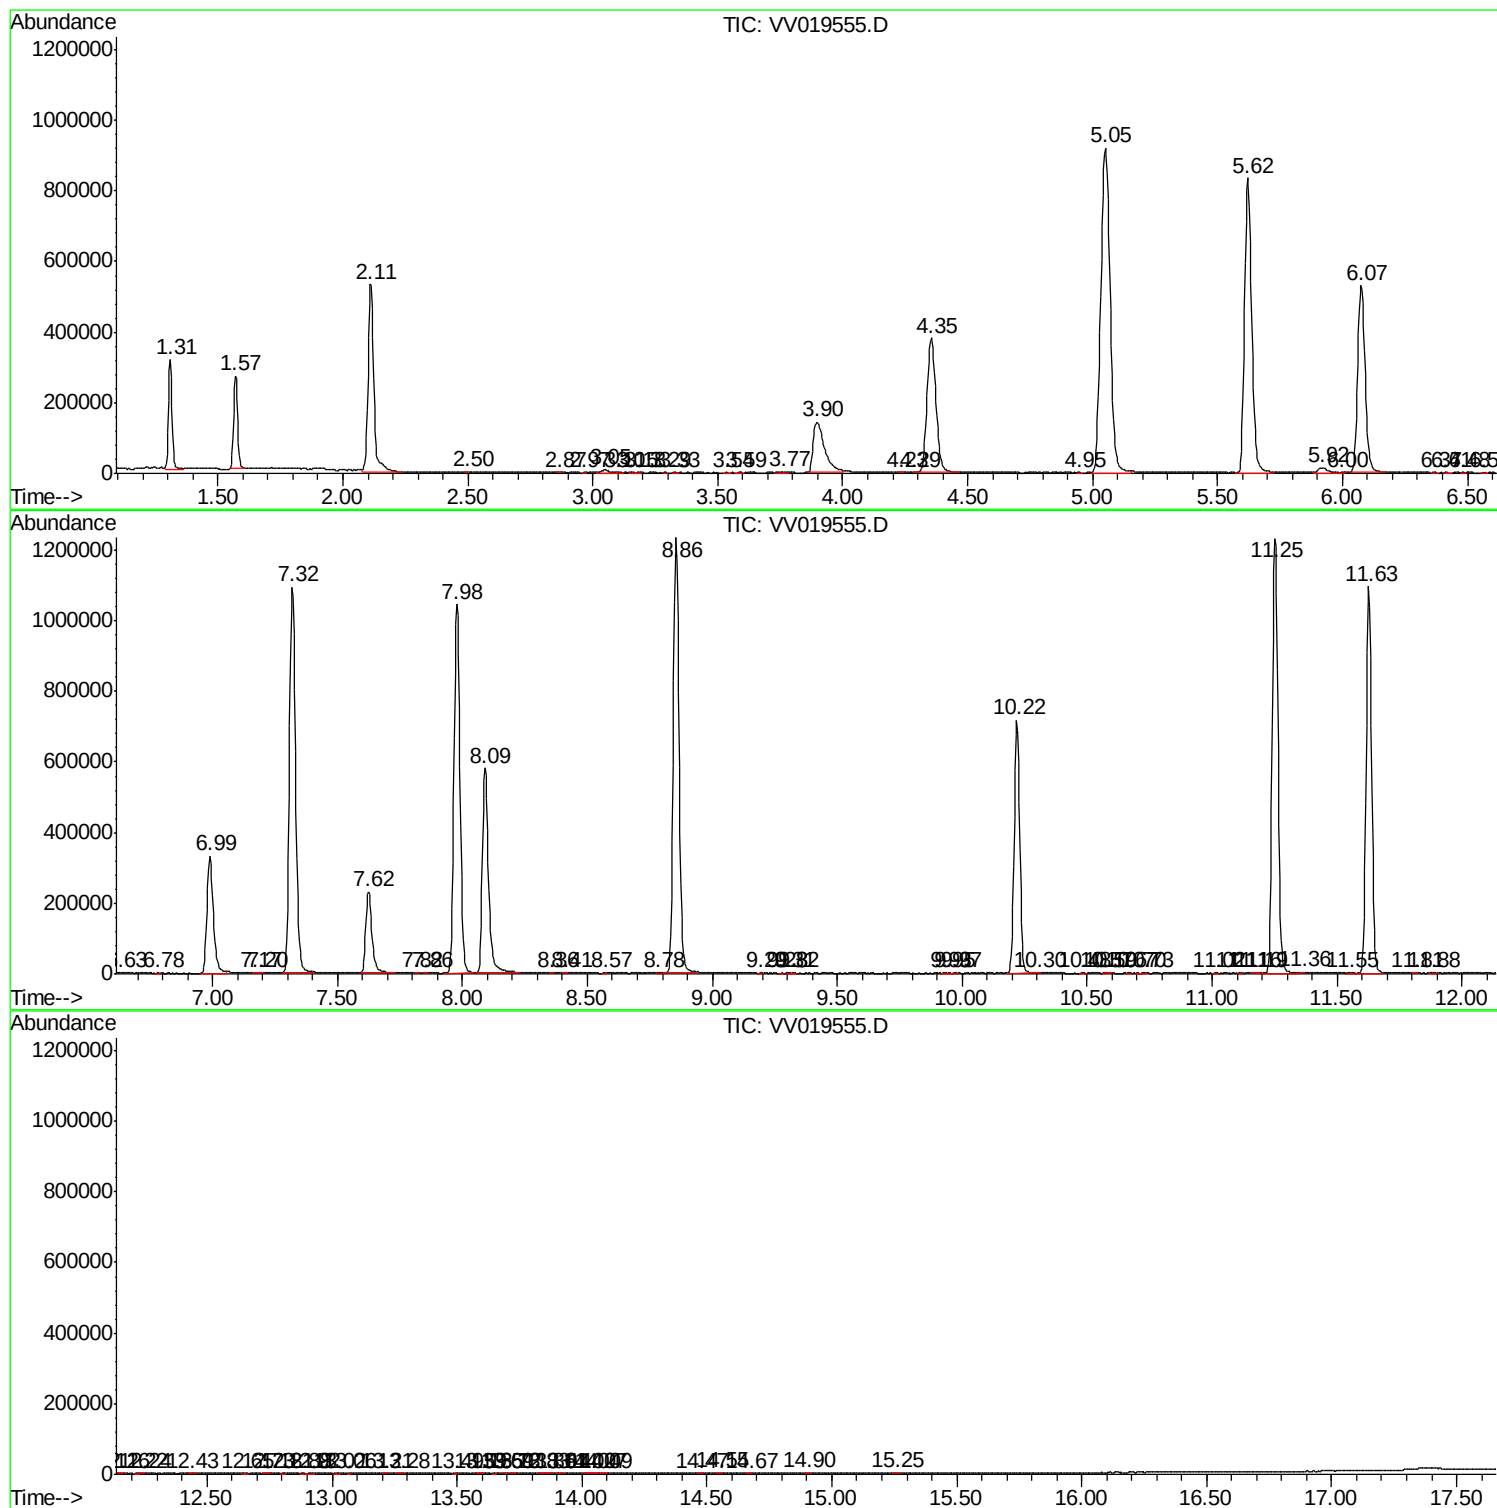

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121220\
Data File : VV019555.D
Acq On : 12 Dec 2020 14:52
Operator : SY/MD
Sample : L5056-04DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4N1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121220\
Data File : VV019555.D
Acq On : 12 Dec 2020 14:52
Operator : SY/MD
Sample : L5056-04DL 1000X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4N1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc