

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019586.D
 Acq On : 13 Dec 2020 04:04
 Operator : SY/MD
 Sample : L4998-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	81	rVB	394074	383464	14.76%	2.017%
2	1.570	142	149	163	rVB	320087	354129	13.63%	1.862%
3	2.110	308	317	354	rVB	623739	971735	37.40%	5.110%
4	2.891	557	560	564	rBV5	641	599	0.02%	0.003%
5	3.123	629	632	633	rBV2	285	173	0.01%	0.001%
6	3.164	642	645	647	rBV2	825	534	0.02%	0.003%
7	3.193	651	654	658	rBV3	512	397	0.02%	0.002%
8	3.213	658	660	663	rBV2	378	195	0.01%	0.001%
9	3.287	678	683	684	rBV3	593	386	0.01%	0.002%
10	3.306	686	689	694	rVB5	785	611	0.02%	0.003%
11	3.344	699	701	703	rVV2	546	245	0.01%	0.001%
12	3.418	723	724	728	rBV2	515	336	0.01%	0.002%
13	3.650	791	796	797	rBV2	456	373	0.01%	0.002%
14	3.663	797	800	802	rVB3	760	457	0.02%	0.002%
15	3.676	802	804	806	rBV	472	238	0.01%	0.001%
16	3.730	819	821	826	rBV3	566	263	0.01%	0.001%
17	3.785	836	838	839	rBV	502	206	0.01%	0.001%
18	3.817	846	848	849	rBV2	244	84	0.00%	0.000%
19	3.897	858	873	912	rBV2	167680	581215	22.37%	3.056%
20	4.354	999	1015	1041	rBV	413177	1018371	39.20%	5.355%
21	4.733	1130	1133	1135	rBV3	738	516	0.02%	0.003%
22	4.772	1142	1145	1146	rBV	784	348	0.01%	0.002%
23	4.894	1181	1183	1185	rBV2	443	223	0.01%	0.001%
24	4.907	1185	1187	1189	rBV2	382	181	0.01%	0.001%
25	4.942	1196	1198	1199	rBV2	221	77	0.00%	0.000%
26	4.971	1203	1207	1210	rBV4	600	389	0.01%	0.002%
27	5.052	1210	1232	1272	rBV2	1003121	2597957	100.00%	13.662%
28	5.479	1362	1365	1368	rBV2	654	513	0.02%	0.003%
29	5.621	1396	1409	1442	rBV	728685	1445788	55.65%	7.603%
30	6.074	1536	1550	1581	rBV	577233	1173111	45.16%	6.169%
31	6.396	1648	1650	1651	rBV	460	194	0.01%	0.001%
32	6.460	1668	1670	1672	rBV2	312	125	0.00%	0.001%
33	6.479	1673	1676	1681	rVB3	1022	732	0.03%	0.004%
34	6.505	1681	1684	1687	rBV2	628	418	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019586.D
 Acq On : 13 Dec 2020 04:04
 Operator : SY/MD
 Sample : L4998-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.592	1707	1711	1714	rBV4	708	571	0.02%	0.003%
36	6.621	1714	1720	1721	rBV4	1250	1024	0.04%	0.005%
37	6.785	1768	1771	1772	rBV3	623	358	0.01%	0.002%
38	6.830	1783	1785	1786	rBV2	366	155	0.01%	0.001%
39	6.865	1791	1796	1799	rBV5	564	491	0.02%	0.003%
40	6.888	1799	1803	1805	rBV2	426	216	0.01%	0.001%
41	6.901	1805	1807	1810	rVB2	595	321	0.01%	0.002%
42	6.917	1810	1812	1818	rBV3	505	432	0.02%	0.002%
43	6.946	1818	1821	1823	rBV4	443	279	0.01%	0.001%
44	6.987	1823	1834	1863	rBV	338388	611817	23.55%	3.217%
45	7.319	1924	1937	1966	rBV	1184652	2036480	78.39%	10.709%
46	7.624	2020	2032	2060	rBV	234584	410712	15.81%	2.160%
47	7.926	2123	2126	2128	rBV4	862	560	0.02%	0.003%
48	7.981	2135	2143	2154	rVB5	7233	13363	0.51%	0.070%
49	8.090	2166	2177	2212	rBV	589813	1019419	39.24%	5.361%
50	8.563	2318	2324	2326	rBV4	594	625	0.02%	0.003%
51	8.688	2361	2363	2366	rBV4	542	411	0.02%	0.002%
52	8.740	2375	2379	2382	rBV4	980	730	0.03%	0.004%
53	8.778	2389	2391	2393	rVB2	596	236	0.01%	0.001%
54	8.791	2393	2395	2397	rBV2	346	223	0.01%	0.001%
55	8.855	2402	2415	2445	rBV	1079135	1751391	67.41%	9.210%
56	9.035	2469	2471	2473	rBV3	838	523	0.02%	0.003%
57	9.322	2558	2560	2561	rBV2	314	139	0.01%	0.001%
58	9.376	2575	2577	2578	rBV	705	283	0.01%	0.001%
59	9.418	2587	2590	2593	rBV4	550	444	0.02%	0.002%
60	9.444	2596	2598	2602	rVV2	442	227	0.01%	0.001%
61	9.634	2655	2657	2660	rVB2	611	265	0.01%	0.001%
62	9.730	2684	2687	2689	rBV2	516	442	0.02%	0.002%
63	9.759	2693	2696	2698	rVV3	746	509	0.02%	0.003%
64	9.788	2702	2705	2709	rBV2	340	300	0.01%	0.002%
65	9.807	2709	2711	2713	rBV3	432	232	0.01%	0.001%
66	9.933	2744	2750	2751	rBV3	878	784	0.03%	0.004%
67	9.971	2759	2762	2763	rBV	428	280	0.01%	0.001%
68	10.013	2773	2775	2777	rBV	537	192	0.01%	0.001%
69	10.032	2779	2781	2784	rVB3	340	185	0.01%	0.001%
70	10.048	2784	2786	2788	rBV2	413	156	0.01%	0.001%
71	10.068	2788	2792	2798	rBV3	465	508	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019586.D
 Acq On : 13 Dec 2020 04:04
 Operator : SY/MD
 Sample : L4998-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.151	2815	2818	2819	rBV3	564	336	0.01%	0.002%
73	10.177	2824	2826	2827	rBV	626	236	0.01%	0.001%
74	10.219	2827	2839	2860	rBV	739361	1168264	44.97%	6.144%
75	10.370	2884	2886	2888	rBV2	416	224	0.01%	0.001%
76	10.383	2888	2890	2894	rVB2	973	707	0.03%	0.004%
77	10.450	2909	2911	2912	rBV	581	254	0.01%	0.001%
78	10.505	2923	2928	2931	rBV2	561	379	0.01%	0.002%
79	10.621	2963	2964	2966	rBV	521	251	0.01%	0.001%
80	10.714	2991	2993	2996	rBV2	374	205	0.01%	0.001%
81	10.785	3011	3015	3017	rBV3	448	385	0.01%	0.002%
82	10.830	3025	3029	3030	rBV3	844	532	0.02%	0.003%
83	10.965	3068	3071	3074	rBV2	852	491	0.02%	0.003%
84	11.093	3107	3111	3113	rBV2	686	583	0.02%	0.003%
85	11.251	3149	3160	3187	rBV	1076101	1656883	63.78%	8.713%
86	11.489	3231	3234	3237	rBV2	909	529	0.02%	0.003%
87	11.627	3264	3277	3302	rBV	1161361	1791526	68.96%	9.421%
88	12.055	3406	3410	3412	rBV2	669	575	0.02%	0.003%
89	12.096	3420	3423	3426	rBV2	964	831	0.03%	0.004%
90	12.338	3495	3498	3501	rBV3	937	757	0.03%	0.004%
91	12.386	3509	3513	3517	rBV5	948	875	0.03%	0.005%
92	12.540	3560	3561	3562	rBV5	470	135	0.01%	0.001%
93	12.630	3586	3589	3592	rBV3	669	649	0.02%	0.003%
94	13.608	3890	3893	3896	rBV2	774	532	0.02%	0.003%


Sum of corrected areas: 19016005

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121220\
Data File : VV019586.D
Acq On : 13 Dec 2020 04:04
Operator : SY/MD
Sample : L4998-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

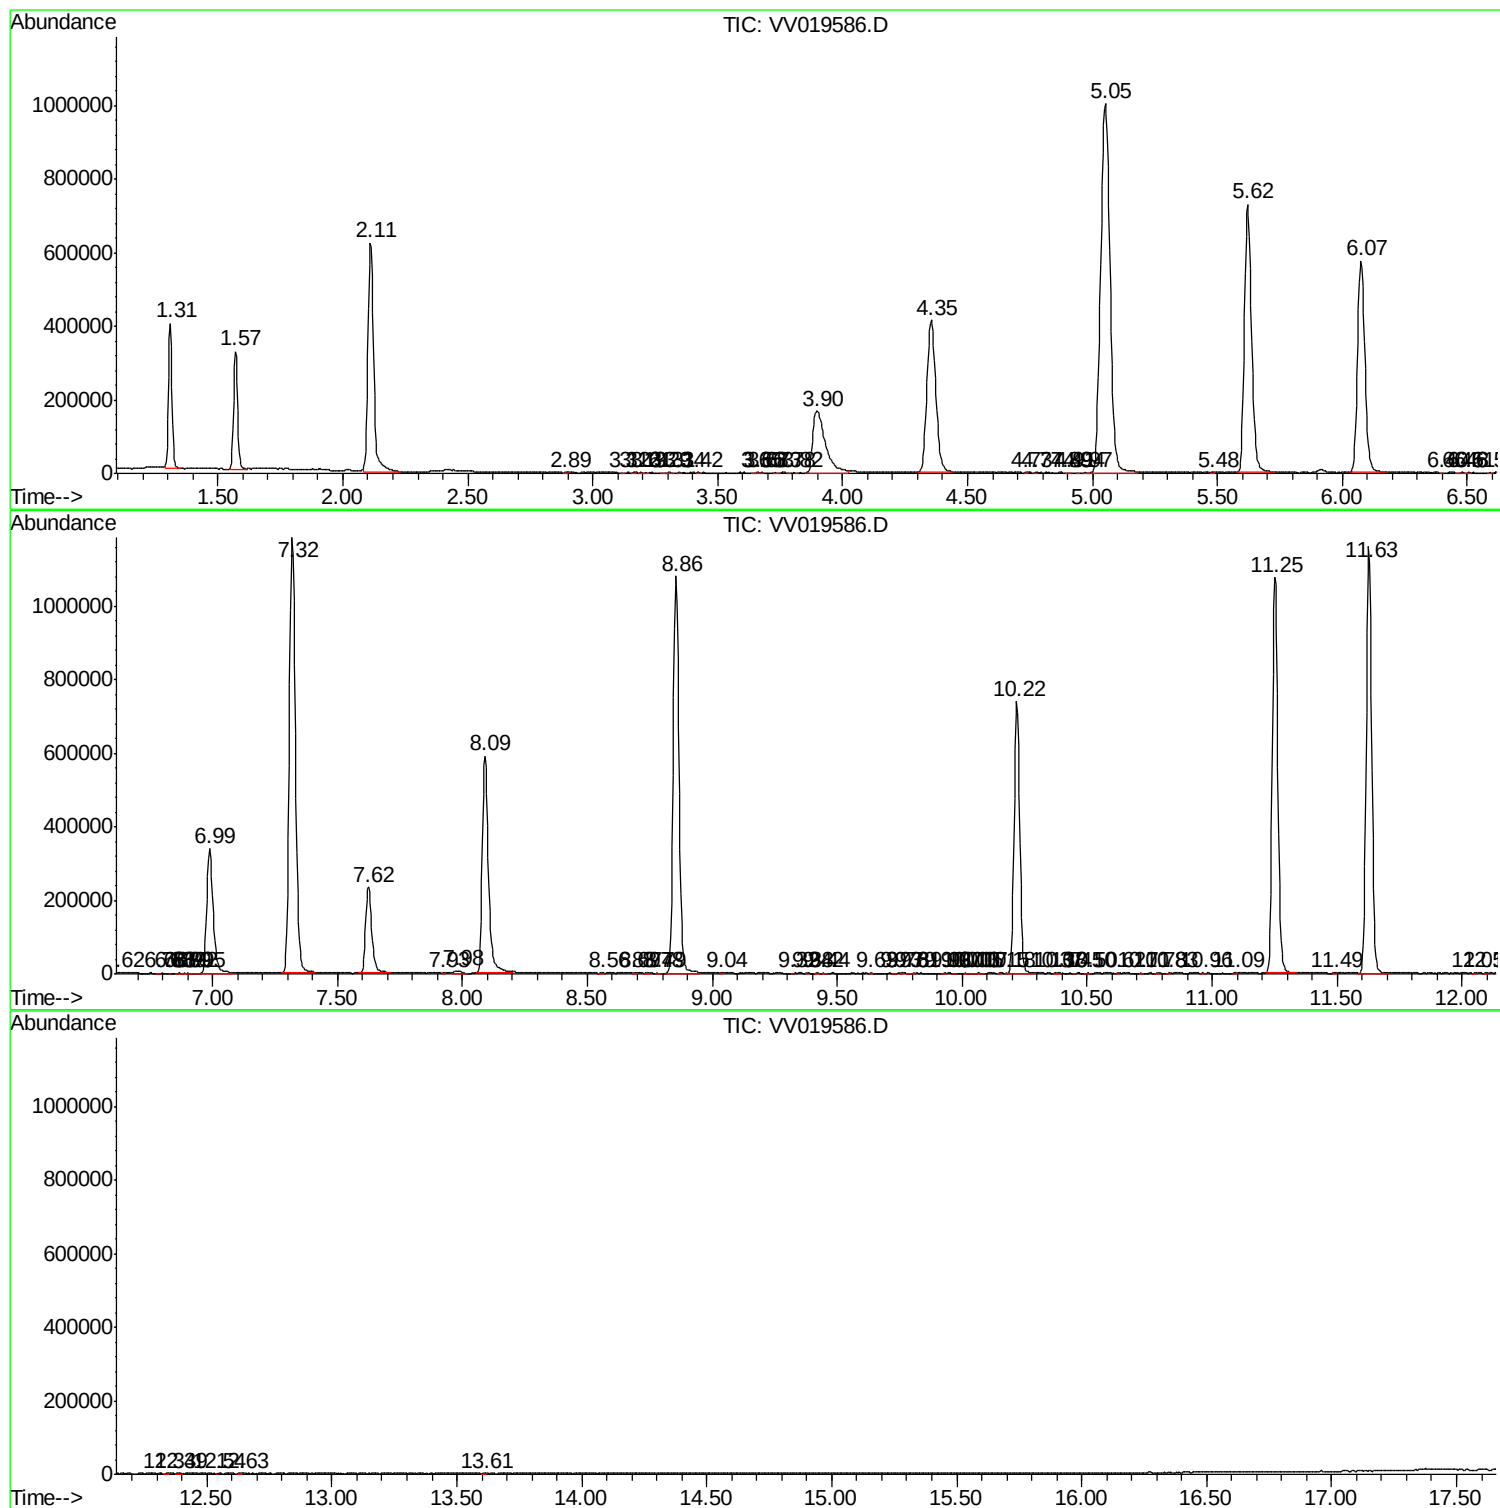

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121220\
Data File : VV019586.D
Acq On : 13 Dec 2020 04:04
Operator : SY/MD
Sample : L4998-16
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AT7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121220\
Data File : VV019586.D
Acq On : 13 Dec 2020 04:04
Operator : SY/MD
Sample : L4998-16
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AT7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc