

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019591.D
 Acq On : 13 Dec 2020 06:04
 Operator : SY/MD
 Sample : L4928-05 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	256639	254643	3.70%	1.125%
2	1.569	143	149	160	rVB	223698	248776	3.61%	1.099%
3	2.110	308	317	347	rVB	428198	676366	9.82%	2.988%
4	2.679	490	494	496	rBV5	815	678	0.01%	0.003%
5	2.955	575	580	583	rBV4	738	895	0.01%	0.004%
6	3.039	602	606	607	rBV2	1248	978	0.01%	0.004%
7	3.216	658	661	664	rBV2	404	335	0.00%	0.001%
8	3.248	668	671	675	rBV4	838	633	0.01%	0.003%
9	3.309	687	690	694	rVB3	584	477	0.01%	0.002%
10	3.325	694	695	696	rBV	451	160	0.00%	0.001%
11	3.370	706	709	711	rBV2	827	574	0.01%	0.003%
12	3.560	765	768	770	rBV2	345	267	0.00%	0.001%
13	3.585	775	776	781	rVB3	392	272	0.00%	0.001%
14	3.611	781	784	785	rBV2	644	325	0.00%	0.001%
15	3.643	791	794	799	rVB4	569	452	0.01%	0.002%
16	3.704	811	813	816	rVB2	368	182	0.00%	0.001%
17	3.727	816	820	822	rBV3	822	688	0.01%	0.003%
18	3.826	847	851	853	rBV3	411	289	0.00%	0.001%
19	3.900	862	874	914	rBV	130514	443270	6.44%	1.958%
20	4.354	998	1015	1044	rBV	337047	833597	12.11%	3.683%
21	4.714	1124	1127	1129	rBV3	436	269	0.00%	0.001%
22	4.859	1169	1172	1175	rBV3	760	438	0.01%	0.002%
23	4.945	1194	1199	1200	rBV3	406	338	0.00%	0.001%
24	4.965	1203	1205	1206	rBV	342	184	0.00%	0.001%
25	5.052	1214	1232	1265	rBV2	793714	2057013	29.87%	9.088%
26	5.524	1377	1379	1383	rBV5	646	439	0.01%	0.002%
27	5.569	1391	1393	1395	rBV	276	151	0.00%	0.001%
28	5.621	1396	1409	1439	rBV	698652	1395992	20.27%	6.168%
29	5.923	1490	1503	1522	rBV5	62438	132926	1.93%	0.587%
30	6.074	1536	1550	1572	rBV	475193	956308	13.89%	4.225%
31	6.344	1631	1634	1637	rBV3	439	296	0.00%	0.001%
32	6.363	1638	1640	1644	rBV4	547	396	0.01%	0.002%
33	6.450	1665	1667	1669	rBV	628	254	0.00%	0.001%
34	6.473	1670	1674	1676	rVV4	759	440	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019591.D
 Acq On : 13 Dec 2020 06:04
 Operator : SY/MD
 Sample : L4928-05 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.502	1681	1683	1684	rBV	346	139	0.00%	0.001%
36	6.547	1694	1697	1703	rVB5	735	475	0.01%	0.002%
37	6.598	1711	1713	1714	rBV	163	57	0.00%	0.000%
38	6.608	1714	1716	1718	rBV2	380	194	0.00%	0.001%
39	6.752	1757	1761	1766	rBV4	744	698	0.01%	0.003%
40	6.797	1773	1775	1777	rBV2	444	278	0.00%	0.001%
41	6.823	1782	1783	1784	rBV2	502	168	0.00%	0.001%
42	6.859	1792	1794	1797	rVB3	405	200	0.00%	0.001%
43	6.881	1797	1801	1803	rBV5	626	480	0.01%	0.002%
44	6.907	1807	1809	1810	rBV	229	85	0.00%	0.000%
45	6.990	1822	1835	1858	rBV	265065	483678	7.02%	2.137%
46	7.318	1925	1937	1961	rBV	872777	1495200	21.71%	6.606%
47	7.624	2022	2032	2061	rBV	186715	325662	4.73%	1.439%
48	7.916	2122	2123	2126	rBV	563	308	0.00%	0.001%
49	7.977	2127	2142	2167	rVV	4131092	6885838	100.00%	30.423%
50	8.090	2168	2177	2208	rVB	517300	889425	12.92%	3.930%
51	8.559	2320	2323	2327	rBV5	743	728	0.01%	0.003%
52	8.736	2376	2378	2379	rBV2	374	147	0.00%	0.001%
53	8.807	2398	2400	2402	rBV	593	251	0.00%	0.001%
54	8.855	2402	2415	2442	rBV	1013451	1634966	23.74%	7.224%
55	9.267	2539	2543	2546	rBV4	860	663	0.01%	0.003%
56	9.363	2569	2573	2574	rBV2	612	462	0.01%	0.002%
57	9.395	2580	2583	2589	rVB3	742	721	0.01%	0.003%
58	9.592	2642	2644	2645	rBV	536	210	0.00%	0.001%
59	9.685	2667	2673	2678	rBV6	924	977	0.01%	0.004%
60	9.736	2684	2689	2690	rBV3	402	315	0.00%	0.001%
61	9.900	2737	2740	2741	rBV2	512	270	0.00%	0.001%
62	9.936	2747	2751	2755	rBV5	576	625	0.01%	0.003%
63	10.055	2784	2788	2790	rBV4	396	313	0.00%	0.001%
64	10.083	2795	2797	2798	rBV	564	266	0.00%	0.001%
65	10.161	2819	2821	2822	rBV	264	123	0.00%	0.001%
66	10.219	2827	2839	2860	rVV	650721	1007329	14.63%	4.451%
67	10.341	2874	2877	2878	rBV2	780	460	0.01%	0.002%
68	10.453	2909	2912	2913	rBV	425	240	0.00%	0.001%
69	10.463	2913	2915	2918	rVV4	624	373	0.01%	0.002%
70	10.482	2918	2921	2924	rVB3	632	400	0.01%	0.002%
71	10.511	2927	2930	2932	rBV4	729	496	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121220\
 Data File : VV019591.D
 Acq On : 13 Dec 2020 06:04
 Operator : SY/MD
 Sample : L4928-05 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.543	2938	2940	2944	rBV3	651	487	0.01%	0.002%
73	10.572	2946	2949	2950	rBV	545	245	0.00%	0.001%
74	10.588	2950	2954	2959	rBV5	885	931	0.01%	0.004%
75	10.849	3029	3035	3037	rBV5	705	846	0.01%	0.004%
76	10.964	3070	3071	3074	rBV3	411	168	0.00%	0.001%
77	11.026	3086	3090	3092	rBV3	593	431	0.01%	0.002%
78	11.209	3143	3147	3149	rBV3	959	688	0.01%	0.003%
79	11.251	3149	3160	3180	rVV	970039	1506034	21.87%	6.654%
80	11.508	3236	3240	3243	rBV3	834	692	0.01%	0.003%
81	11.556	3250	3255	3256	rBV3	639	523	0.01%	0.002%
82	11.627	3263	3277	3303	rBV	883298	1376427	19.99%	6.081%
83	11.807	3330	3333	3334	rBV2	797	539	0.01%	0.002%
84	11.852	3343	3347	3348	rBV2	494	334	0.00%	0.001%
85	12.067	3412	3414	3416	rBV	382	144	0.00%	0.001%
86	12.125	3429	3432	3435	rBV4	608	496	0.01%	0.002%
87	12.283	3478	3481	3482	rBV2	716	363	0.01%	0.002%
88	12.926	3679	3681	3686	rVB4	1023	755	0.01%	0.003%
89	12.961	3686	3692	3696	rBV3	735	1018	0.01%	0.004%
90	13.788	3947	3949	3951	rBV2	643	342	0.00%	0.002%


Sum of corrected areas: 22633984

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121220\
Data File : VV019591.D
Acq On : 13 Dec 2020 06:04
Operator : SY/MD
Sample : L4928-05 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

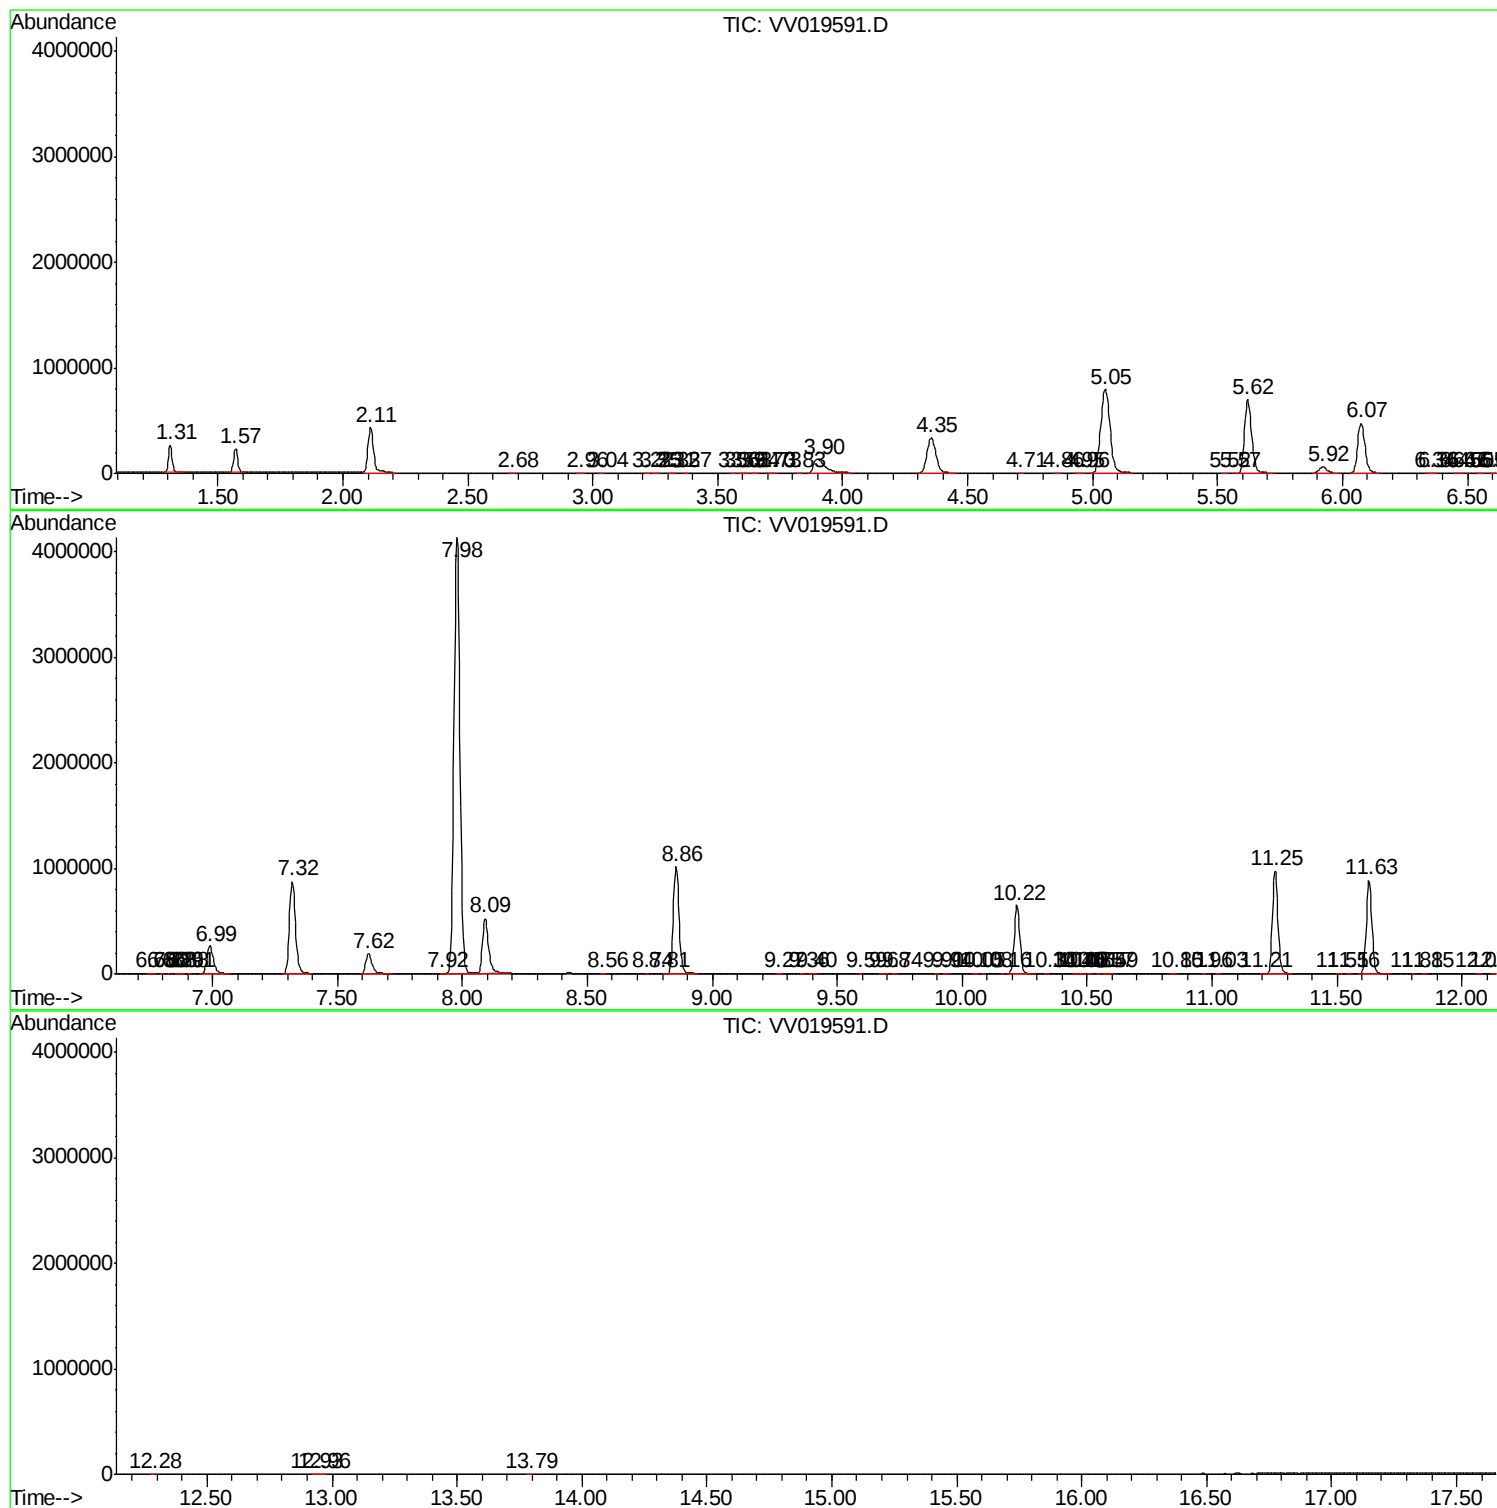

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121220\
Data File : VV019591.D
Acq On : 13 Dec 2020 06:04
Operator : SY/MD
Sample : L4928-05 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121220\
Data File : VV019591.D
Acq On : 13 Dec 2020 06:04
Operator : SY/MD
Sample : L4928-05 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc