


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121220\
 Data File : VV019544.D
 Acq On : 12 Dec 2020 09:27
 Operator : SY/MD
 Sample : BFB64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 14 09:50:38 2020

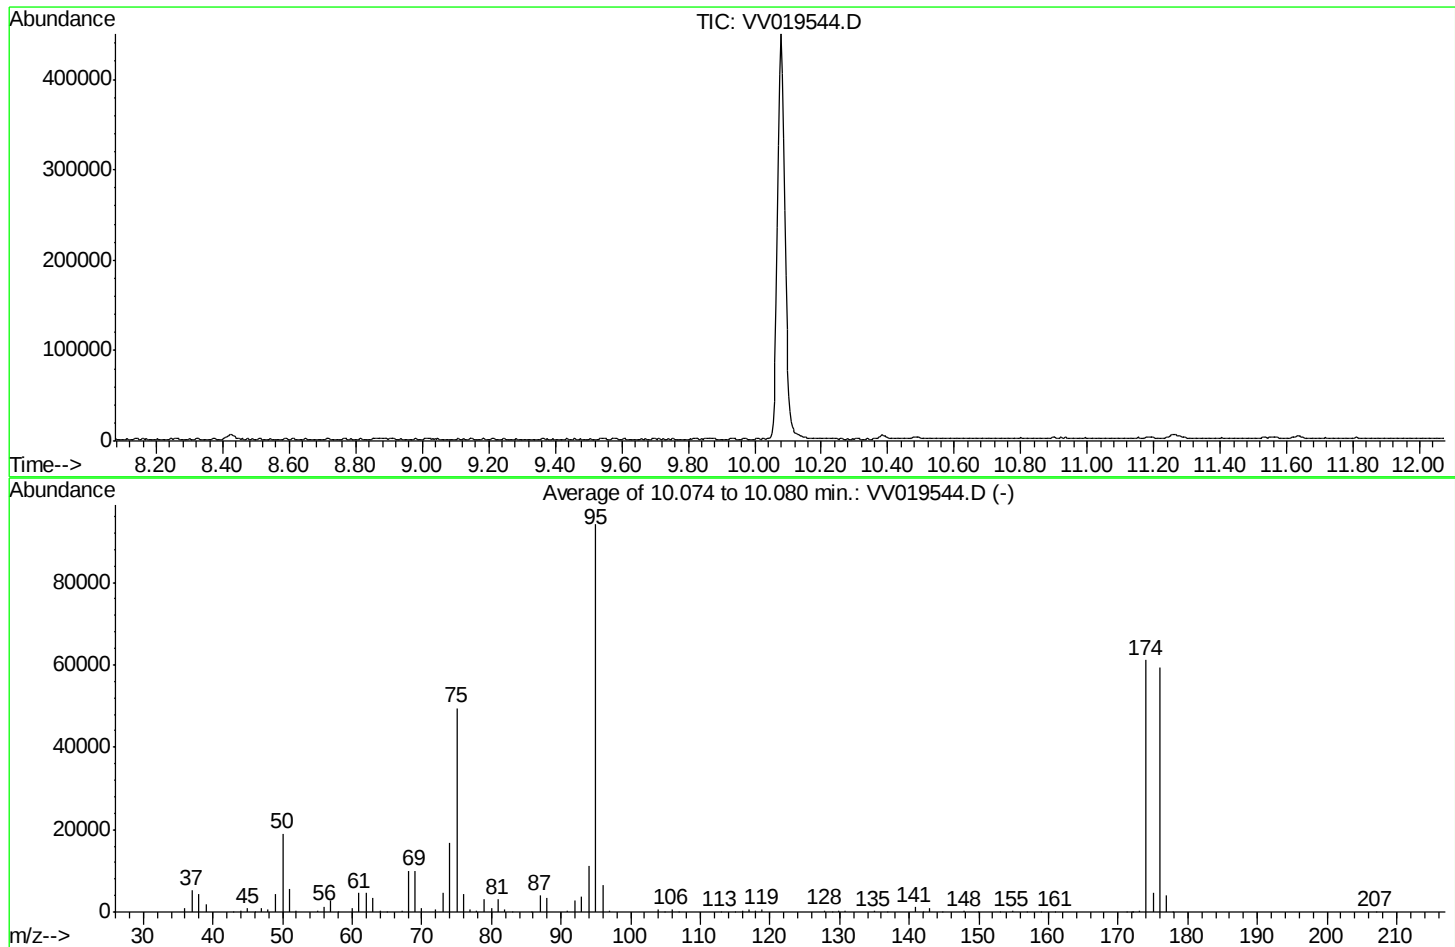

AutoFind: Scans 2794, 2795, 2796; Background Corrected with Scan 2783

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	19042	PASS
75	95	30	80	52.5	49440	PASS
95	95	100	100	100.0	94104	PASS
96	95	5	9	6.8	6390	PASS
173	174	0.00	2	0.5	282	PASS
174	95	50	120	64.9	61082	PASS
175	174	5	9	7.8	4756	PASS
176	174	95	101	97.2	59397	PASS
177	176	5	9	6.8	4034	PASS

m/z	Abundance
36.00	915.0
37.00	4816.0
38.00	3881.0
39.10	1846.0
40.00	342.0
40.90	204.0
42.10	121.0
43.10	178.0
44.00	1543.0
45.00	905.0
46.10	111.0
47.00	1020.0
47.90	596.0
49.00	4116.0
50.00	18256.0
51.00	5599.0
52.00	284.0
54.90	301.0
56.00	1322.0
57.00	2659.0
58.00	161.0
60.00	852.0
61.00	4495.0
62.00	4458.0
63.00	3291.0
64.00	349.0
67.10	260.0
68.00	9263.0
69.00	9458.0
70.00	713.0
72.00	636.0
73.00	4439.0
74.00	15517.0
75.00	46880.0
76.00	4134.0
77.00	679.0
78.00	310.0
78.90	2995.0
80.00	910.0
80.90	2862.0
81.90	638.0
83.10	157.0
86.90	3388.0
87.90	3202.0
91.00	371.0
92.00	2701.0
93.00	3470.0
94.00	10427.0
95.00	88376.0
96.00	6075.0
96.90	139.0
103.90	481.0
104.80	151.0
105.90	488.0
107.00	102.0
112.90	125.0
116.00	350.0
116.90	482.0
117.90	359.0
118.90	627.0
127.90	334.0
128.90	126.0
129.90	337.0
130.80	151.0
135.00	129.0
136.90	133.0
140.80	1079.0
142.00	120.0
142.90	897.0
144.80	111.0
147.90	220.0
154.90	168.0
156.90	117.0
161.00	133.0
172.00	124.0
174.00	54728.0
175.00	4341.0
176.00	54464.0
177.00	3749.0
177.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	1062.0
37.00	5438.0
38.00	4333.0
39.00	1870.0
40.00	317.0
40.90	144.0
43.00	182.0
44.00	1603.0
45.00	922.0
46.10	112.0
47.00	1063.0
48.00	613.0
49.00	4376.0
50.00	19632.0
51.00	5936.0
52.00	258.0
55.00	305.0
56.00	1371.0
57.00	2898.0
58.00	144.0
60.00	854.0
61.00	4781.0
62.00	4818.0
63.00	3507.0
64.00	372.0
64.90	112.0
67.10	283.0
68.00	10174.0
69.00	10347.0
70.00	841.0
72.00	678.0
73.00	4887.0
74.00	17304.0
75.00	51208.0
76.00	4542.0
77.00	748.0
78.00	357.0
78.90	3237.0
79.90	994.0
80.90	3047.0
81.90	747.0
82.90	152.0
86.90	4043.0
87.90	3414.0
90.90	375.0
92.00	2986.0
93.00	3946.0
94.00	11574.0
95.00	97256.0
96.00	6657.0
97.00	176.0
103.90	580.0
104.90	131.0
105.90	598.0
107.00	152.0
112.90	161.0
116.00	374.0
116.90	578.0
117.90	439.0
118.90	615.0
127.90	403.0
128.90	172.0
129.90	389.0
130.80	187.0
135.00	192.0
136.90	169.0
140.80	1202.0
142.00	116.0
142.90	985.0
147.90	226.0
149.90	111.0
153.00	102.0
154.80	194.0
156.90	147.0
160.90	177.0
172.20	153.0
173.10	848.0
174.00	63160.0
175.00	4942.0
176.00	61272.0
177.00	4211.0
177.90	116.0
207.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	1111.0
37.00	5301.0
38.00	4429.0
39.00	1787.0
39.90	278.0
41.00	115.0
43.00	185.0
44.00	1539.0
45.00	833.0
47.00	989.0
48.00	572.0
49.00	4210.0
50.00	19240.0
51.00	5682.0
52.00	237.0
55.00	325.0
56.00	1464.0
57.00	2955.0
57.90	119.0
60.00	855.0
61.00	4686.0
62.00	4577.0
63.00	3321.0
64.00	335.0
64.90	106.0
67.10	273.0
68.00	10235.0
69.00	10303.0
70.00	900.0
72.00	621.0
73.00	4810.0
74.00	17264.0
75.00	50232.0
76.00	4370.0
77.00	685.0
77.80	462.0
78.90	3017.0
79.90	952.0
80.90	3092.0
81.90	743.0
82.90	152.0
85.80	105.0
87.00	4322.0
87.90	3488.0
90.90	404.0
92.00	2912.0
93.00	4072.0
94.00	11222.0
95.00	96680.0
96.00	6439.0
97.10	200.0
103.90	570.0
104.80	115.0
105.90	671.0
106.80	163.0
112.90	158.0
114.90	113.0
116.00	358.0
116.90	640.0
117.90	478.0
118.90	517.0
127.90	407.0
128.90	182.0
129.90	411.0
130.90	199.0
135.00	220.0
136.90	175.0
140.80	1112.0
142.90	975.0
147.90	231.0
149.90	122.0
154.80	227.0
156.90	144.0
158.90	131.0
160.90	185.0
171.20	120.0
172.20	175.0
174.00	65360.0
175.00	4987.0
176.00	62456.0
177.00	4142.0
177.80	105.0
207.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
39.00	102.0
40.10	317.0
40.90	201.0
42.00	130.0
42.90	167.0
43.90	1186.0
52.90	121.0
56.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64