

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121222\
 Data File : VW029598.D
 Acq On : 12 Dec 2022 16:15
 Operator : SY/MD
 Sample : N5915-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N18

Quant Time: Dec 13 03:39:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 13 03:35:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	537946	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	495857	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	251835	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	148505	45.081	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.160%		
7) Chloroethane-d5	1.564	69	119807	47.696	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.400%		
11) 1,1-Dichloroethene-d2	2.105	63	189109	36.806	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.620%		
21) 2-Butanone-d5	3.873	46	174108	86.641	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	86.640%		
24) Chloroform-d	4.339	84	255155	41.161	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.320%		
26) 1,2-Dichloroethane-d4	5.024	65	152625	43.109	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.220%		
32) Benzene-d6	5.043	84	562834	42.957	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.920%		
36) 1,2-Dichloropropane-d6	6.063	67	169230	42.285	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.580%		
41) Toluene-d8	7.307	98	505096	40.914	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.820%		
43) trans-1,3-Dichloroprop...	7.612	79	69875	34.576	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.160%		
47) 2-Hexanone-d5	8.082	63	148389	86.828	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.830%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	230388	40.285	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	80.560%		
66) 1,2-Dichlorobenzene-d4	11.612	152	194637	40.600	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.200%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.982	75	4111	0.741	ug/L	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029598.D
Acq On : 12 Dec 2022 16:15
Operator : SY/MD
Sample : N5915-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N18

Quant Time: Dec 13 03:39:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 13 03:35:01 2022
Response via : Initial Calibration

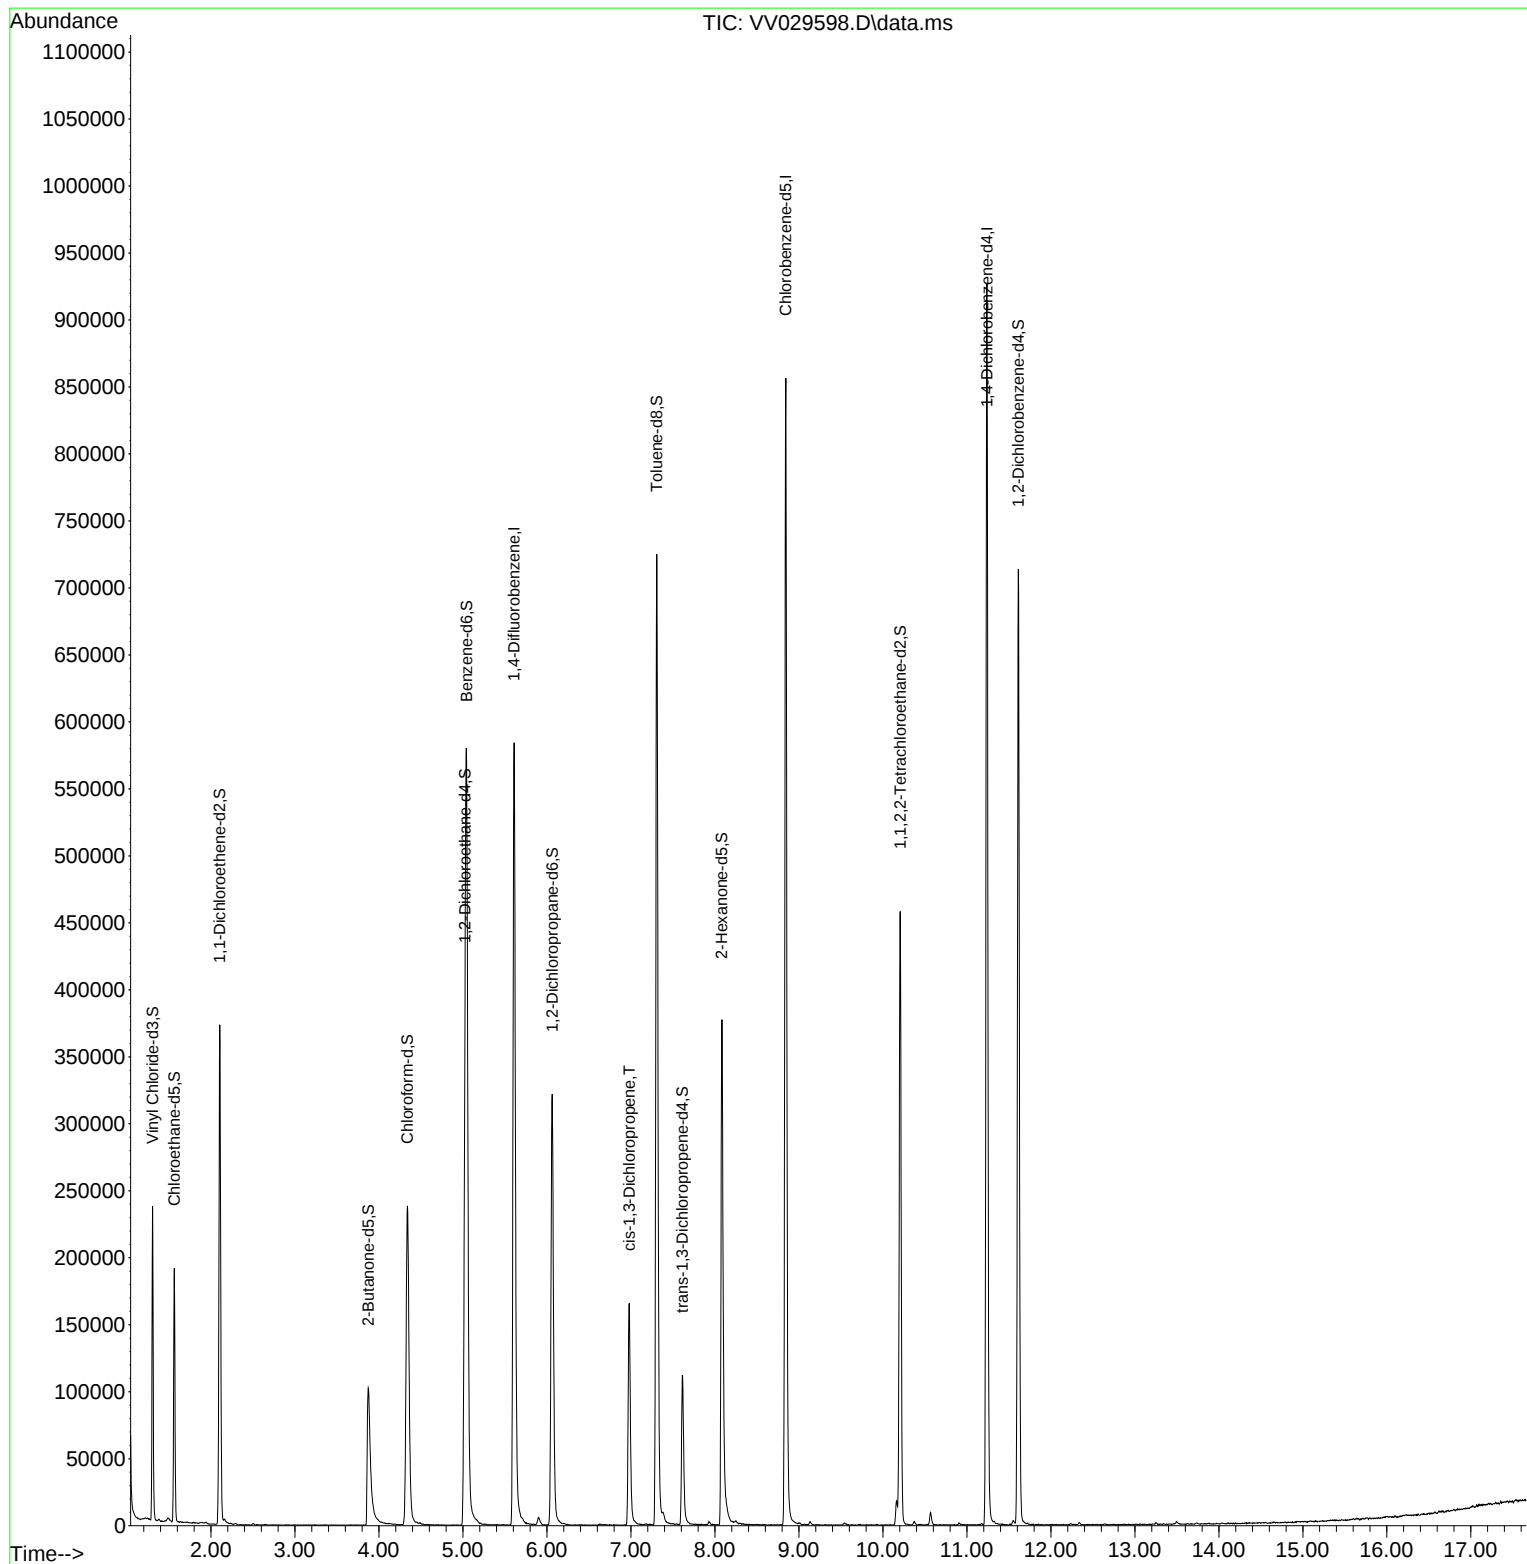

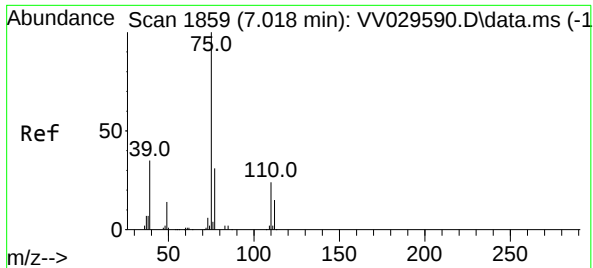

#39
 cis-1,3-Dichloropropene
 Concen: 0.741 ug/L
 RT: 6.982 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VV029598.D
 Acq: 12 Dec 2022 16:15

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N18

Tgt Ion: 75 Resp: 4111
 Ion Ratio Lower Upper
 75 100
 77 52.5 21.9 40.7#

