

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121222\
 Data File : VW029603.D
 Acq On : 12 Dec 2022 18:11
 Operator : SY/MD
 Sample : N5950-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF49

Quant Time: Dec 13 03:40:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 13 03:35:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	449338	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	414131	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	213986	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	120992	43.972	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.940%
7) Chloroethane-d5	1.564	69	104311	49.716	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.440%
11) 1,1-Dichloroethene-d2	2.104	63	162142	37.781	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.560%
21) 2-Butanone-d5	3.866	46	171578	102.220	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.220%
24) Chloroform-d	4.339	84	241951	46.728	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.460%
26) 1,2-Dichloroethane-d4	5.024	65	147659	49.931	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.860%
32) Benzene-d6	5.043	84	517662	47.306	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.620%
36) 1,2-Dichloropropane-d6	6.063	67	161135	48.208	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.420%
41) Toluene-d8	7.307	98	464286	45.030	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.060%
43) trans-1,3-Dichloroprop...	7.612	79	65272	38.672	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.340%
47) 2-Hexanone-d5	8.082	63	142594	99.903	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.900%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	225323	47.174	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.340%
66) 1,2-Dichlorobenzene-d4	11.612	152	188431	46.258	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.520%
Target Compounds						
39) cis-1,3-Dichloropropene	6.979	75	3856	0.832	ug/L	Qvalue # 32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029603.D
Acq On : 12 Dec 2022 18:11
Operator : SY/MD
Sample : N5950-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF49

Quant Time: Dec 13 03:40:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 13 03:35:01 2022
Response via : Initial Calibration

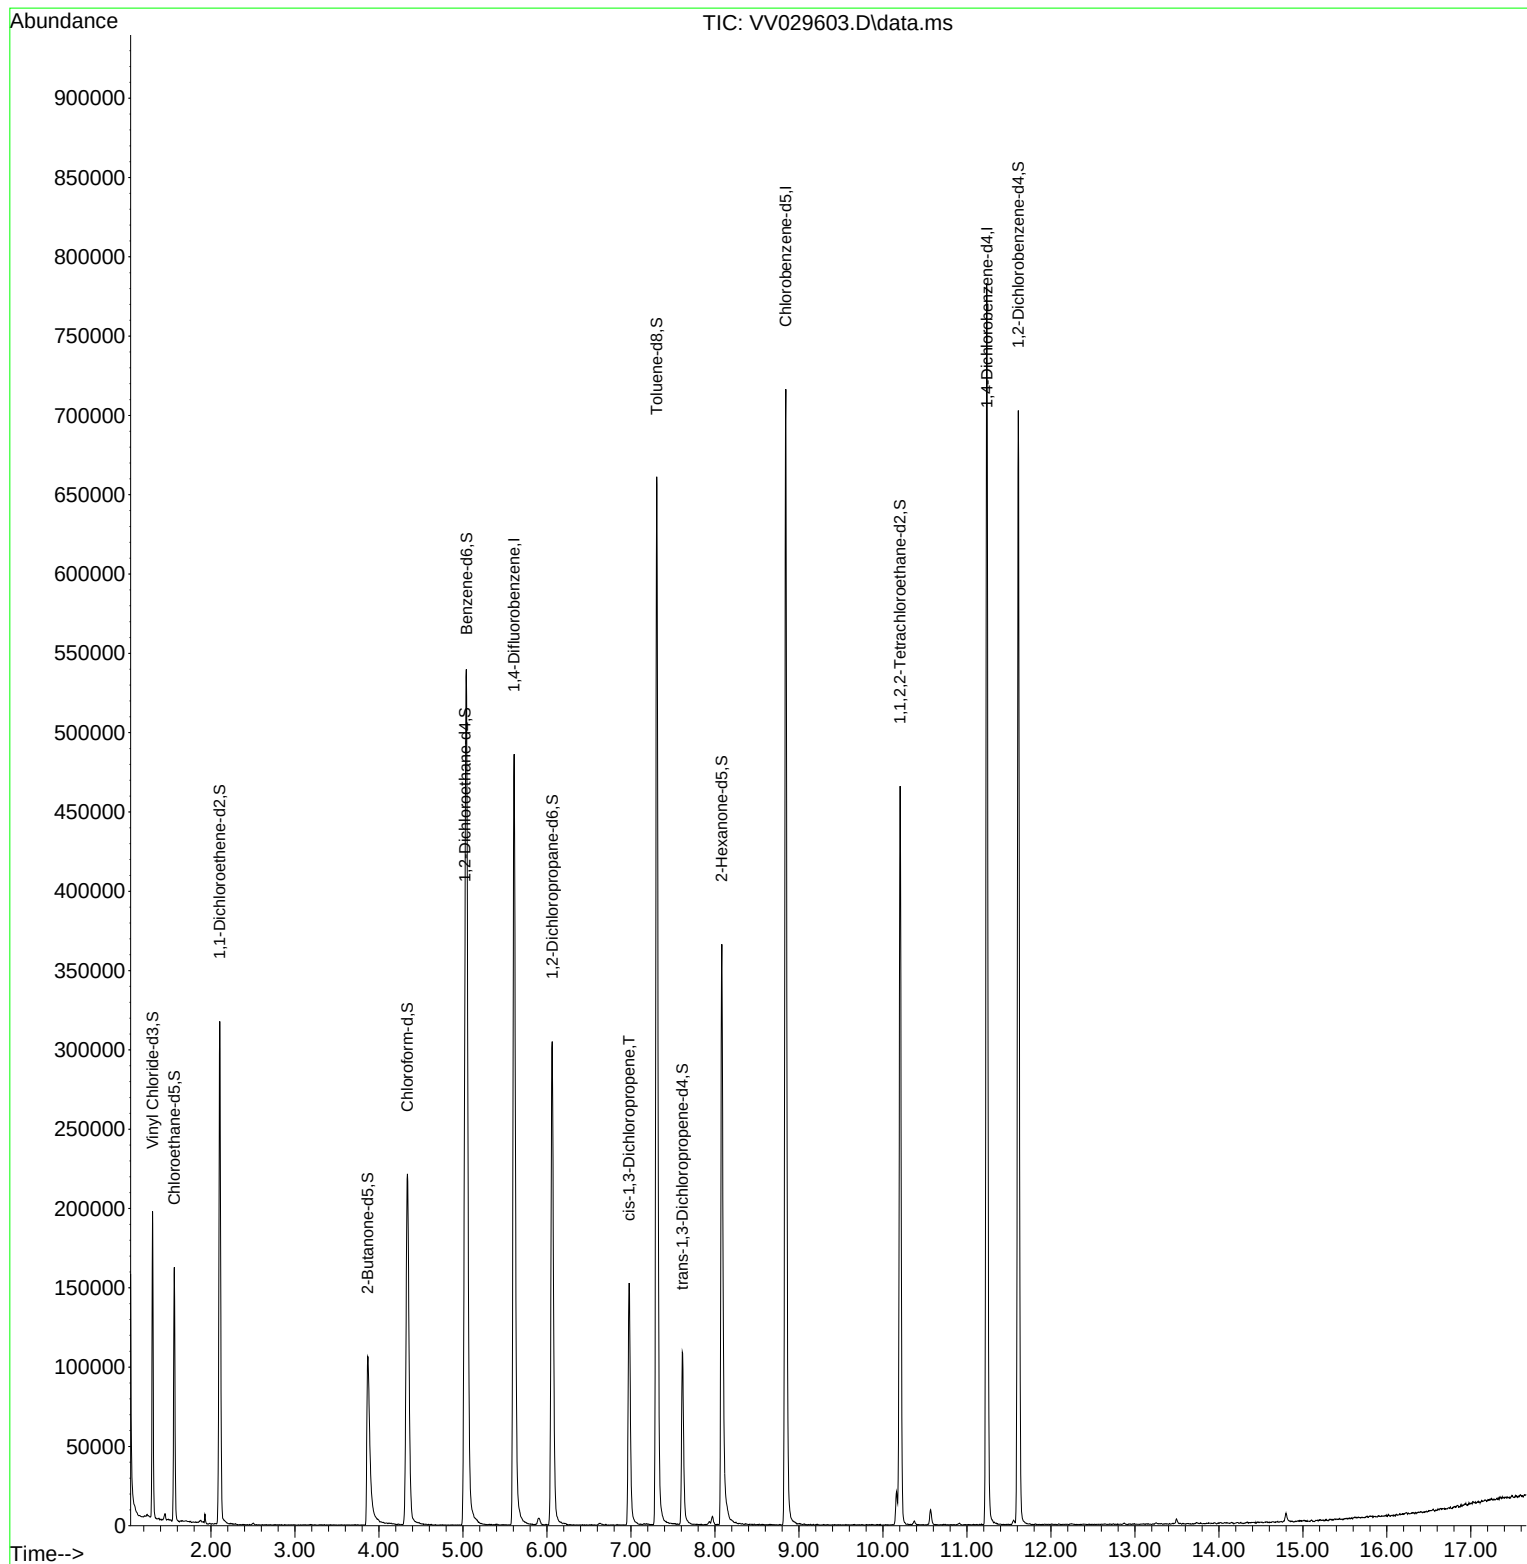

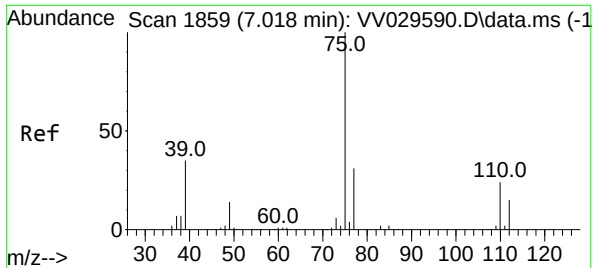

#39

cis-1,3-Dichloropropene

Concen: 0.832 ug/L

RT: 6.979 min Scan# 11

Delta R.T. -0.039 min

Lab File: VV029603.D

Acq: 12 Dec 2022 18:11

Instrument :

MSVOA_V

ClientSampleId :

EYF49

Tgt Ion: 75 Resp: 3856

Ion Ratio Lower Upper

75 100

77 68.6 21.9 40.7#

