

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
 Data File : VV029591.D
 Acq On : 12 Dec 2022 13:31
 Operator : SY/MD
 Sample : VV1212WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029591.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	235568	228590	14.12%	1.736%
2	1.564	155	163	178	rVB	185707	210441	12.99%	1.598%
3	2.105	320	331	345	rBV	360633	518782	32.03%	3.940%
4	2.503	447	455	467	rVB3	4475	7284	0.45%	0.055%
5	2.764	528	536	551	rVB8	3090	5463	0.34%	0.041%
6	2.899	574	578	582	rVB2	285	275	0.02%	0.002%
7	2.931	585	588	592	rVV3	262	215	0.01%	0.002%
8	2.950	592	594	596	rVB2	242	109	0.01%	0.001%
9	3.053	623	626	627	rBV	269	147	0.01%	0.001%
10	3.127	646	649	653	rBV3	232	152	0.01%	0.001%
11	3.166	659	661	662	rBV3	308	113	0.01%	0.001%
12	3.259	688	690	693	rVB	290	120	0.01%	0.001%
13	3.297	696	702	707	rBV2	187	269	0.02%	0.002%
14	3.394	729	732	737	rVB	254	170	0.01%	0.001%
15	3.506	761	767	770	rBV	336	349	0.02%	0.003%
16	3.539	773	777	781	rVV2	234	195	0.01%	0.001%
17	3.596	792	795	799	rVB2	269	192	0.01%	0.001%
18	3.632	804	806	810	rVB2	207	129	0.01%	0.001%
19	3.696	823	826	830	rBV2	193	132	0.01%	0.001%
20	3.744	838	841	846	rVB	217	147	0.01%	0.001%
21	3.776	846	851	856	rBV2	348	299	0.02%	0.002%
22	3.870	870	880	932	rBV	121418	365753	22.58%	2.778%
23	4.336	1010	1025	1055	rBV	245874	608816	37.59%	4.624%
24	4.580	1099	1101	1106	rBV3	472	423	0.03%	0.003%
25	4.706	1139	1140	1144	rBV	211	141	0.01%	0.001%
26	4.725	1144	1146	1148	rVV2	236	150	0.01%	0.001%
27	4.796	1166	1168	1170	rBV3	293	180	0.01%	0.001%
28	4.815	1170	1174	1176	rBV	394	345	0.02%	0.003%
29	4.915	1202	1205	1207	rBV	175	119	0.01%	0.001%
30	5.037	1224	1243	1289	rBV2	609636	1619451	100.00%	12.299%
31	5.606	1406	1420	1460	rBV	531233	1097227	67.75%	8.333%
32	5.899	1502	1511	1512	rBV4	5817	6504	0.40%	0.049%
33	6.059	1548	1561	1590	rBV	340670	712597	44.00%	5.412%
34	6.307	1635	1638	1643	rBV2	257	227	0.01%	0.002%
35	6.391	1660	1664	1667	rBV2	152	127	0.01%	0.001%
36	6.506	1694	1700	1707	rBV3	651	971	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
 Data File : VV029591.D
 Acq On : 12 Dec 2022 13:31
 Operator : SY/MD
 Sample : VV1212WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.535	1707	1709	1712	rVB2	358	152	0.01%	0.001%
38	6.564	1712	1718	1721	rBV	240	231	0.01%	0.002%
39	6.625	1730	1737	1740	rBV3	990	1085	0.07%	0.008%
40	6.702	1758	1761	1764	rVB2	281	177	0.01%	0.001%
41	6.796	1786	1790	1793	rBV	208	229	0.01%	0.002%
42	6.834	1798	1802	1804	rBV2	486	319	0.02%	0.002%
43	6.915	1824	1827	1830	rVB	368	226	0.01%	0.002%
44	6.931	1830	1832	1834	rBV	219	137	0.01%	0.001%
45	6.979	1834	1847	1878	rBV	177826	329585	20.35%	2.503%
46	7.233	1920	1926	1934	rVB5	2142	3585	0.22%	0.027%
47	7.307	1937	1949	1987	rVV	760907	1337835	82.61%	10.160%
48	7.612	2034	2044	2067	rBV	124217	222127	13.72%	1.687%
49	7.770	2092	2093	2096	rBV2	289	160	0.01%	0.001%
50	7.837	2109	2114	2115	rBV3	1352	1067	0.07%	0.008%
51	7.892	2128	2131	2133	rBV2	364	280	0.02%	0.002%
52	7.969	2149	2155	2164	rVB6	2011	2956	0.18%	0.022%
53	8.082	2180	2190	2225	rBV	432084	776442	47.94%	5.897%
54	8.577	2341	2344	2346	rBV2	340	224	0.01%	0.002%
55	8.638	2359	2363	2365	rBV3	328	264	0.02%	0.002%
56	8.699	2379	2382	2384	rBV2	278	208	0.01%	0.002%
57	8.844	2413	2427	2455	rBV	789574	1315849	81.25%	9.993%
58	9.011	2471	2479	2489	rVB3	3604	6083	0.38%	0.046%
59	9.136	2512	2518	2529	rVB4	3090	4952	0.31%	0.038%
60	9.204	2534	2539	2546	rVB2	388	431	0.03%	0.003%
61	9.239	2546	2550	2552	rBV2	279	217	0.01%	0.002%
62	9.271	2557	2560	2562	rBV	176	107	0.01%	0.001%
63	9.345	2580	2583	2584	rBV	257	135	0.01%	0.001%
64	9.455	2613	2617	2619	rBV2	225	156	0.01%	0.001%
65	9.542	2634	2644	2645	rBV2	3977	4771	0.29%	0.036%
66	9.657	2678	2680	2684	rVB	381	222	0.01%	0.002%
67	9.696	2688	2692	2694	rBV4	390	273	0.02%	0.002%
68	9.722	2696	2700	2702	rBV3	652	495	0.03%	0.004%
69	9.767	2712	2714	2717	rBV2	351	200	0.01%	0.002%
70	9.837	2733	2736	2738	rBV	153	105	0.01%	0.001%
71	9.879	2746	2749	2753	rBV4	300	294	0.02%	0.002%
72	9.921	2753	2762	2773	rVB2	4022	6116	0.38%	0.046%
73	10.001	2783	2787	2791	rBV3	279	236	0.01%	0.002%
74	10.043	2798	2800	2802	rBV	242	116	0.01%	0.001%
75	10.072	2807	2809	2812	rBV	227	122	0.01%	0.001%
76	10.162	2826	2837	2841	rVV	24015	35472	2.19%	0.269%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
 Data File : VV029591.D
 Acq On : 12 Dec 2022 13:31
 Operator : SY/MD
 Sample : VV1212WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.207	2842	2851	2879	rVV	511873	810833	50.07%	6.158%
78	10.304	2879	2881	2882	rVB	467	107	0.01%	0.001%
79	10.361	2895	2899	2901	rBV	302	207	0.01%	0.002%
80	10.377	2901	2904	2908	rBV	233	212	0.01%	0.002%
81	10.435	2920	2922	2925	rBV2	243	141	0.01%	0.001%
82	10.532	2944	2952	2955	rBV2	4111	4956	0.31%	0.038%
83	10.789	3030	3032	3034	rBV	255	116	0.01%	0.001%
84	10.847	3047	3050	3052	rBV3	290	176	0.01%	0.001%
85	10.905	3061	3068	3078	rVB4	4649	6473	0.40%	0.049%
86	10.982	3090	3092	3098	rVB2	300	249	0.02%	0.002%
87	11.175	3144	3152	3160	rBV3	6512	9685	0.60%	0.074%
88	11.236	3160	3171	3198	rBV	902456	1406618	86.86%	10.683%
89	11.422	3227	3229	3232	rBV4	374	218	0.01%	0.002%
90	11.612	3276	3288	3310	rBV	820808	1282148	79.17%	9.737%
91	11.840	3357	3359	3364	rBV4	348	248	0.02%	0.002%
92	12.336	3509	3513	3514	rBV2	316	177	0.01%	0.001%
93	12.384	3526	3528	3531	rVB	304	138	0.01%	0.001%
94	12.413	3531	3537	3551	rBV6	1964	3454	0.21%	0.026%
95	12.631	3598	3605	3617	rBV2	9880	14339	0.89%	0.109%
96	12.773	3647	3649	3651	rBV	328	176	0.01%	0.001%
97	13.249	3788	3797	3814	rBV2	17492	26967	1.67%	0.205%
98	13.323	3818	3820	3822	rBV2	531	296	0.02%	0.002%
99	13.493	3866	3873	3895	rVB	79010	127728	7.89%	0.970%
100	13.731	3939	3947	3958	rVB2	20571	31302	1.93%	0.238%

Sum of corrected areas: 13167209




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029591.D
Acq On : 12 Dec 2022 13:31
Operator : SY/MD
Sample : VV1212WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

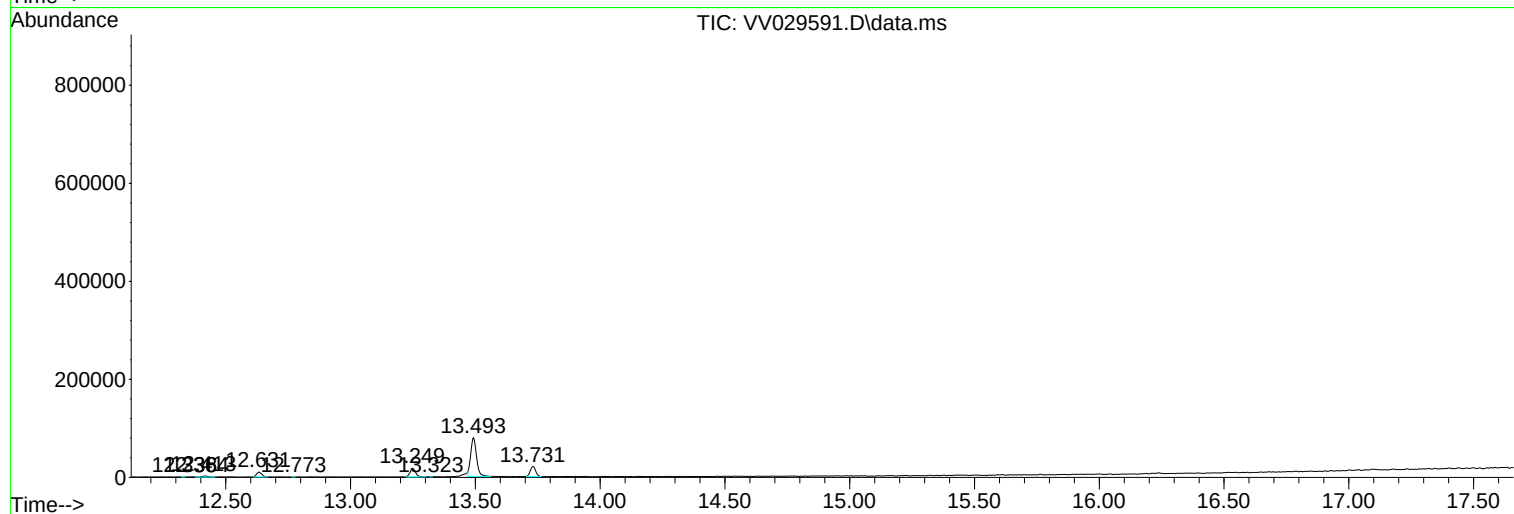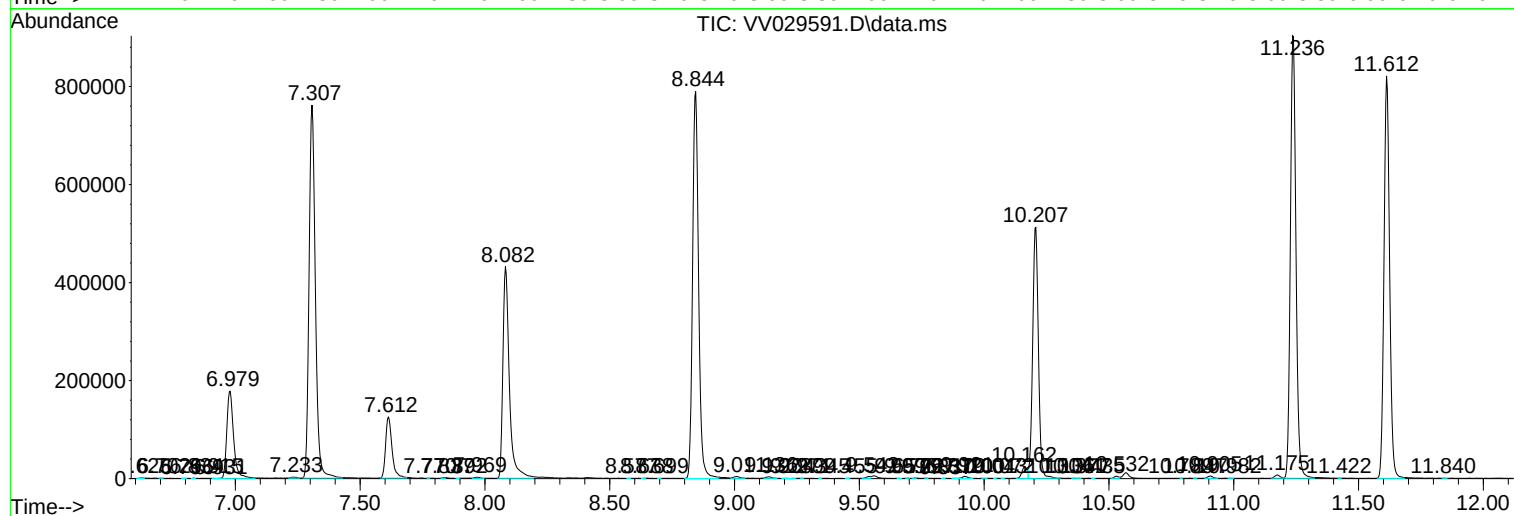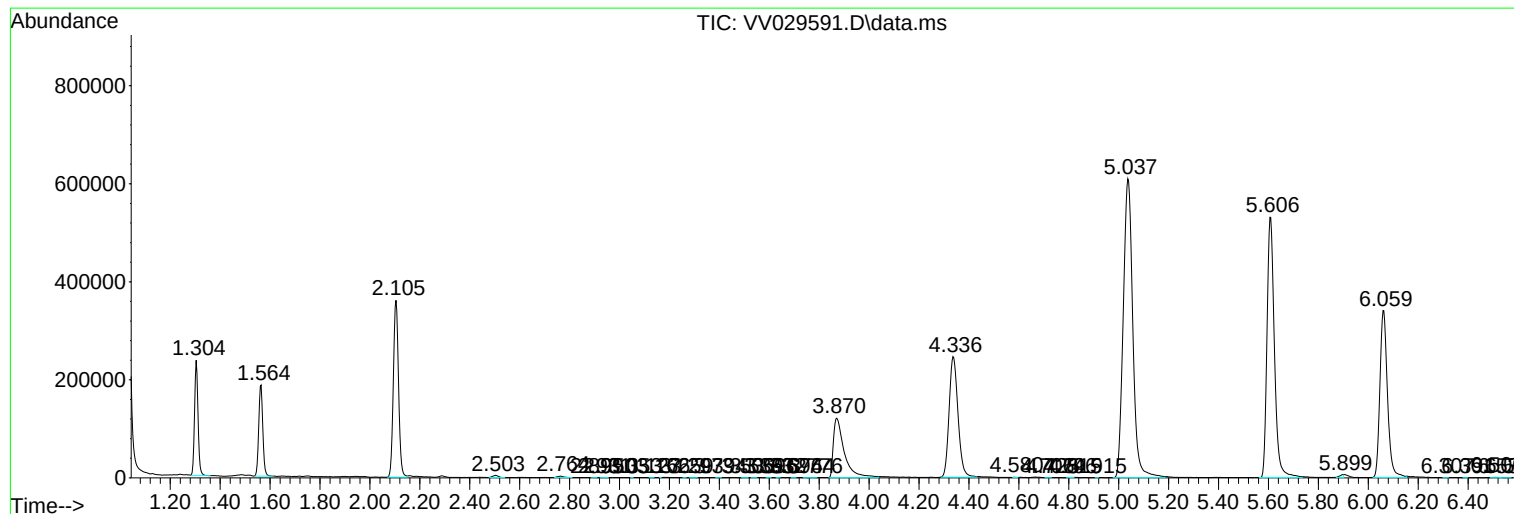

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029591.D
Acq On : 12 Dec 2022 13:31
Operator : SY/MD
Sample : VV1212WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029591.D
Acq On : 12 Dec 2022 13:31
Operator : SY/MD
Sample : VV1212WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc