

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
 Data File : VV029592.D
 Acq On : 12 Dec 2022 13:54
 Operator : SY/MD
 Sample : N5929-15DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB2	288818	302193	18.82%	1.920%
2	1.561	155	162	179	rVB2	185418	269000	16.75%	1.709%
3	2.105	320	331	348	rBV	354055	513061	31.95%	3.259%
4	2.468	441	444	445	rVB3	290	165	0.01%	0.001%
5	2.503	445	455	470	rVB2	12870	21466	1.34%	0.136%
6	2.680	507	510	512	rBV	111	73	0.00%	0.000%
7	2.761	524	535	550	rBV2	13486	24371	1.52%	0.155%
8	2.899	575	578	581	rBV2	411	322	0.02%	0.002%
9	3.111	642	644	646	rBV	111	58	0.00%	0.000%
10	3.182	651	666	699	rVV	439541	926960	57.72%	5.889%
11	3.468	751	755	762	rBV3	321	369	0.02%	0.002%
12	3.532	773	775	777	rBV	186	105	0.01%	0.001%
13	3.581	788	790	792	rVB2	178	54	0.00%	0.000%
14	3.626	802	804	805	rBV	157	72	0.00%	0.000%
15	3.696	823	826	829	rVB	279	174	0.01%	0.001%
16	3.757	842	845	848	rBV2	247	212	0.01%	0.001%
17	3.902	870	890	924	rBV2	498624	1474046	91.79%	9.364%
18	4.339	1009	1026	1051	rBV2	247438	609917	37.98%	3.875%
19	4.603	1098	1108	1128	rVB3	9235	22968	1.43%	0.146%
20	4.703	1137	1139	1141	rBV2	229	91	0.01%	0.001%
21	4.744	1150	1152	1154	rVB	222	94	0.01%	0.001%
22	4.767	1154	1159	1160	rBV2	207	115	0.01%	0.001%
23	4.780	1160	1163	1166	rVV	143	102	0.01%	0.001%
24	4.844	1181	1183	1184	rBV	155	55	0.00%	0.000%
25	4.876	1190	1193	1196	rBV2	148	92	0.01%	0.001%
26	4.892	1196	1198	1203	rVB3	177	166	0.01%	0.001%
27	4.934	1209	1211	1213	rBV2	141	62	0.00%	0.000%
28	5.040	1225	1244	1300	rBV2	606119	1605966	100.00%	10.202%
29	5.381	1344	1350	1351	rBV	374	304	0.02%	0.002%
30	5.429	1363	1365	1367	rVB	251	97	0.01%	0.001%
31	5.535	1396	1398	1399	rBV	161	65	0.00%	0.000%
32	5.609	1408	1421	1459	rBV	566904	1159468	72.20%	7.366%
33	5.912	1504	1515	1531	rVB4	19766	42510	2.65%	0.270%
34	6.063	1547	1562	1587	rBV	340449	703412	43.80%	4.468%
35	6.288	1630	1632	1635	rVB	118	63	0.00%	0.000%
36	6.301	1635	1636	1640	rVB	269	144	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121222\
 Data File : VW029592.D
 Acq On : 12 Dec 2022 13:54
 Operator : SY/MD
 Sample : N5929-15DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.330	1640	1645	1647	rBV2	320	188	0.01%	0.001%
38	6.381	1659	1661	1664	rVB2	223	132	0.01%	0.001%
39	6.397	1664	1666	1668	rBV	84	51	0.00%	0.000%
40	6.413	1668	1671	1674	rVV2	285	173	0.01%	0.001%
41	6.429	1674	1676	1680	rBV2	192	112	0.01%	0.001%
42	6.468	1685	1688	1690	rBV	140	95	0.01%	0.001%
43	6.580	1719	1723	1724	rBV	167	139	0.01%	0.001%
44	6.613	1730	1733	1734	rBV2	902	452	0.03%	0.003%
45	6.706	1759	1762	1766	rVB	316	217	0.01%	0.001%
46	6.732	1766	1770	1771	rBV2	190	146	0.01%	0.001%
47	6.757	1776	1778	1779	rBV	121	49	0.00%	0.000%
48	6.815	1791	1796	1798	rBV2	326	237	0.01%	0.002%
49	6.850	1803	1807	1808	rVB	198	106	0.01%	0.001%
50	6.863	1808	1811	1812	rBV	213	101	0.01%	0.001%
51	6.895	1819	1821	1823	rBV	181	110	0.01%	0.001%
52	6.934	1831	1833	1835	rVB	386	86	0.01%	0.001%
53	6.979	1835	1847	1873	rBV	175226	319198	19.88%	2.028%
54	7.223	1919	1923	1927	rBV4	813	898	0.06%	0.006%
55	7.310	1936	1950	1968	rBV	754630	1317667	82.05%	8.371%
56	7.613	2034	2044	2074	rBV	121139	216199	13.46%	1.373%
57	7.831	2107	2112	2126	rBV6	3290	5555	0.35%	0.035%
58	7.924	2139	2141	2142	rBV2	555	235	0.01%	0.001%
59	8.082	2180	2190	2230	rBV	434321	777213	48.40%	4.937%
60	8.516	2323	2325	2328	rBV2	452	204	0.01%	0.001%
61	8.551	2334	2336	2339	rBV2	332	269	0.02%	0.002%
62	8.651	2365	2367	2373	rVB2	451	374	0.02%	0.002%
63	8.677	2373	2375	2376	rBV2	178	70	0.00%	0.000%
64	8.693	2376	2380	2384	rBV3	331	381	0.02%	0.002%
65	8.796	2408	2412	2414	rBV2	270	199	0.01%	0.001%
66	8.844	2414	2427	2454	rBV	835023	1365730	85.04%	8.676%
67	9.130	2509	2516	2534	rVB2	8599	15207	0.95%	0.097%
68	9.194	2534	2536	2538	rBV2	293	171	0.01%	0.001%
69	9.246	2549	2552	2554	rBV2	176	93	0.01%	0.001%
70	9.262	2554	2557	2559	rVV2	417	175	0.01%	0.001%
71	9.275	2559	2561	2564	rVV2	154	80	0.00%	0.001%
72	9.291	2564	2566	2569	rVB	432	195	0.01%	0.001%
73	9.310	2569	2572	2575	rBV	100	83	0.01%	0.001%
74	9.336	2577	2580	2583	rBV	214	177	0.01%	0.001%
75	9.407	2599	2602	2605	rVB	254	132	0.01%	0.001%
76	9.535	2632	2642	2661	rBV2	47258	78197	4.87%	0.497%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121222\
 Data File : VW029592.D
 Acq On : 12 Dec 2022 13:54
 Operator : SY/MD
 Sample : N5929-15DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.767	2711	2714	2716	rBV2	217	109	0.01%	0.001%
78	9.783	2716	2719	2722	rBV	202	172	0.01%	0.001%
79	9.924	2756	2763	2773	rVB2	2592	4033	0.25%	0.026%
80	9.992	2780	2784	2785	rBV	180	113	0.01%	0.001%
81	10.114	2820	2822	2823	rBV	188	78	0.00%	0.000%
82	10.162	2827	2837	2841	rBV2	23546	34966	2.18%	0.222%
83	10.207	2842	2851	2876	rVB	503056	802608	49.98%	5.099%
84	10.342	2888	2893	2905	rVB	3427	5192	0.32%	0.033%
85	10.439	2915	2923	2940	rVB2	17325	27803	1.73%	0.177%
86	10.529	2943	2951	2957	rBV2	12382	17747	1.11%	0.113%
87	10.683	2995	2999	3003	rBV2	612	561	0.03%	0.004%
88	10.728	3003	3013	3023	rVV	20896	31737	1.98%	0.202%
89	10.905	3058	3068	3087	rBV	51594	78169	4.87%	0.497%
90	11.037	3107	3109	3110	rBV	156	66	0.00%	0.000%
91	11.111	3129	3132	3134	rBV2	329	211	0.01%	0.001%
92	11.175	3145	3152	3160	rBV5	2351	3501	0.22%	0.022%
93	11.236	3160	3171	3190	rVV	952056	1478492	92.06%	9.392%
94	11.323	3192	3198	3217	rVB	41423	65727	4.09%	0.418%
95	11.519	3248	3259	3270	rBV	15017	24016	1.50%	0.153%
96	11.612	3277	3288	3308	rBV	809028	1291178	80.40%	8.202%
97	11.911	3371	3381	3395	rBV	23357	42378	2.64%	0.269%
98	12.458	3544	3551	3556	rBV2	1830	2466	0.15%	0.016%
99	12.870	3670	3679	3686	rBV5	3404	4786	0.30%	0.030%
100	13.493	3862	3873	3886	rBV	27697	46022	2.87%	0.292%


Sum of corrected areas: 15741619

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029592.D
Acq On : 12 Dec 2022 13:54
Operator : SY/MD
Sample : N5929-15DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

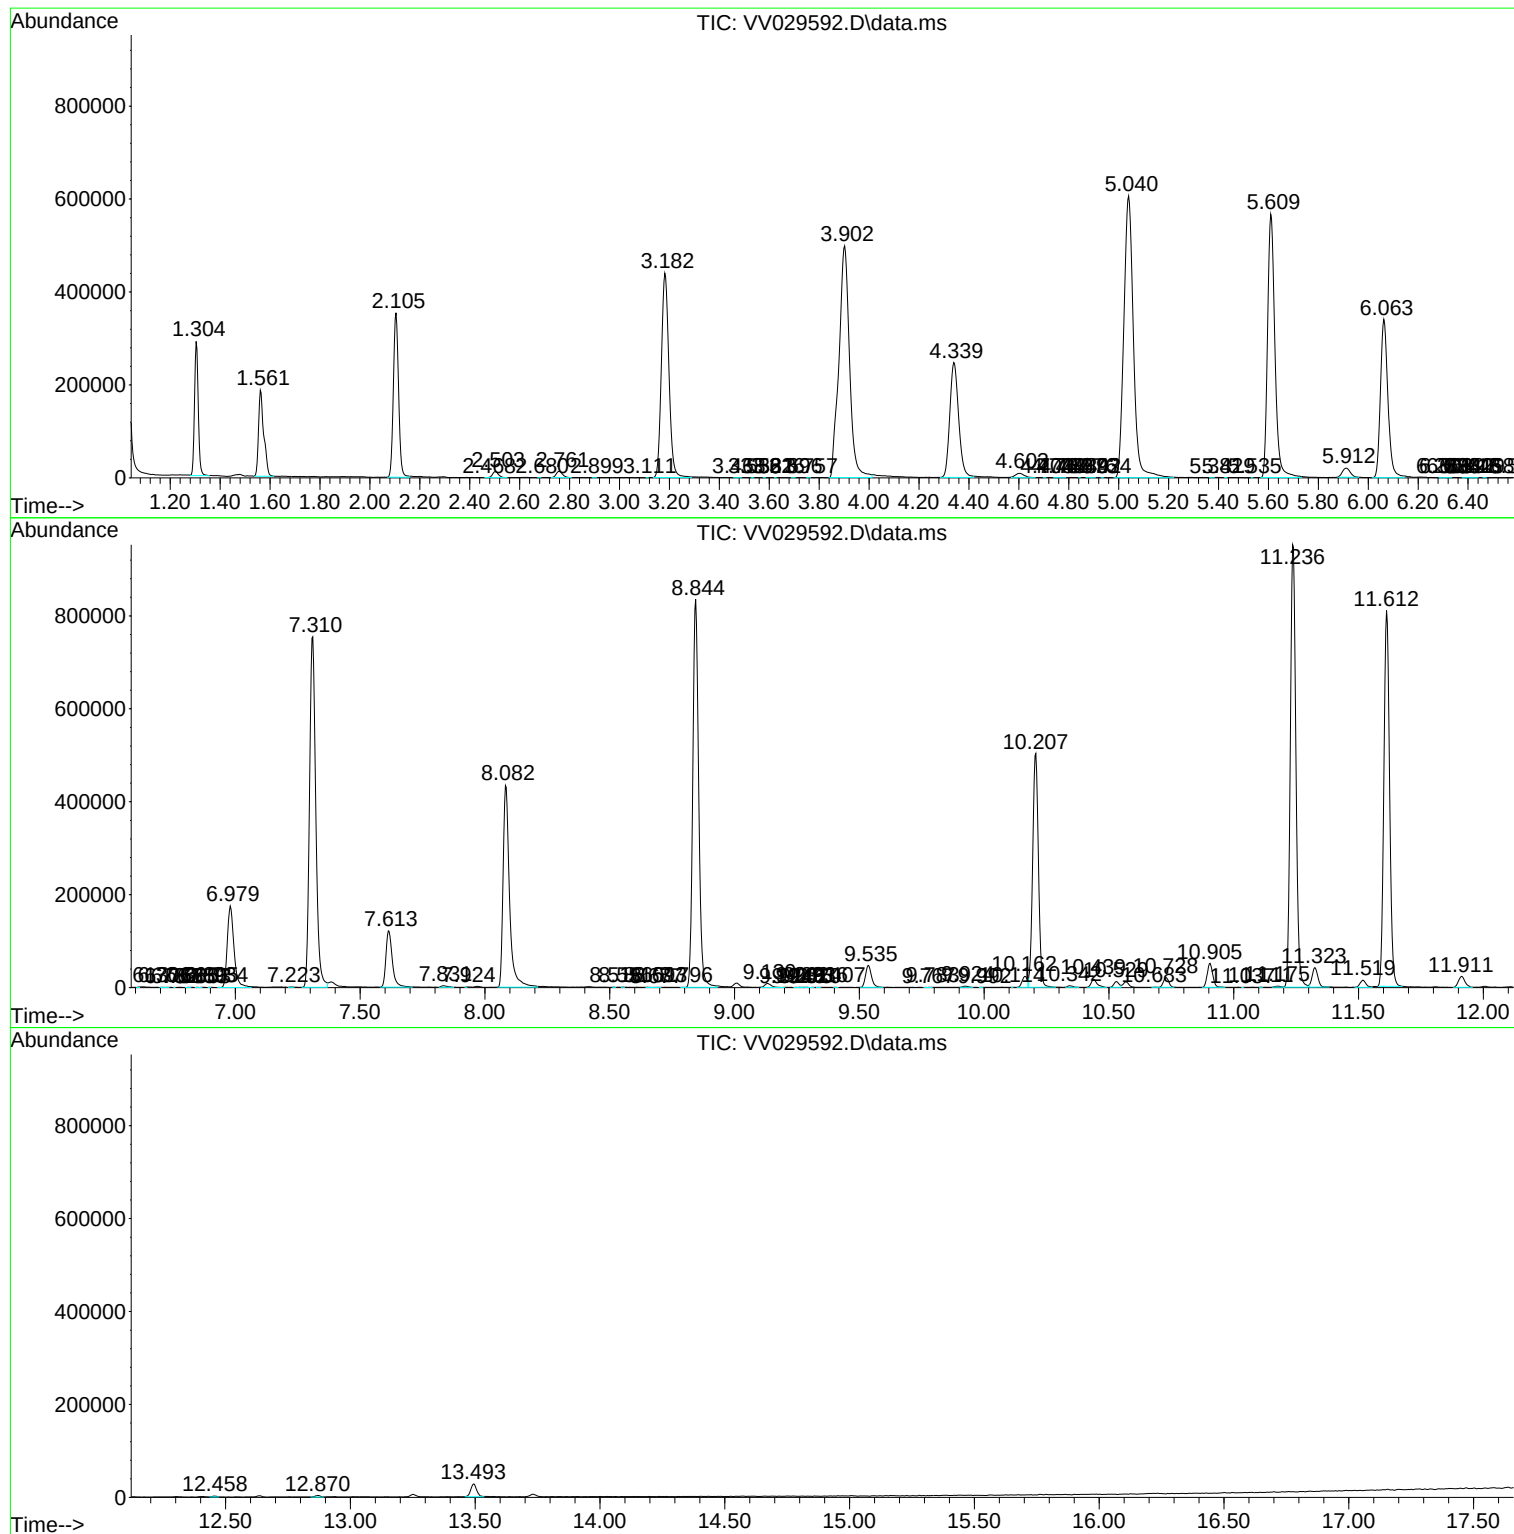

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029592.D
Acq On : 12 Dec 2022 13:54
Operator : SY/MD
Sample : N5929-15DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029592.D
Acq On : 12 Dec 2022 13:54
Operator : SY/MD
Sample : N5929-15DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc