

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
 Data File : VV029594.D
 Acq On : 12 Dec 2022 14:41
 Operator : SY/MD
 Sample : N5920-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	243690	241685	15.60%	1.777%
2	1.565	155	163	177	rVB	190377	215363	13.90%	1.584%
3	2.105	320	331	349	rBV2	391816	578467	37.34%	4.254%
4	2.503	445	455	469	rVB2	10471	17321	1.12%	0.127%
5	2.610	481	488	492	rBV4	684	973	0.06%	0.007%
6	2.671	504	507	508	rBV	160	70	0.00%	0.001%
7	2.799	545	547	551	rBV2	160	134	0.01%	0.001%
8	2.835	556	558	560	rBV	145	74	0.00%	0.001%
9	2.902	576	579	585	rBV2	295	314	0.02%	0.002%
10	2.979	598	603	604	rBV2	286	218	0.01%	0.002%
11	3.008	611	612	615	rVB2	148	41	0.00%	0.000%
12	3.050	622	625	629	rVB2	260	179	0.01%	0.001%
13	3.079	629	634	636	rBV2	239	223	0.01%	0.002%
14	3.179	658	665	666	rBV2	381	396	0.03%	0.003%
15	3.317	706	708	710	rBV	143	59	0.00%	0.000%
16	3.349	715	718	719	rBV	124	67	0.00%	0.000%
17	3.359	719	721	724	rVB2	315	142	0.01%	0.001%
18	3.423	738	741	744	rBV2	239	172	0.01%	0.001%
19	3.468	752	755	757	rBV	165	103	0.01%	0.001%
20	3.529	769	774	781	rBV2	147	168	0.01%	0.001%
21	3.574	786	788	790	rVB	157	66	0.00%	0.000%
22	3.703	825	828	829	rBV	99	55	0.00%	0.000%
23	3.741	837	840	841	rBV	114	69	0.00%	0.001%
24	3.780	848	852	853	rBV	158	105	0.01%	0.001%
25	3.815	860	863	865	rBV	68	47	0.00%	0.000%
26	3.873	869	881	912	rBV	116096	388315	25.06%	2.855%
27	4.339	1010	1026	1055	rBV2	233449	583241	37.64%	4.289%
28	4.603	1093	1108	1126	rVB2	13690	33067	2.13%	0.243%
29	4.703	1136	1139	1141	rBV2	138	72	0.00%	0.001%
30	4.780	1159	1163	1165	rBV2	168	117	0.01%	0.001%
31	4.812	1171	1173	1176	rBV2	220	103	0.01%	0.001%
32	4.825	1176	1177	1178	rBV2	127	36	0.00%	0.000%
33	4.957	1215	1218	1221	rVB2	169	103	0.01%	0.001%
34	5.040	1221	1244	1280	rBV2	591742	1549377	100.00%	11.393%
35	5.458	1371	1374	1376	rBV2	232	127	0.01%	0.001%
36	5.535	1395	1398	1399	rBV	97	58	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121222\
 Data File : VW029594.D
 Acq On : 12 Dec 2022 14:41
 Operator : SY/MD
 Sample : N5920-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1406	1421	1473	rBV	564579	1155677	74.59%	8.498%
38	5.905	1500	1513	1548	rBV	425753	855315	55.20%	6.289%
39	6.063	1549	1562	1583	rBV	327922	669637	43.22%	4.924%
40	6.342	1648	1649	1651	rBV	150	37	0.00%	0.000%
41	6.368	1655	1657	1659	rVV2	249	121	0.01%	0.001%
42	6.391	1662	1664	1671	rVB2	211	187	0.01%	0.001%
43	6.442	1676	1680	1682	rBV2	270	212	0.01%	0.002%
44	6.468	1686	1688	1691	rVB2	215	79	0.01%	0.001%
45	6.487	1691	1694	1695	rBV2	137	68	0.00%	0.001%
46	6.513	1699	1702	1706	rVB2	161	111	0.01%	0.001%
47	6.542	1706	1711	1712	rBV	95	82	0.01%	0.001%
48	6.551	1712	1714	1715	rBV	179	77	0.00%	0.001%
49	6.580	1722	1723	1724	rBV	180	41	0.00%	0.000%
50	6.593	1725	1727	1731	rBV	299	239	0.02%	0.002%
51	6.625	1731	1737	1738	rBV3	597	595	0.04%	0.004%
52	6.735	1768	1771	1773	rBV	186	99	0.01%	0.001%
53	6.754	1775	1777	1779	rVV	198	92	0.01%	0.001%
54	6.770	1780	1782	1786	rVB	264	136	0.01%	0.001%
55	6.789	1786	1788	1793	rBV2	239	201	0.01%	0.001%
56	6.831	1798	1801	1804	rVV2	172	121	0.01%	0.001%
57	6.844	1804	1805	1808	rVB2	118	46	0.00%	0.000%
58	6.908	1823	1825	1828	rVB2	147	80	0.01%	0.001%
59	6.924	1828	1830	1831	rBV2	121	51	0.00%	0.000%
60	6.979	1831	1847	1875	rBV	166719	306466	19.78%	2.254%
61	7.240	1924	1928	1930	rBV2	314	276	0.02%	0.002%
62	7.307	1936	1949	1977	rBV	734574	1302292	84.05%	9.576%
63	7.613	2031	2044	2069	rBV	116726	208360	13.45%	1.532%
64	7.966	2151	2154	2157	rBV2	817	593	0.04%	0.004%
65	8.082	2180	2190	2224	rBV	387054	707988	45.70%	5.206%
66	8.645	2362	2365	2367	rBV2	208	110	0.01%	0.001%
67	8.657	2367	2369	2373	rVB2	317	130	0.01%	0.001%
68	8.693	2379	2380	2381	rBV2	336	116	0.01%	0.001%
69	8.738	2392	2394	2396	rVB3	204	90	0.01%	0.001%
70	8.844	2415	2427	2447	rBV	814487	1345440	86.84%	9.894%
71	9.120	2511	2513	2514	rBV	365	141	0.01%	0.001%
72	9.265	2556	2558	2562	rVB	241	106	0.01%	0.001%
73	9.297	2562	2568	2573	rBV2	209	287	0.02%	0.002%
74	9.522	2637	2638	2639	rBV	314	114	0.01%	0.001%
75	9.587	2655	2658	2662	rVB2	654	390	0.03%	0.003%
76	9.702	2691	2694	2697	rVB2	205	101	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121222\
 Data File : VW029594.D
 Acq On : 12 Dec 2022 14:41
 Operator : SY/MD
 Sample : N5920-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

77	9.738	2703	2705	2708	rBV2	138	52	0.00%	0.000%
78	9.757	2708	2711	2715	rVB2	256	163	0.01%	0.001%
79	9.883	2746	2750	2757	rVB3	230	245	0.02%	0.002%
80	9.928	2757	2764	2772	rBV3	739	904	0.06%	0.007%
81	9.985	2781	2782	2783	rVB3	107	21	0.00%	0.000%
82	10.056	2802	2804	2806	rBV2	149	90	0.01%	0.001%
83	10.117	2820	2823	2825	rBV2	208	112	0.01%	0.001%
84	10.162	2828	2837	2841	rVV	22192	32443	2.09%	0.239%
85	10.207	2842	2851	2882	rVB	468658	745423	48.11%	5.481%
86	10.368	2898	2901	2912	rVB4	530	692	0.04%	0.005%
87	10.567	2955	2963	2981	rVB2	9663	16336	1.05%	0.120%
88	10.770	3024	3026	3031	rVB	440	224	0.01%	0.002%
89	10.969	3085	3088	3090	rBV	167	103	0.01%	0.001%
90	11.236	3160	3171	3199	rBV	903670	1419810	91.64%	10.440%
91	11.503	3252	3254	3258	rVB3	355	237	0.02%	0.002%
92	11.535	3261	3264	3266	rBV	146	105	0.01%	0.001%
93	11.564	3270	3273	3276	rBV3	374	302	0.02%	0.002%
94	11.612	3276	3288	3316	rBV	768031	1205543	77.81%	8.865%
95	12.014	3410	3413	3415	rBV2	283	183	0.01%	0.001%
96	13.252	3792	3798	3806	rVB8	2900	4585	0.30%	0.034%
97	13.731	3941	3947	3955	rBV5	3014	4137	0.27%	0.030%


Sum of corrected areas: 13599141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029594.D
Acq On : 12 Dec 2022 14:41
Operator : SY/MD
Sample : N5920-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

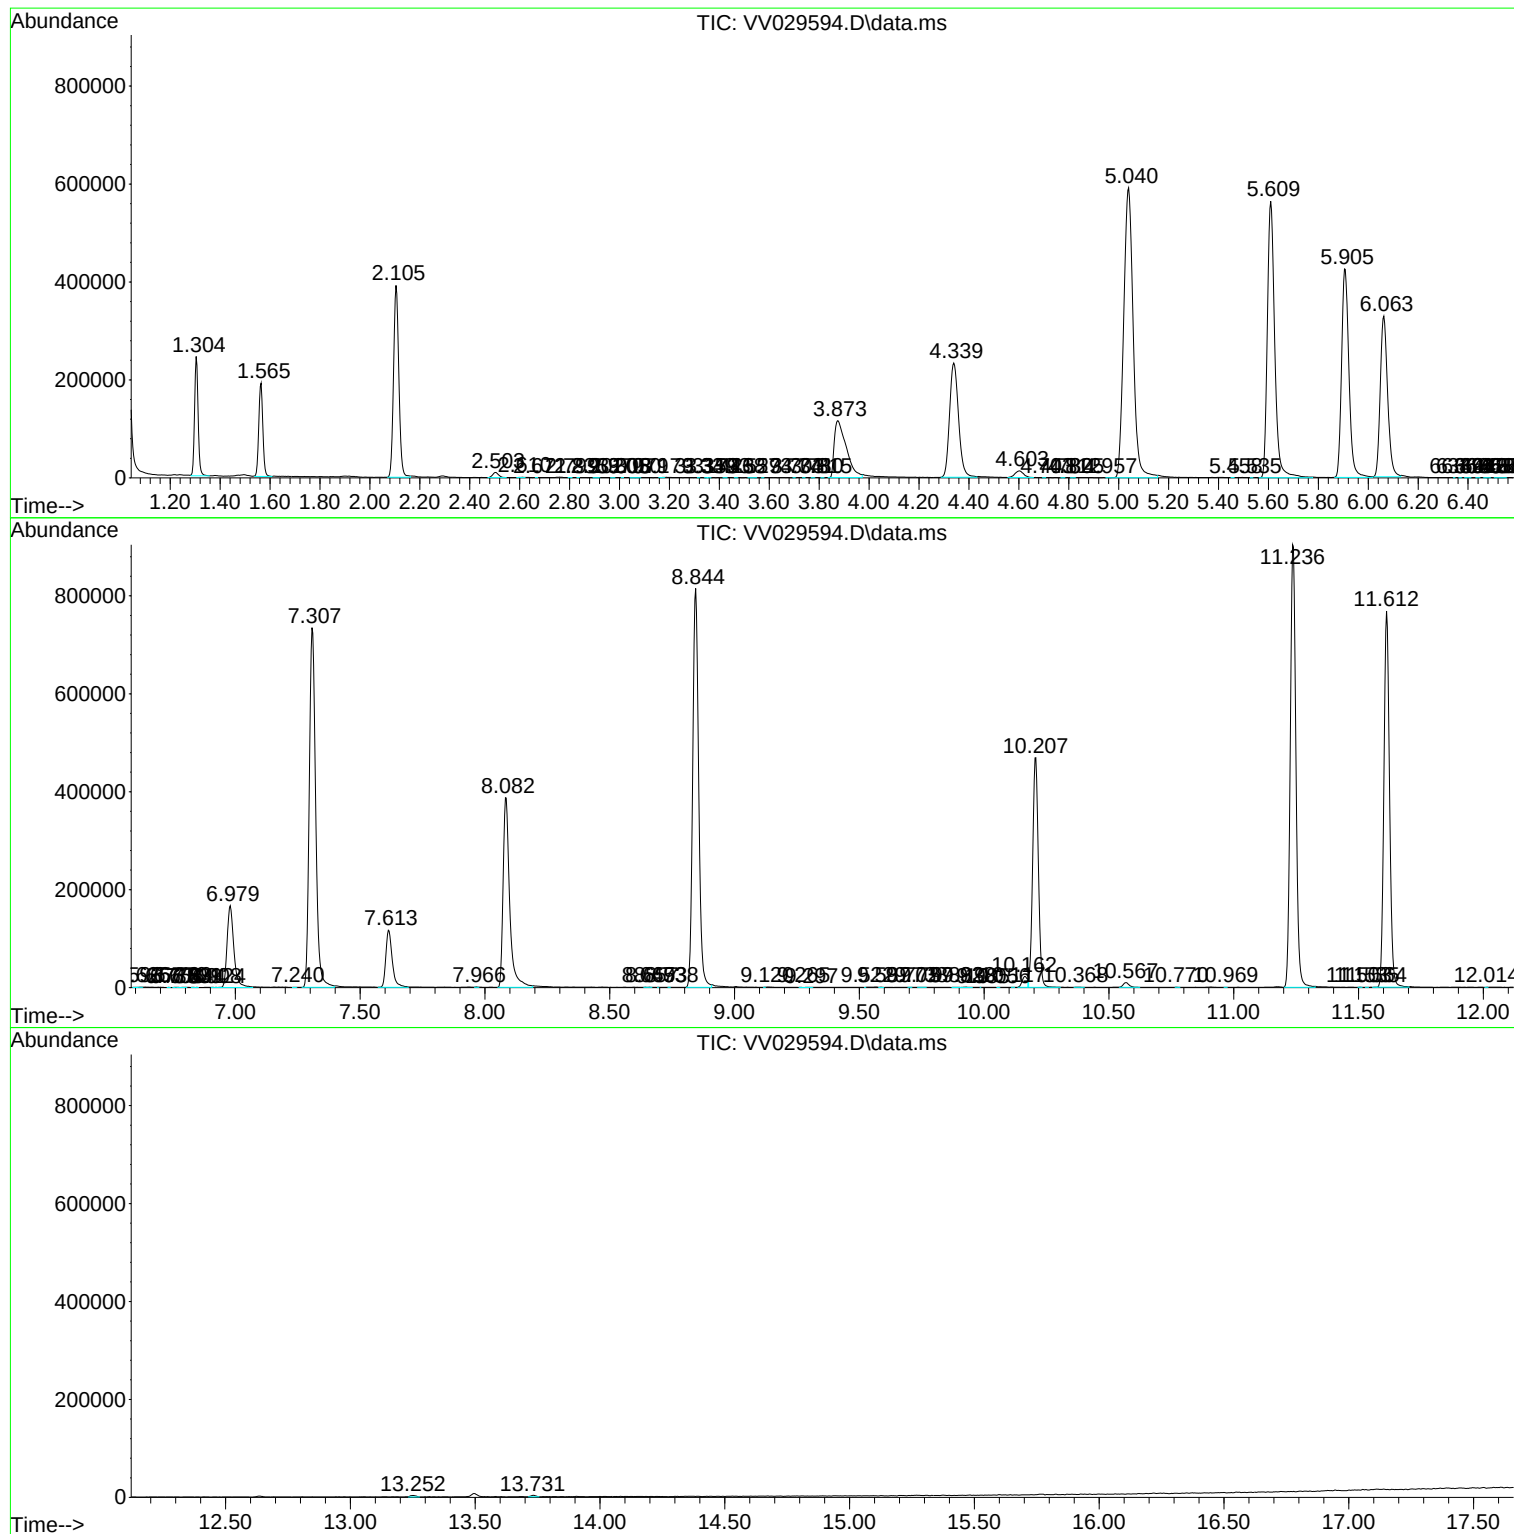

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029594.D
Acq On : 12 Dec 2022 14:41
Operator : SY/MD
Sample : N5920-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029594.D
Acq On : 12 Dec 2022 14:41
Operator : SY/MD
Sample : N5920-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------