

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
 Data File : VV029596.D
 Acq On : 12 Dec 2022 15:28
 Operator : SY/MD
 Sample : N5915-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N08DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	242520	248118	13.39%	1.813%
2	1.564	155	163	176	rVB	190708	211367	11.41%	1.544%
3	2.104	321	331	352	rBV	372748	540617	29.17%	3.950%
4	2.423	427	430	433	rBV2	237	215	0.01%	0.002%
5	2.461	439	442	448	rBV2	208	251	0.01%	0.002%
6	2.503	448	455	465	rVV	4298	6473	0.35%	0.047%
7	2.632	482	495	515	rBV3	4567	12194	0.66%	0.089%
8	2.764	524	536	557	rVB	51593	106565	5.75%	0.779%
9	2.931	585	588	590	rBV2	356	276	0.01%	0.002%
10	3.188	654	668	685	rBV	17504	37193	2.01%	0.272%
11	3.291	693	700	701	rBV	507	455	0.02%	0.003%
12	3.330	710	712	715	rBV	124	67	0.00%	0.000%
13	3.391	729	731	735	rBV2	144	98	0.01%	0.001%
14	3.468	752	755	764	rVB	171	197	0.01%	0.001%
15	3.580	786	790	793	rBV	209	158	0.01%	0.001%
16	3.674	816	819	822	rBV2	131	76	0.00%	0.001%
17	3.741	837	840	844	rBV2	129	109	0.01%	0.001%
18	3.773	849	850	854	rVB2	199	85	0.00%	0.001%
19	3.815	854	863	866	rBV2	226	295	0.02%	0.002%
20	3.899	870	889	919	rBV3	181284	663763	35.82%	4.850%
21	4.339	1010	1026	1060	rBV	240509	601252	32.44%	4.393%
22	4.587	1099	1103	1106	rBV2	521	358	0.02%	0.003%
23	4.628	1113	1116	1122	rBV2	523	533	0.03%	0.004%
24	4.677	1122	1131	1134	rBV4	979	1455	0.08%	0.011%
25	4.802	1165	1170	1172	rBV	152	112	0.01%	0.001%
26	4.818	1173	1175	1177	rVB2	197	88	0.00%	0.001%
27	4.844	1177	1183	1184	rBV	161	84	0.00%	0.001%
28	4.931	1205	1210	1212	rBV2	313	264	0.01%	0.002%
29	5.040	1226	1244	1299	rBV2	582938	1569022	84.66%	11.464%
30	5.458	1372	1374	1376	rBV	186	106	0.01%	0.001%
31	5.609	1407	1421	1459	rBV	600901	1216816	65.66%	8.890%
32	5.911	1499	1515	1530	rBV5	23355	51982	2.80%	0.380%
33	6.063	1548	1562	1601	rBV	323413	674527	36.40%	4.928%
34	6.268	1624	1626	1628	rBV	226	86	0.00%	0.001%
35	6.304	1634	1637	1641	rVB	229	130	0.01%	0.001%
36	6.345	1648	1650	1652	rVB	371	106	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121222\
 Data File : VW029596.D
 Acq On : 12 Dec 2022 15:28
 Operator : SY/MD
 Sample : N5915-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N08DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.371	1653	1658	1659	rVB3	319	185	0.01%	0.001%
38	6.403	1665	1668	1670	rBV	317	236	0.01%	0.002%
39	6.513	1700	1702	1706	rBV2	79	69	0.00%	0.001%
40	6.545	1706	1712	1716	rBV2	160	218	0.01%	0.002%
41	6.596	1723	1728	1729	rBV2	133	111	0.01%	0.001%
42	6.670	1750	1751	1756	rVB3	232	109	0.01%	0.001%
43	6.738	1769	1772	1775	rVB2	133	86	0.00%	0.001%
44	6.770	1775	1782	1783	rBV2	170	159	0.01%	0.001%
45	6.815	1793	1796	1799	rBV2	196	105	0.01%	0.001%
46	6.979	1835	1847	1877	rBV	164438	303348	16.37%	2.216%
47	7.165	1900	1905	1906	rBV2	541	503	0.03%	0.004%
48	7.233	1925	1926	1931	rVB2	422	196	0.01%	0.001%
49	7.262	1931	1935	1936	rBV	300	221	0.01%	0.002%
50	7.307	1937	1949	1986	rBV	731040	1295061	69.88%	9.462%
51	7.612	2035	2044	2069	rBV	113310	201985	10.90%	1.476%
52	7.937	2135	2145	2153	rBV3	3464	6174	0.33%	0.045%
53	8.085	2180	2191	2219	rBV	364210	668134	36.05%	4.882%
54	8.570	2339	2342	2344	rBV2	353	253	0.01%	0.002%
55	8.677	2372	2375	2376	rBV	168	88	0.00%	0.001%
56	8.712	2379	2386	2389	rBV3	489	660	0.04%	0.005%
57	8.844	2414	2427	2430	rBV	923950	1293806	69.81%	9.453%
58	9.191	2533	2535	2537	rBV2	357	191	0.01%	0.001%
59	9.239	2548	2550	2553	rBV	190	76	0.00%	0.001%
60	9.255	2553	2555	2556	rBV	299	142	0.01%	0.001%
61	9.316	2570	2574	2576	rBV3	276	212	0.01%	0.002%
62	9.329	2576	2578	2579	rBV	312	98	0.01%	0.001%
63	9.448	2613	2615	2616	rBV	174	67	0.00%	0.000%
64	9.474	2621	2623	2625	rBV2	105	69	0.00%	0.001%
65	9.500	2629	2631	2635	rVB2	229	116	0.01%	0.001%
66	9.538	2635	2643	2645	rBV2	831	918	0.05%	0.007%
67	9.641	2672	2675	2677	rVV	197	93	0.01%	0.001%
68	9.712	2694	2697	2700	rBV2	215	208	0.01%	0.002%
69	9.799	2720	2724	2725	rBV	277	175	0.01%	0.001%
70	9.844	2736	2738	2742	rBV	178	92	0.00%	0.001%
71	9.866	2742	2745	2747	rBV	390	218	0.01%	0.002%
72	9.924	2756	2763	2771	rBV3	2766	3467	0.19%	0.025%
73	9.982	2779	2781	2783	rVB3	344	142	0.01%	0.001%
74	10.001	2785	2787	2790	rVB	300	112	0.01%	0.001%
75	10.040	2797	2799	2801	rBV	178	75	0.00%	0.001%
76	10.078	2809	2811	2815	rVB2	257	159	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121222\
 Data File : VW029596.D
 Acq On : 12 Dec 2022 15:28
 Operator : SY/MD
 Sample : N5915-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N08DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2825	2837	2841	rBV2	23597	34825	1.88%	0.254%
78	10.207	2842	2851	2877	rVB	460576	730496	39.42%	5.337%
79	10.377	2896	2904	2914	rBV3	3277	4839	0.26%	0.035%
80	10.455	2925	2928	2932	rVV3	345	223	0.01%	0.002%
81	10.474	2932	2934	2938	rVB2	237	110	0.01%	0.001%
82	10.509	2943	2945	2946	rBV2	145	68	0.00%	0.000%
83	10.567	2954	2963	2976	rVB2	10448	16902	0.91%	0.123%
84	10.696	3002	3003	3007	rBV	188	92	0.00%	0.001%
85	10.722	3008	3011	3013	rBV	288	186	0.01%	0.001%
86	10.770	3023	3026	3027	rBV	163	95	0.01%	0.001%
87	10.898	3062	3066	3067	rBV	403	263	0.01%	0.002%
88	11.172	3140	3151	3160	rBV	64110	100457	5.42%	0.734%
89	11.239	3161	3172	3204	rVB2	1001324	1853239	100.00%	13.540%
90	11.439	3230	3234	3238	rBV	439	464	0.03%	0.003%
91	11.512	3251	3257	3264	rBV4	1313	1744	0.09%	0.013%
92	11.548	3266	3268	3270	rBV3	676	370	0.02%	0.003%
93	11.612	3275	3288	3323	rVV	734633	1215677	65.60%	8.882%
94	11.844	3359	3360	3363	rBV2	150	80	0.00%	0.001%
95	11.860	3363	3365	3366	rVB	304	81	0.00%	0.001%
96	11.873	3366	3369	3371	rBV2	504	311	0.02%	0.002%
97	11.934	3385	3388	3390	rBV3	293	235	0.01%	0.002%
98	12.107	3440	3442	3446	rBV2	483	317	0.02%	0.002%
99	12.368	3521	3523	3525	rBV2	247	167	0.01%	0.001%
100	12.631	3601	3605	3612	rBV5	1407	1839	0.10%	0.013%




Sum of corrected areas: 13686910

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029596.D
Acq On : 12 Dec 2022 15:28
Operator : SY/MD
Sample : N5915-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

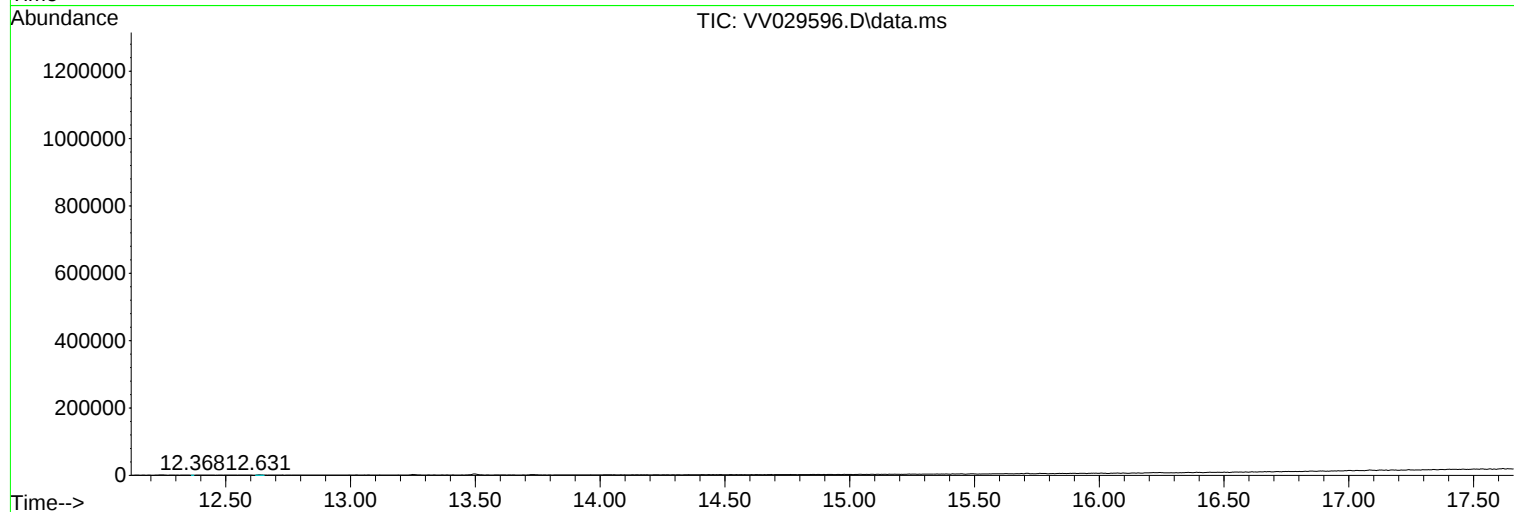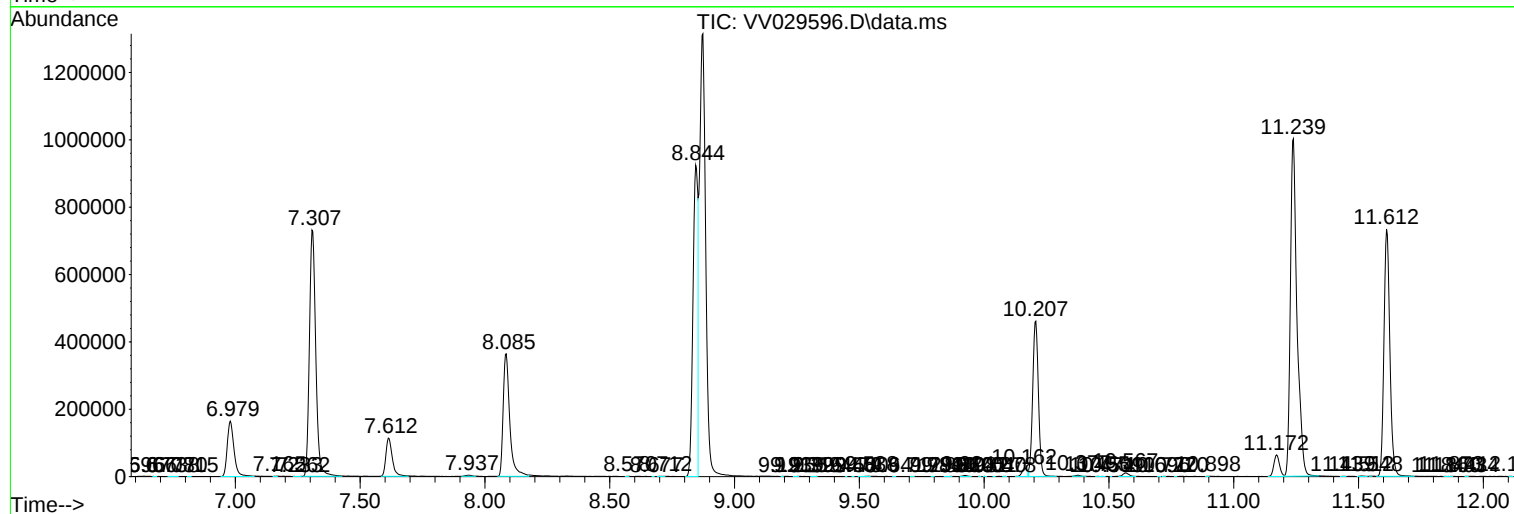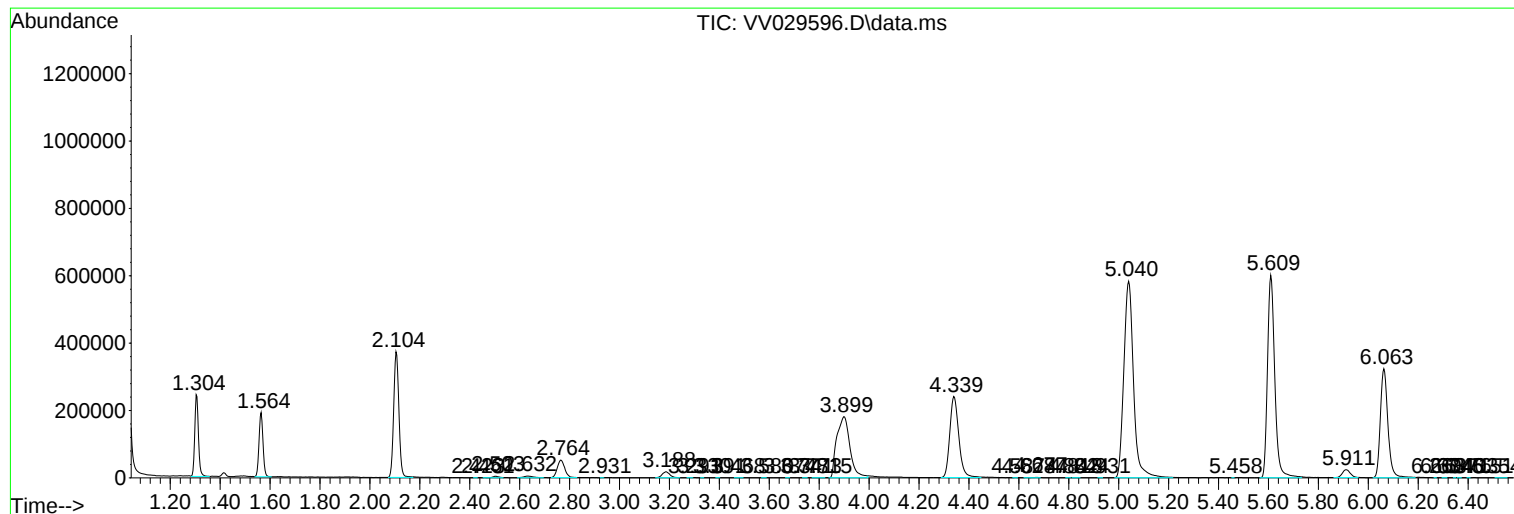

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029596.D
Acq On : 12 Dec 2022 15:28
Operator : SY/MD
Sample : N5915-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
Data File : VV029596.D
Acq On : 12 Dec 2022 15:28
Operator : SY/MD
Sample : N5915-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------