
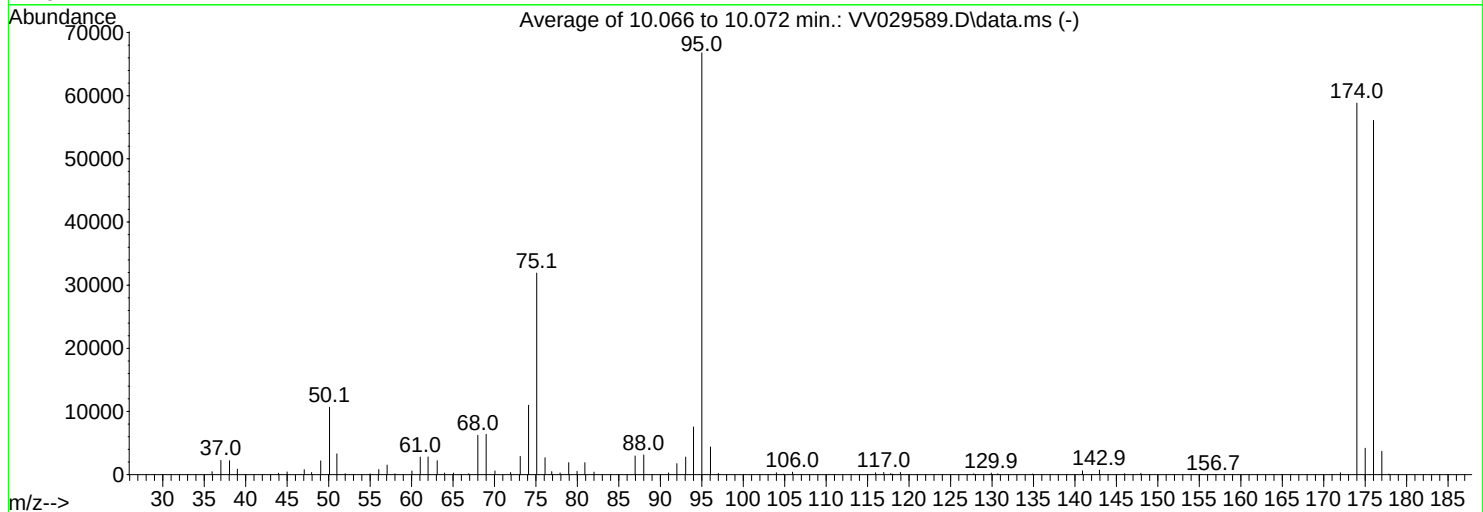


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121222\
 Data File : VV029589.D
 Acq On : 12 Dec 2022 12:40
 Operator : SY/MD
 Sample : BFB354
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB354

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 13 04:57:44 2022

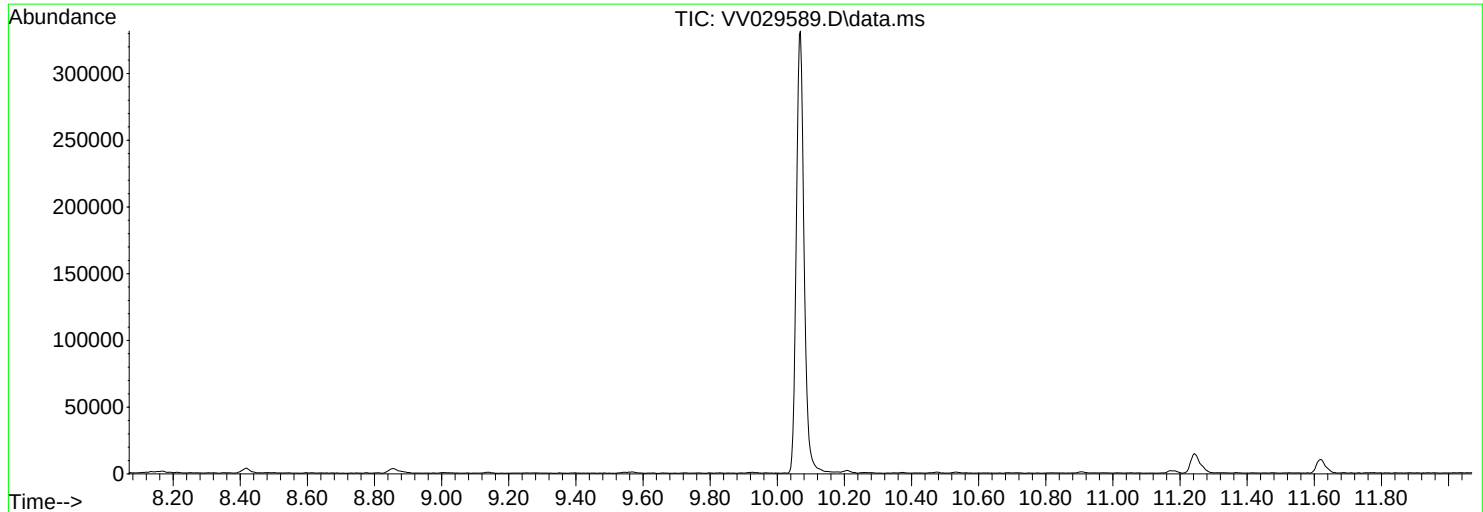

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	10673	PASS
75	95	30	80	47.8	31923	PASS
95	95	100	100	100.0	66787	PASS
96	95	5	9	6.6	4382	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.1	58832	PASS
175	174	5	9	7.1	4177	PASS
176	174	95	105	95.3	56088	PASS
177	176	5	10	6.6	3712	PASS

m/z	Abundance
39.90	239.0
43.90	369.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
36.00	515.0
37.00	2451.0
38.10	2203.0
39.00	887.0
39.90	302.0
44.00	587.0
45.00	487.0
47.10	762.0
48.00	341.0
49.00	2344.0
50.10	11345.0
51.00	3431.0
52.00	147.0
54.90	140.0
56.00	859.0
57.10	1581.0
58.00	109.0
60.00	569.0
61.00	2845.0
62.00	2944.0
63.10	2314.0
64.00	248.0
65.10	328.0
66.90	134.0
68.00	6418.0
69.00	6820.0
70.10	644.0
72.00	357.0
73.10	3126.0
74.10	11205.0
75.10	33320.0
76.10	2827.0
76.90	438.0
77.90	289.0
79.00	2016.0
80.00	566.0
80.90	1974.0
82.00	450.0
87.00	3035.0
88.00	3105.0
91.00	263.0
92.00	1871.0
93.00	2793.0
94.00	7773.0
95.00	68928.0
96.00	4481.0
97.00	206.0
104.00	290.0
104.80	103.0
106.00	459.0
116.00	337.0
116.90	357.0
117.80	247.0
118.90	338.0
127.80	231.0
129.90	240.0
130.70	151.0
134.90	103.0
140.90	579.0
143.00	680.0
146.00	151.0
147.90	204.0
159.10	107.0
172.00	311.0
174.00	59016.0
175.00	4352.0
176.00	56096.0
177.00	3911.0
177.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
36.00	506.0
37.00	2306.0
38.00	2265.0
39.00	901.0
39.90	260.0
44.00	606.0
45.00	456.0
47.00	828.0
48.00	349.0
49.10	2251.0
50.10	10919.0
51.00	3400.0
52.00	162.0
55.00	137.0
56.10	843.0
57.10	1604.0
58.00	141.0
60.00	587.0
61.10	2837.0
62.00	2914.0
63.10	2259.0
64.00	250.0
65.00	260.0
66.90	144.0
68.00	6413.0
69.00	6572.0
70.10	616.0
71.90	314.0
73.10	3001.0
74.10	11410.0
75.10	32984.0
76.10	2768.0
76.90	496.0
77.90	290.0
79.00	1979.0
79.90	559.0
80.90	1957.0
82.00	404.0
86.90	3035.0
88.00	3249.0
91.00	289.0
92.00	1808.0
93.00	2917.0
94.00	7815.0
95.00	69096.0
96.00	4496.0
97.00	211.0
104.00	338.0
104.90	102.0
105.90	408.0
116.00	304.0
116.90	361.0
117.80	259.0
118.90	353.0
127.80	207.0
129.90	268.0
130.70	179.0
134.90	115.0
140.90	618.0
142.90	748.0
146.00	159.0
148.00	219.0
172.00	325.0
174.00	60824.0
175.00	4266.0
176.00	58040.0
177.00	3785.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
35.90	423.0
37.00	2039.0
38.00	2120.0
39.00	782.0
39.90	215.0
44.00	597.0
45.00	374.0
47.00	790.0
47.90	308.0
49.10	1975.0
50.10	9754.0
51.00	3048.0
52.00	162.0
55.10	120.0
56.10	697.0
57.00	1388.0
58.00	130.0
60.10	569.0
61.10	2654.0
62.00	2608.0
63.10	2060.0
63.90	265.0
65.00	172.0
66.90	160.0
68.00	5865.0
69.00	5774.0
70.00	529.0
71.90	289.0
73.10	2564.0
74.10	10348.0
75.10	29464.0
76.10	2474.0
76.90	503.0
77.90	274.0
78.90	1739.0
79.90	511.0
80.90	1769.0
82.00	333.0
86.90	2849.0
88.00	3023.0
91.00	252.0
92.00	1610.0
93.10	2692.0
94.00	7088.0
95.00	62336.0
96.10	4168.0
97.00	172.0
104.00	312.0
105.90	350.0
115.90	249.0
117.00	368.0
118.00	233.0
119.00	364.0
128.00	177.0
129.90	247.0
130.70	135.0
134.90	113.0
140.90	616.0
142.90	740.0
146.00	135.0
148.00	185.0
155.20	101.0
156.70	113.0
172.00	292.0
174.00	56656.0
175.00	3912.0
176.00	54128.0
177.00	3440.0
177.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354