

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033254.D
 Acq On : 12 Dec 2023 11:24
 Operator : SY/MD
 Sample : VV1212MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	34	39	59	rBV	18644	24812	2.42%	0.308%
2	1.281	68	75	87	rVB	138953	146253	14.27%	1.817%
3	1.532	145	153	165	rBV	100836	118092	11.52%	1.467%
4	2.059	306	317	336	rBV	217569	319315	31.15%	3.968%
5	2.211	360	364	366	rBV2	427	321	0.03%	0.004%
6	2.362	409	411	416	rVB2	354	233	0.02%	0.003%
7	2.387	416	419	422	rBV	327	228	0.02%	0.003%
8	2.442	432	436	437	rBV2	1036	694	0.07%	0.009%
9	2.500	451	454	457	rBV2	333	315	0.03%	0.004%
10	2.558	467	472	476	rVB2	356	374	0.04%	0.005%
11	2.719	520	522	525	rBV2	382	212	0.02%	0.003%
12	2.966	595	599	602	rBV	231	206	0.02%	0.003%
13	3.024	615	617	623	rVB2	246	243	0.02%	0.003%
14	3.059	624	628	630	rBV	371	237	0.02%	0.003%
15	3.114	639	645	647	rBV3	428	483	0.05%	0.006%
16	3.288	696	699	704	rVB	288	234	0.02%	0.003%
17	3.397	728	733	735	rBV	258	214	0.02%	0.003%
18	3.471	753	756	757	rBV	283	179	0.02%	0.002%
19	3.484	758	760	766	rVB2	334	305	0.03%	0.004%
20	3.526	767	773	776	rBB	281	287	0.03%	0.004%
21	3.548	776	780	784	rBV2	280	289	0.03%	0.004%
22	3.776	843	851	881	rBV	51775	137518	13.42%	1.709%
23	4.246	981	997	1030	rBV	166680	428721	41.82%	5.327%
24	4.487	1068	1072	1074	rBV	423	329	0.03%	0.004%
25	4.506	1074	1078	1079	rVV3	384	251	0.02%	0.003%
26	4.728	1145	1147	1149	rBV	368	197	0.02%	0.002%
27	4.783	1161	1164	1170	rVB2	336	278	0.03%	0.003%
28	4.953	1199	1217	1250	rBV3	384220	1025045	100.00%	12.736%
29	5.442	1366	1369	1370	rBV3	532	256	0.02%	0.003%
30	5.532	1383	1397	1435	rBV	309521	640570	62.49%	7.959%
31	5.770	1467	1471	1473	rBV2	467	351	0.03%	0.004%
32	5.828	1479	1489	1509	rVB4	8355	19519	1.90%	0.243%
33	5.985	1525	1538	1563	rBV2	209530	432346	42.18%	5.372%
34	6.278	1626	1629	1633	rBV	283	224	0.02%	0.003%
35	6.329	1643	1645	1647	rVV2	491	290	0.03%	0.004%
36	6.342	1647	1649	1652	rVV	498	294	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033254.D
 Acq On : 12 Dec 2023 11:24
 Operator : SY/MD
 Sample : VV1212MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.635	1737	1740	1745	rBV2	214	248	0.02%	0.003%
38	6.770	1778	1782	1789	rBV	246	363	0.04%	0.005%
39	6.911	1813	1826	1849	rBV	124175	232175	22.65%	2.885%
40	7.243	1917	1929	1958	rBV	494246	876398	85.50%	10.889%
41	7.500	2007	2009	2012	rBV2	424	200	0.02%	0.002%
42	7.551	2015	2025	2042	rBV	91966	160392	15.65%	1.993%
43	7.789	2096	2099	2106	rVB3	530	479	0.05%	0.006%
44	7.828	2109	2111	2114	rBV	383	254	0.02%	0.003%
45	7.924	2138	2141	2143	rBV2	277	201	0.02%	0.002%
46	8.021	2162	2171	2184	rBV	184497	341635	33.33%	4.245%
47	8.362	2273	2277	2280	rBV4	633	625	0.06%	0.008%
48	8.509	2319	2323	2326	rBV2	597	421	0.04%	0.005%
49	8.529	2326	2329	2334	rBV2	379	314	0.03%	0.004%
50	8.673	2372	2374	2378	rBV2	319	193	0.02%	0.002%
51	8.731	2389	2392	2394	rBV	282	212	0.02%	0.003%
52	8.783	2396	2408	2438	rBV	496405	826596	80.64%	10.271%
53	9.040	2484	2488	2489	rBV2	317	187	0.02%	0.002%
54	9.124	2511	2514	2517	rVB2	441	332	0.03%	0.004%
55	9.146	2517	2521	2524	rBB2	321	295	0.03%	0.004%
56	9.201	2536	2538	2542	rVV2	218	174	0.02%	0.002%
57	9.342	2578	2582	2587	rBV2	366	396	0.04%	0.005%
58	9.371	2588	2591	2593	rBV2	542	270	0.03%	0.003%
59	9.468	2617	2621	2624	rBV2	270	236	0.02%	0.003%
60	9.574	2651	2654	2657	rBV2	232	243	0.02%	0.003%
61	9.628	2666	2671	2674	rBV2	218	284	0.03%	0.004%
62	9.689	2687	2690	2693	rBV	379	267	0.03%	0.003%
63	9.799	2720	2724	2727	rVB2	290	264	0.03%	0.003%
64	9.818	2727	2730	2733	rBV2	318	320	0.03%	0.004%
65	9.863	2742	2744	2747	rBV2	295	217	0.02%	0.003%
66	9.879	2747	2749	2751	rVV	318	183	0.02%	0.002%
67	9.963	2772	2775	2778	rVB2	348	248	0.02%	0.003%
68	9.982	2778	2781	2782	rBV	307	193	0.02%	0.002%
69	10.152	2823	2834	2854	rBV	291248	458560	44.74%	5.698%
70	10.480	2934	2936	2941	rBV2	345	285	0.03%	0.004%
71	10.603	2971	2974	2976	rBV2	383	268	0.03%	0.003%
72	10.718	3007	3010	3016	rVB2	404	492	0.05%	0.006%
73	10.747	3016	3019	3020	rBV	254	170	0.02%	0.002%
74	10.850	3048	3051	3054	rBV2	410	322	0.03%	0.004%
75	10.959	3084	3085	3089	rVB	365	177	0.02%	0.002%
76	11.130	3136	3138	3142	rBV2	578	375	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033254.D
 Acq On : 12 Dec 2023 11:24
 Operator : SY/MD
 Sample : VV1212MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3179	rBV	590771	903311	88.12%	11.224%
78	11.455	3232	3239	3243	rBB4	387	451	0.04%	0.006%
79	11.484	3244	3248	3250	rBV2	307	207	0.02%	0.003%
80	11.561	3259	3272	3300	rBV	592866	926954	90.43%	11.518%
81	11.760	3331	3334	3337	rVB3	369	188	0.02%	0.002%
82	11.779	3337	3340	3343	rBV3	261	228	0.02%	0.003%
83	11.940	3386	3390	3394	rBV2	222	267	0.03%	0.003%
84	12.037	3417	3420	3424	rBV	375	353	0.03%	0.004%
85	12.094	3433	3438	3441	rBV	220	213	0.02%	0.003%
86	12.152	3452	3456	3459	rBV	331	299	0.03%	0.004%
87	12.242	3480	3484	3485	rBV	264	181	0.02%	0.002%
88	12.496	3561	3563	3565	rBV	386	221	0.02%	0.003%
89	12.635	3600	3606	3609	rBV2	354	293	0.03%	0.004%
90	13.114	3753	3755	3762	rVB	303	212	0.02%	0.003%
91	13.152	3765	3767	3771	rVB2	489	308	0.03%	0.004%
92	13.429	3850	3853	3854	rBV2	567	296	0.03%	0.004%
93	13.448	3855	3859	3873	rVB2	3221	5266	0.51%	0.065%
94	13.686	3928	3933	3935	rBV3	868	821	0.08%	0.010%
95	13.856	3984	3986	3989	rBV	462	343	0.03%	0.004%
96	13.985	4018	4026	4028	rBV3	988	1269	0.12%	0.016%
97	14.046	4043	4045	4047	rBV2	405	182	0.02%	0.002%
98	14.500	4183	4186	4190	rBV3	474	406	0.04%	0.005%
99	14.776	4270	4272	4275	rBV2	567	399	0.04%	0.005%
100	15.027	4348	4350	4353	rVB2	563	309	0.03%	0.004%




Sum of corrected areas: 8048156

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033254.D
Acq On : 12 Dec 2023 11:24
Operator : SY/MD
Sample : VV1212MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

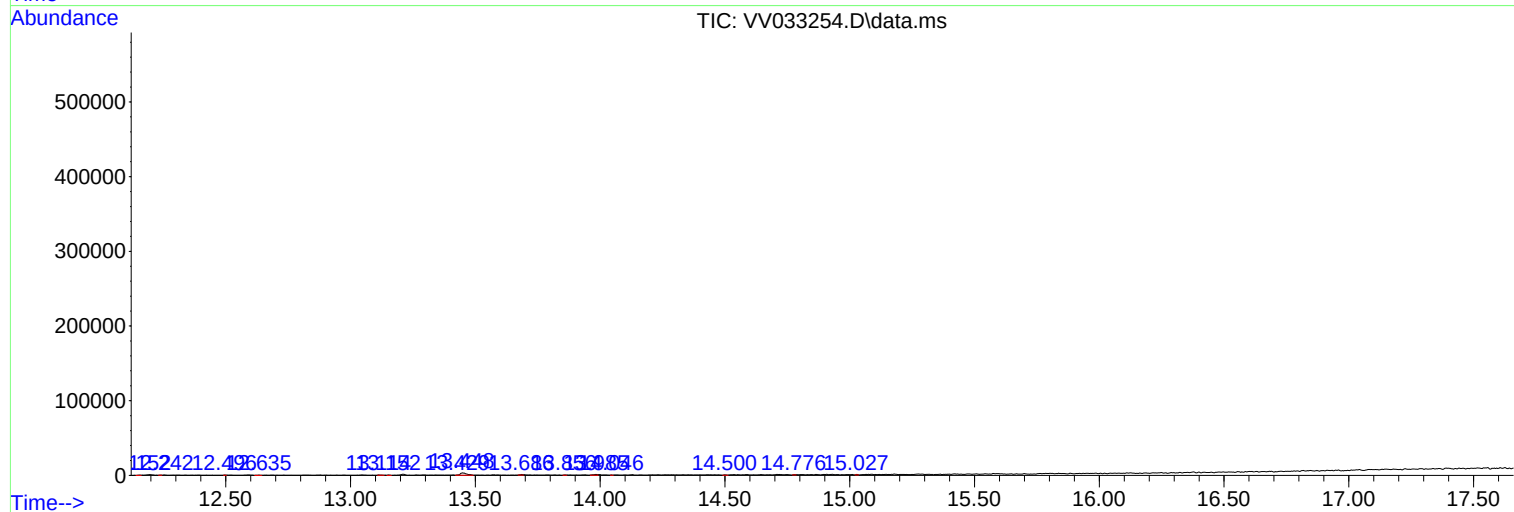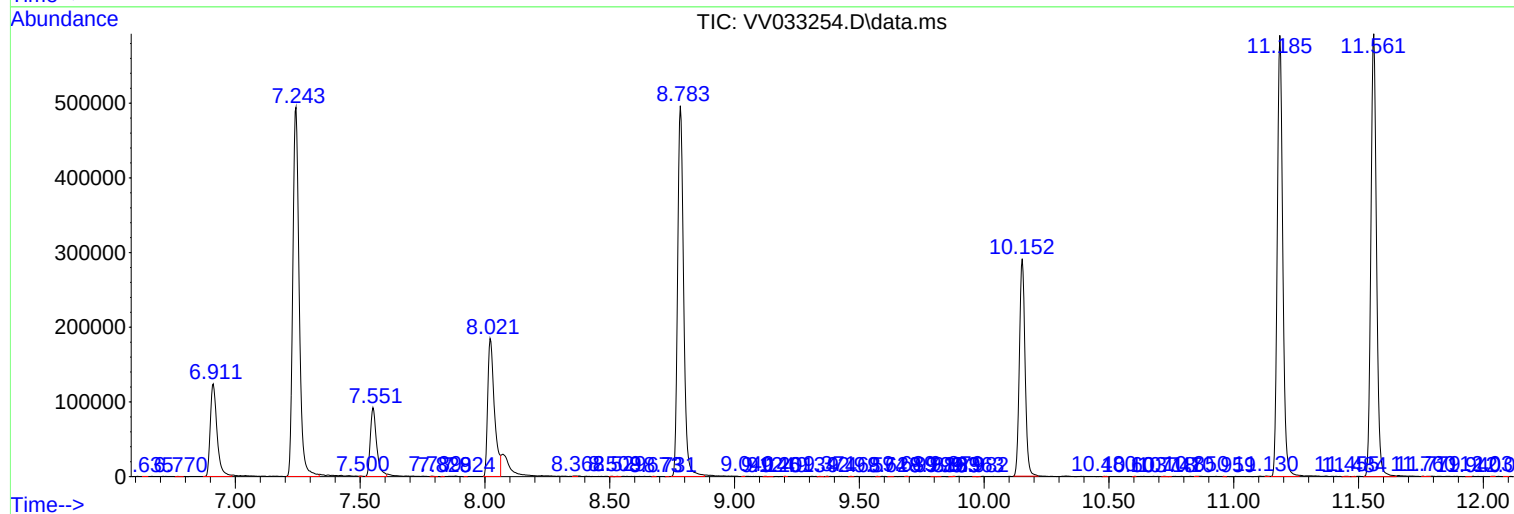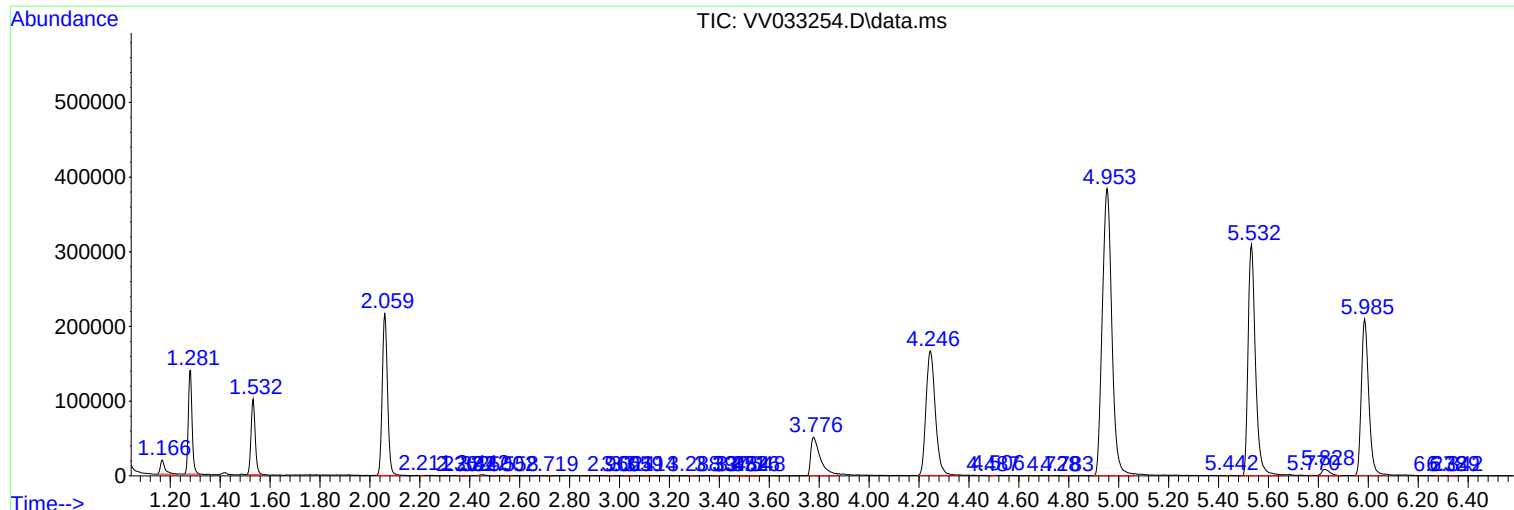

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033254.D
Acq On : 12 Dec 2023 11:24
Operator : SY/MD
Sample : VV1212MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033254.D
Acq On : 12 Dec 2023 11:24
Operator : SY/MD
Sample : VV1212MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
