

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033255.D
 Acq On : 12 Dec 2023 11:47
 Operator : SY/MD
 Sample : VV1212WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	35	40	60	rVB	15375	20097	2.05%	0.263%
2	1.281	68	75	88	rVB	130761	137735	14.06%	1.801%
3	1.532	146	153	168	rVB	94504	111587	11.39%	1.459%
4	2.059	307	317	341	rVB	206934	307400	31.37%	4.020%
5	2.323	397	399	404	rVB3	421	317	0.03%	0.004%
6	2.352	404	408	411	rBV2	207	214	0.02%	0.003%
7	2.391	415	420	422	rBV	276	245	0.03%	0.003%
8	2.452	432	439	449	rVB5	1351	1847	0.19%	0.024%
9	2.551	467	470	472	rBV	305	218	0.02%	0.003%
10	2.818	546	553	556	rBB2	329	348	0.04%	0.005%
11	2.838	556	559	563	rBV2	412	391	0.04%	0.005%
12	2.879	568	572	576	rVB2	308	335	0.03%	0.004%
13	2.928	584	587	589	rBV	266	198	0.02%	0.003%
14	2.986	600	605	606	rBB	375	234	0.02%	0.003%
15	3.037	617	621	624	rBV	298	215	0.02%	0.003%
16	3.455	747	751	754	rBV	297	245	0.03%	0.003%
17	3.580	787	790	793	rBV2	321	253	0.03%	0.003%
18	3.600	793	796	801	rVB2	280	239	0.02%	0.003%
19	3.731	834	837	840	rBV2	242	182	0.02%	0.002%
20	3.780	844	852	886	rBV	49211	132954	13.57%	1.739%
21	4.146	960	966	971	rBV2	478	745	0.08%	0.010%
22	4.249	981	998	1029	rBV	164502	413293	42.18%	5.405%
23	4.596	1103	1106	1109	rBV	401	359	0.04%	0.005%
24	4.657	1121	1125	1128	rVB2	436	269	0.03%	0.004%
25	4.702	1134	1139	1141	rVB3	454	331	0.03%	0.004%
26	4.725	1141	1146	1148	rBV	414	293	0.03%	0.004%
27	4.870	1186	1191	1192	rBV2	340	265	0.03%	0.003%
28	4.957	1199	1218	1242	rBV2	370012	979864	100.00%	12.813%
29	5.326	1331	1333	1337	rVB	513	275	0.03%	0.004%
30	5.465	1373	1376	1382	rBV3	553	453	0.05%	0.006%
31	5.532	1386	1397	1434	rVV	299113	619202	63.19%	8.097%
32	5.831	1481	1490	1508	rVB5	8858	19414	1.98%	0.254%
33	5.918	1513	1517	1519	rBV2	441	253	0.03%	0.003%
34	5.989	1526	1539	1570	rBV2	203293	419681	42.83%	5.488%
35	6.201	1601	1605	1606	rBV	484	334	0.03%	0.004%
36	6.297	1632	1635	1639	rBV2	313	214	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033255.D
 Acq On : 12 Dec 2023 11:47
 Operator : SY/MD
 Sample : VV1212WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.657	1745	1747	1751	rVB2	284	181	0.02%	0.002%
38	6.911	1816	1826	1847	rBV	120018	222196	22.68%	2.906%
39	7.201	1913	1916	1918	rBV2	526	292	0.03%	0.004%
40	7.243	1918	1929	1957	rBV	474689	843941	86.13%	11.036%
41	7.551	2016	2025	2045	rBV	85638	151636	15.48%	1.983%
42	7.702	2068	2072	2074	rBV	493	324	0.03%	0.004%
43	7.776	2092	2095	2099	rVB3	541	369	0.04%	0.005%
44	7.870	2122	2124	2128	rBV2	314	244	0.02%	0.003%
45	7.960	2147	2152	2154	rBV2	213	215	0.02%	0.003%
46	8.024	2163	2172	2194	rBV	176950	327935	33.47%	4.288%
47	8.358	2271	2276	2280	rBV4	880	938	0.10%	0.012%
48	8.423	2292	2296	2300	rVB2	258	196	0.02%	0.003%
49	8.461	2304	2308	2310	rBV	264	197	0.02%	0.003%
50	8.783	2396	2408	2440	rBV	479942	795227	81.16%	10.399%
51	9.024	2478	2483	2488	rVB2	498	542	0.06%	0.007%
52	9.050	2488	2491	2492	rBV	376	219	0.02%	0.003%
53	9.059	2492	2494	2496	rVV	406	191	0.02%	0.002%
54	9.120	2507	2513	2516	rBV3	298	300	0.03%	0.004%
55	9.175	2526	2530	2532	rBV	285	260	0.03%	0.003%
56	9.210	2538	2541	2542	rBV	371	218	0.02%	0.003%
57	9.297	2565	2568	2570	rBV2	289	188	0.02%	0.002%
58	9.329	2575	2578	2581	rBV2	328	252	0.03%	0.003%
59	9.368	2586	2590	2592	rBV	376	245	0.03%	0.003%
60	9.545	2640	2645	2647	rBV	291	297	0.03%	0.004%
61	9.680	2682	2687	2691	rVB2	225	233	0.02%	0.003%
62	9.706	2691	2695	2697	rBV	289	240	0.02%	0.003%
63	9.850	2737	2740	2742	rBV2	396	283	0.03%	0.004%
64	9.873	2743	2747	2751	rVB3	334	251	0.03%	0.003%
65	9.898	2751	2755	2758	rBV2	328	307	0.03%	0.004%
66	9.937	2763	2767	2774	rVB2	227	330	0.03%	0.004%
67	10.069	2804	2808	2810	rBV	415	322	0.03%	0.004%
68	10.091	2811	2815	2819	rVB	270	233	0.02%	0.003%
69	10.152	2822	2834	2858	rBV	281920	447514	45.67%	5.852%
70	10.529	2948	2951	2954	rBV2	269	183	0.02%	0.002%
71	10.619	2975	2979	2983	rBV2	374	372	0.04%	0.005%
72	10.641	2983	2986	2988	rVB2	331	212	0.02%	0.003%
73	10.683	2994	2999	3004	rBV2	399	589	0.06%	0.008%
74	10.760	3021	3023	3028	rBV	293	240	0.02%	0.003%
75	10.866	3054	3056	3061	rBV	238	205	0.02%	0.003%
76	11.008	3096	3100	3104	rBV2	223	273	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033255.D
 Acq On : 12 Dec 2023 11:47
 Operator : SY/MD
 Sample : VV1212WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3181	rBV	528662	810993	82.77%	10.605%
78	11.349	3203	3206	3207	rBV2	488	255	0.03%	0.003%
79	11.403	3220	3223	3227	rBV3	516	436	0.04%	0.006%
80	11.426	3227	3230	3233	rVB	705	353	0.04%	0.005%
81	11.455	3236	3239	3240	rBV	326	174	0.02%	0.002%
82	11.561	3260	3272	3297	rBV	546861	858566	87.62%	11.227%
83	11.786	3334	3342	3343	rBV2	400	416	0.04%	0.005%
84	11.834	3355	3357	3362	rVB3	257	173	0.02%	0.002%
85	12.033	3414	3419	3422	rBV	365	329	0.03%	0.004%
86	12.143	3452	3453	3459	rVB	247	197	0.02%	0.003%
87	12.374	3521	3525	3527	rBV	296	281	0.03%	0.004%
88	12.464	3547	3553	3556	rBV3	334	342	0.03%	0.004%
89	12.519	3567	3570	3574	rVB2	257	213	0.02%	0.003%
90	13.014	3721	3724	3726	rBV	245	184	0.02%	0.002%
91	13.059	3734	3738	3739	rBV	389	261	0.03%	0.003%
92	13.210	3781	3785	3786	rBV2	621	402	0.04%	0.005%
93	13.287	3806	3809	3814	rBV3	271	338	0.03%	0.004%
94	13.355	3827	3830	3832	rBV	459	302	0.03%	0.004%
95	13.397	3839	3843	3844	rBV	338	199	0.02%	0.003%
96	13.451	3852	3860	3867	rBV3	1726	2663	0.27%	0.035%
97	13.557	3888	3893	3894	rBV3	308	294	0.03%	0.004%
98	13.622	3911	3913	3916	rBV	504	279	0.03%	0.004%
99	13.641	3916	3919	3924	rBV3	375	381	0.04%	0.005%
100	13.747	3948	3952	3953	rBV3	318	204	0.02%	0.003%


Sum of corrected areas: 7647124

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033255.D
Acq On : 12 Dec 2023 11:47
Operator : SY/MD
Sample : VV1212WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

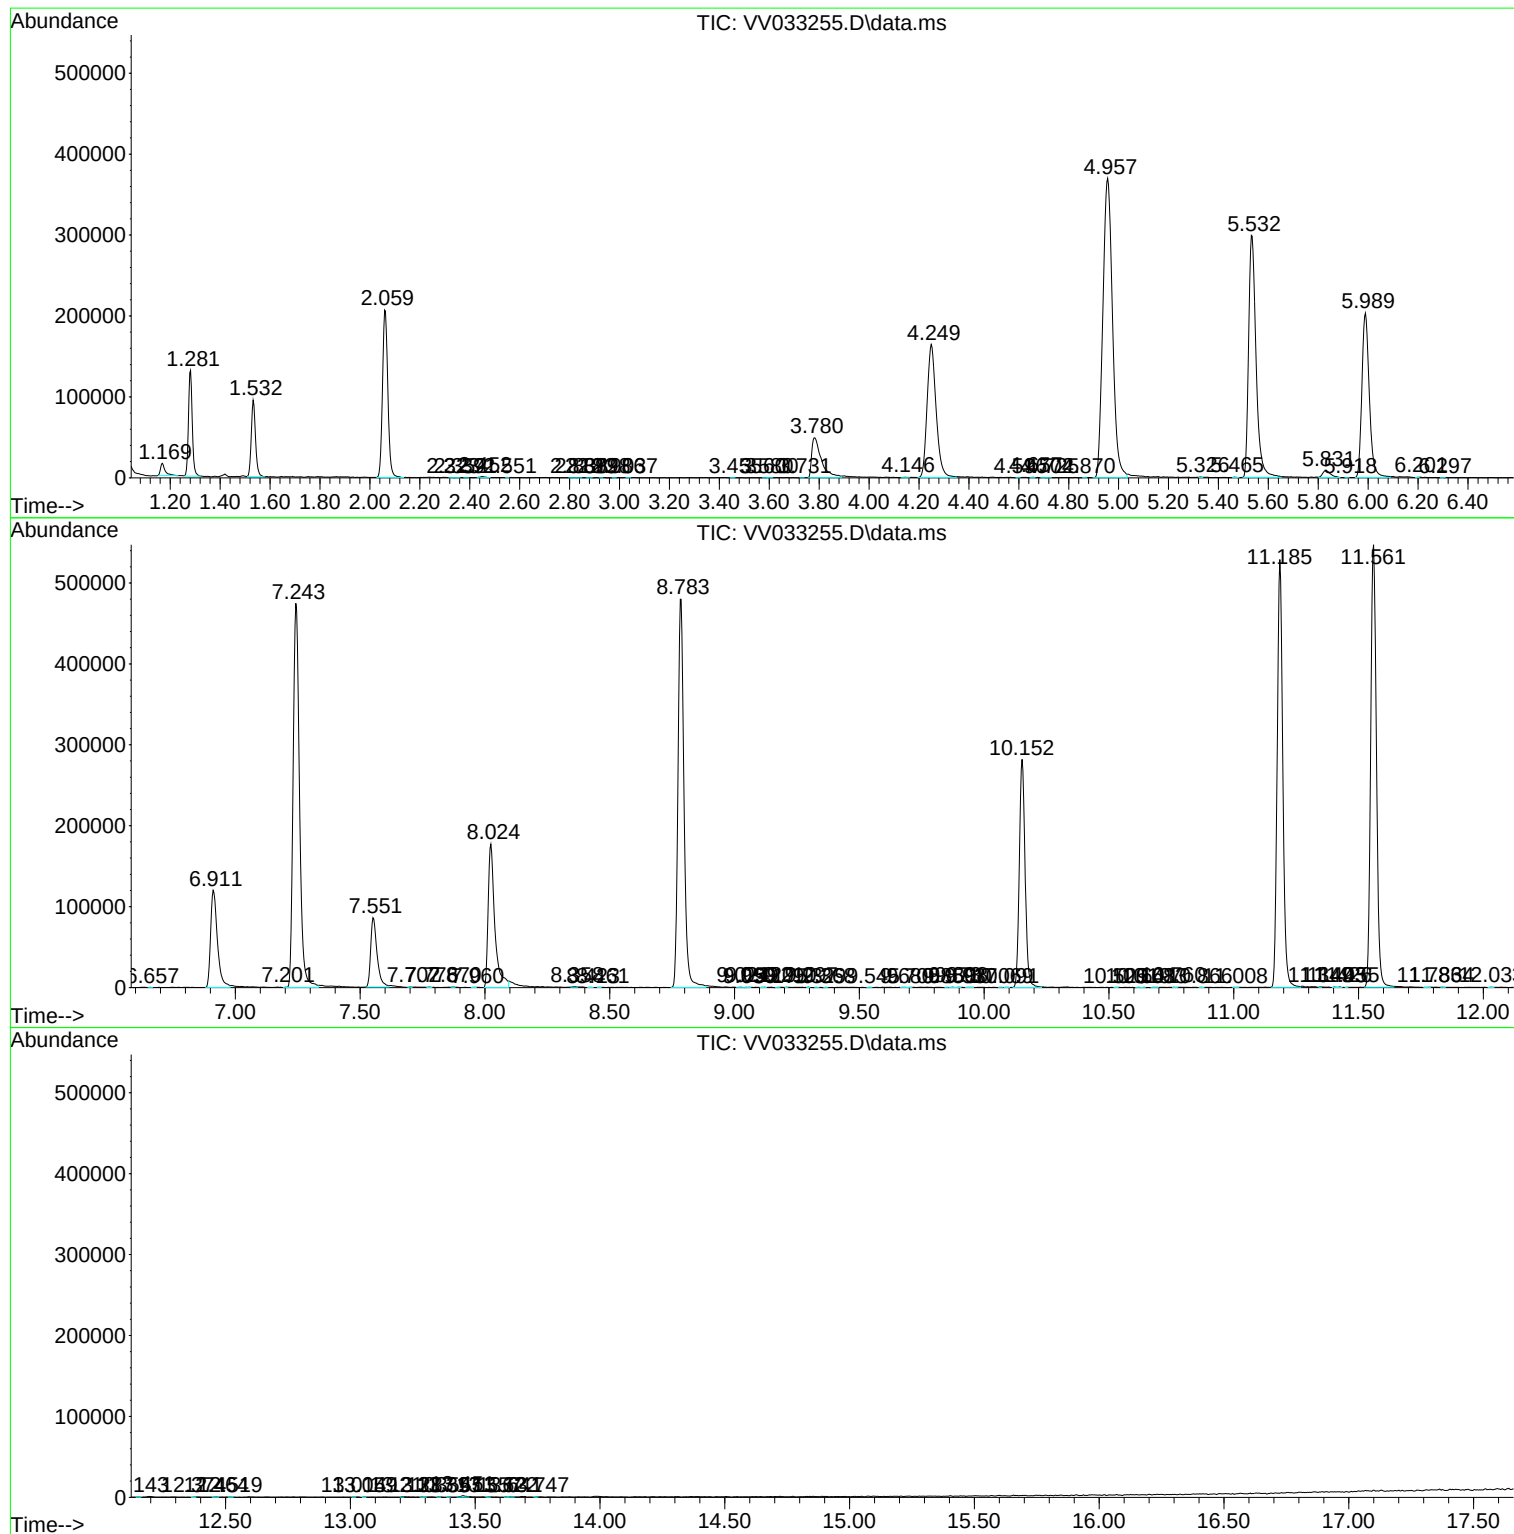

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033255.D
Acq On : 12 Dec 2023 11:47
Operator : SY/MD
Sample : VV1212WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033255.D
Acq On : 12 Dec 2023 11:47
Operator : SY/MD
Sample : VV1212WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc