

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033258.D
 Acq On : 12 Dec 2023 12:57
 Operator : SY/MD
 Sample : 05751-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	34	40	55	rBV	13813	18470	1.92%	0.250%
2	1.278	68	74	92	rVB	130526	138375	14.38%	1.870%
3	1.420	114	118	124	rVB5	3205	2988	0.31%	0.040%
4	1.532	146	153	169	rVB	101589	115709	12.02%	1.564%
5	2.060	306	317	331	rBV	203409	298673	31.04%	4.037%
6	2.275	383	384	388	rVB2	353	174	0.02%	0.002%
7	2.330	394	401	403	rBV	380	334	0.03%	0.005%
8	2.375	413	415	419	rBV2	357	249	0.03%	0.003%
9	2.452	433	439	450	rVB4	786	1135	0.12%	0.015%
10	2.558	470	472	475	rVV2	376	203	0.02%	0.003%
11	2.597	481	484	488	rVB2	263	211	0.02%	0.003%
12	2.812	548	551	556	rBB	377	320	0.03%	0.004%
13	2.847	557	562	566	rBV2	297	341	0.04%	0.005%
14	2.915	580	583	588	rVB2	302	305	0.03%	0.004%
15	2.950	588	594	596	rBV2	403	389	0.04%	0.005%
16	2.973	596	601	603	rVV2	262	258	0.03%	0.003%
17	3.021	613	616	618	rBV	295	202	0.02%	0.003%
18	3.079	631	634	637	rBV2	246	179	0.02%	0.002%
19	3.159	655	659	662	rBV2	338	359	0.04%	0.005%
20	3.230	678	681	684	rVB2	252	197	0.02%	0.003%
21	3.259	685	690	691	rBV	270	240	0.02%	0.003%
22	3.310	703	706	709	rBV2	274	232	0.02%	0.003%
23	3.391	728	731	736	rVB	338	299	0.03%	0.004%
24	3.433	740	744	745	rBV	294	213	0.02%	0.003%
25	3.670	817	818	824	rBB2	330	263	0.03%	0.004%
26	3.716	830	832	836	rBB2	276	174	0.02%	0.002%
27	3.783	843	853	882	rBV	47969	128658	13.37%	1.739%
28	4.249	983	998	1034	rBV	159099	401439	41.72%	5.426%
29	4.539	1085	1088	1090	rBV2	365	248	0.03%	0.003%
30	4.625	1113	1115	1121	rBV3	472	433	0.04%	0.006%
31	4.783	1160	1164	1167	rVB2	249	177	0.02%	0.002%
32	4.815	1167	1174	1176	rVB2	316	305	0.03%	0.004%
33	4.957	1201	1218	1248	rBV2	362064	962330	100.00%	13.006%
34	5.265	1313	1314	1317	rBV2	407	191	0.02%	0.003%
35	5.310	1325	1328	1330	rBV	266	183	0.02%	0.002%
36	5.535	1385	1398	1425	rBV	283313	588758	61.18%	7.957%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033258.D
 Acq On : 12 Dec 2023 12:57
 Operator : SY/MD
 Sample : 05751-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.831	1480	1490	1512	rVB3	10052	22517	2.34%	0.304%
38	5.989	1525	1539	1560	rBV	198350	405912	42.18%	5.486%
39	6.230	1612	1614	1617	rVB2	550	254	0.03%	0.003%
40	6.268	1623	1626	1630	rBV2	252	180	0.02%	0.002%
41	6.577	1718	1722	1724	rBV2	275	215	0.02%	0.003%
42	6.596	1724	1728	1731	rVB	288	282	0.03%	0.004%
43	6.622	1731	1736	1739	rBV	341	304	0.03%	0.004%
44	6.799	1787	1791	1793	rBV2	308	231	0.02%	0.003%
45	6.876	1809	1815	1816	rBV	433	459	0.05%	0.006%
46	6.912	1816	1826	1852	rVV	116546	218106	22.66%	2.948%
47	7.137	1894	1896	1897	rBV	359	168	0.02%	0.002%
48	7.182	1908	1910	1916	rVB2	479	327	0.03%	0.004%
49	7.243	1916	1929	1959	rBV	469454	816757	84.87%	11.039%
50	7.551	2016	2025	2053	rBV	85320	154062	16.01%	2.082%
51	7.747	2085	2086	2092	rVB	329	292	0.03%	0.004%
52	7.780	2093	2096	2098	rBV	404	278	0.03%	0.004%
53	7.802	2101	2103	2108	rVB2	387	270	0.03%	0.004%
54	7.873	2115	2125	2136	rBV4	3702	6827	0.71%	0.092%
55	8.024	2162	2172	2206	rBV	172205	334405	34.75%	4.520%
56	8.323	2263	2265	2270	rVB2	496	327	0.03%	0.004%
57	8.391	2281	2286	2288	rBV2	464	435	0.05%	0.006%
58	8.490	2312	2317	2319	rVB2	299	194	0.02%	0.003%
59	8.670	2367	2373	2376	rVB2	233	221	0.02%	0.003%
60	8.738	2389	2394	2396	rBV2	200	231	0.02%	0.003%
61	8.783	2397	2408	2436	rBV	452926	745356	77.45%	10.074%
62	9.108	2506	2509	2511	rBV	519	236	0.02%	0.003%
63	9.124	2512	2514	2519	rVV2	349	211	0.02%	0.003%
64	9.365	2581	2589	2593	rBV2	254	401	0.04%	0.005%
65	9.522	2634	2638	2640	rBV	232	211	0.02%	0.003%
66	9.577	2653	2655	2658	rVV	272	189	0.02%	0.003%
67	9.622	2665	2669	2672	rBV	285	216	0.02%	0.003%
68	9.738	2703	2705	2710	rVB2	244	178	0.02%	0.002%
69	9.796	2720	2723	2725	rBV2	311	269	0.03%	0.004%
70	9.815	2727	2729	2733	rVV2	234	187	0.02%	0.003%
71	9.902	2752	2756	2760	rBV2	417	298	0.03%	0.004%
72	10.153	2822	2834	2857	rBV	275055	433964	45.10%	5.865%
73	10.326	2881	2888	2900	rVB3	4600	6688	0.69%	0.090%
74	10.387	2901	2907	2911	rBV	278	243	0.03%	0.003%
75	10.529	2947	2951	2958	rBV2	288	351	0.04%	0.005%
76	10.638	2982	2985	2990	rBB2	168	169	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033258.D
 Acq On : 12 Dec 2023 12:57
 Operator : SY/MD
 Sample : 05751-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.718	3006	3010	3013	rBV	239	208	0.02%	0.003%
78	10.924	3072	3074	3075	rBV	449	230	0.02%	0.003%
79	11.014	3098	3102	3105	rBV	243	196	0.02%	0.003%
80	11.120	3133	3135	3136	rBV2	410	175	0.02%	0.002%
81	11.185	3142	3155	3181	rBV	489547	757406	78.71%	10.236%
82	11.561	3260	3272	3293	rBV	522522	818527	85.06%	11.063%
83	11.776	3334	3339	3344	rBV4	402	424	0.04%	0.006%
84	11.802	3344	3347	3348	rBV	344	191	0.02%	0.003%
85	12.323	3507	3509	3512	rBV3	280	196	0.02%	0.003%
86	12.378	3525	3526	3532	rBV2	247	210	0.02%	0.003%
87	12.432	3540	3543	3546	rBV	248	197	0.02%	0.003%
88	12.561	3580	3583	3586	rBV	232	178	0.02%	0.002%
89	12.590	3589	3592	3593	rBV2	311	219	0.02%	0.003%
90	12.931	3695	3698	3702	rBV2	267	269	0.03%	0.004%
91	13.172	3768	3773	3775	rBV	350	292	0.03%	0.004%
92	13.188	3775	3778	3779	rBV	299	191	0.02%	0.003%
93	13.535	3882	3886	3887	rBV2	405	241	0.03%	0.003%
94	13.548	3887	3890	3895	rVB2	604	471	0.05%	0.006%
95	13.644	3917	3920	3923	rBV2	361	307	0.03%	0.004%
96	13.689	3929	3934	3940	rVB5	1093	1371	0.14%	0.019%
97	13.722	3940	3944	3946	rBV2	749	587	0.06%	0.008%
98	14.095	4058	4060	4062	rBV	369	213	0.02%	0.003%
99	14.255	4106	4110	4111	rBV2	496	310	0.03%	0.004%
100	14.355	4137	4141	4146	rBV5	684	829	0.09%	0.011%




Sum of corrected areas: 7399073

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033258.D
Acq On : 12 Dec 2023 12:57
Operator : SY/MD
Sample : 05751-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

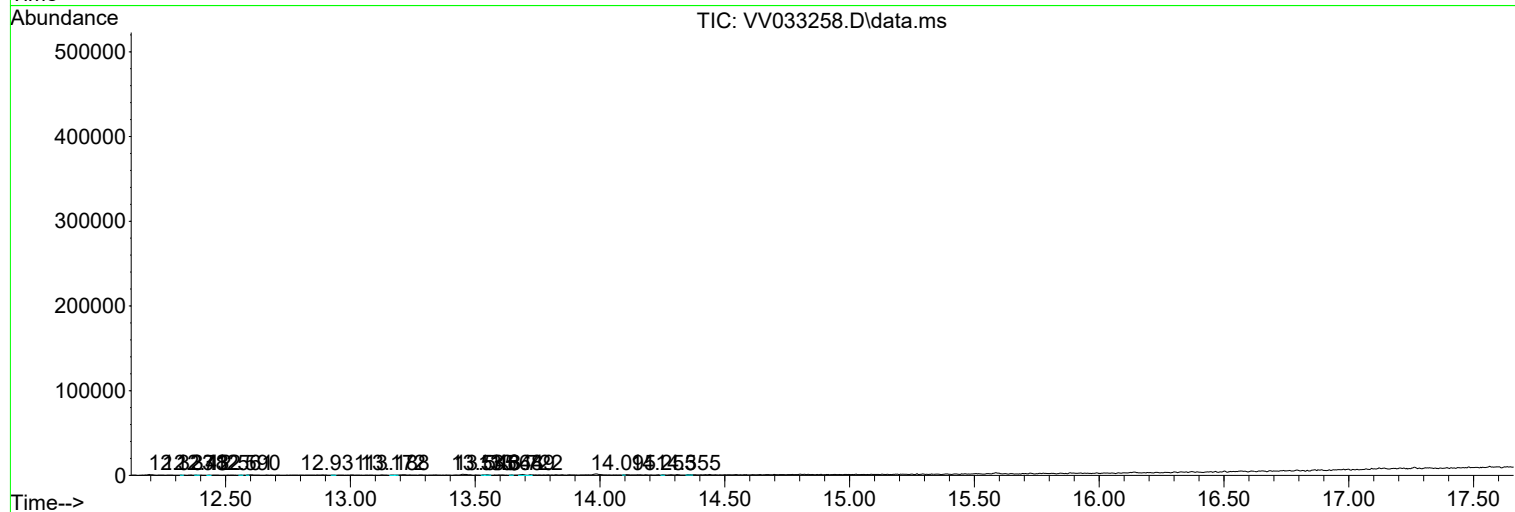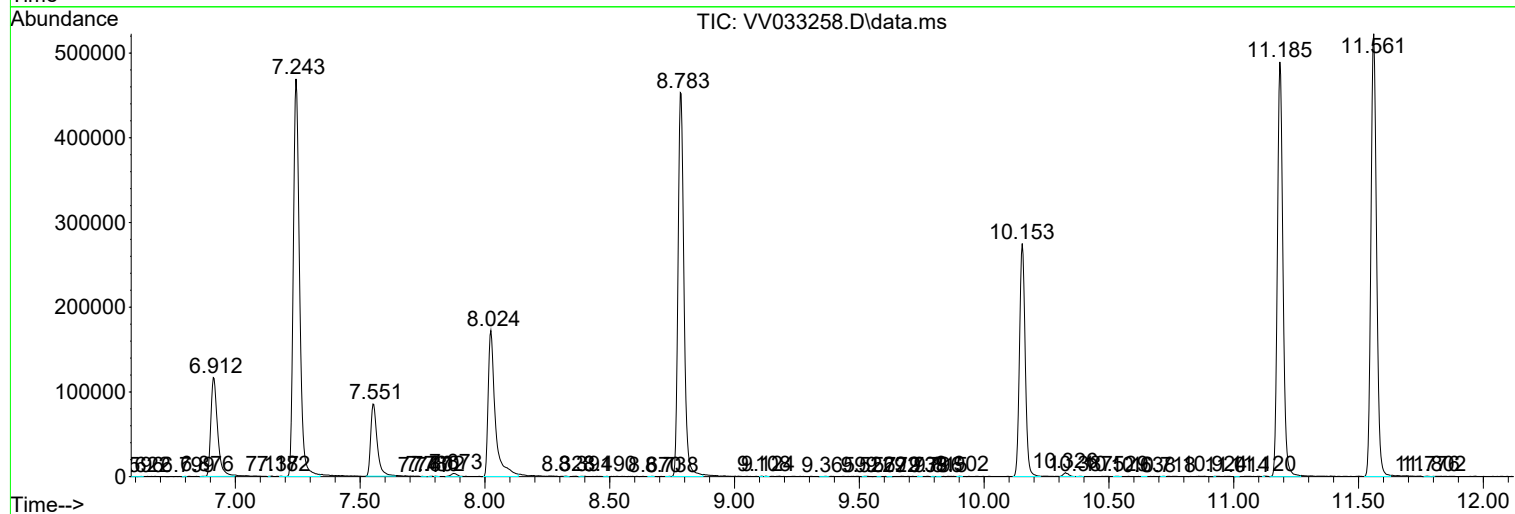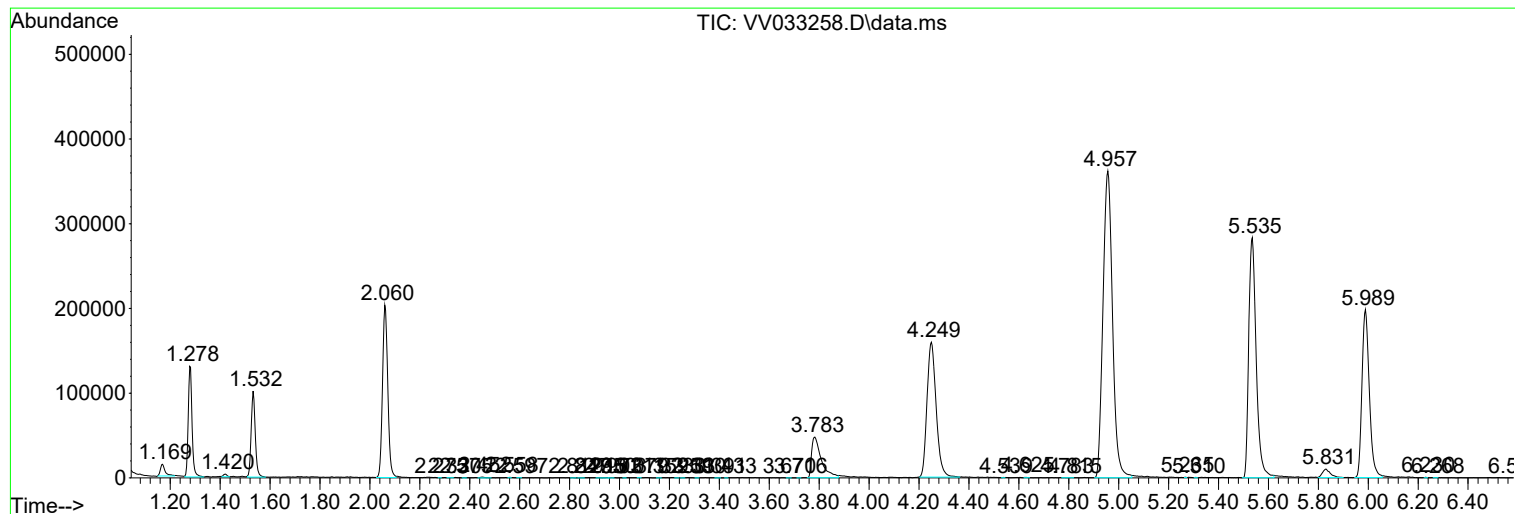

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033258.D
Acq On : 12 Dec 2023 12:57
Operator : SY/MD
Sample : 05751-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033258.D
Acq On : 12 Dec 2023 12:57
Operator : SY/MD
Sample : 05751-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------