

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033259.D
 Acq On : 12 Dec 2023 13:20
 Operator : SY/MD
 Sample : 05752-04 20X
 Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	108456	114238	4.31%	1.277%
2	1.436	111	123	128	rVB5	10505	13197	0.50%	0.148%
3	1.529	145	152	166	rVB	77023	91883	3.47%	1.027%
4	2.059	306	317	335	rBV	172504	251108	9.48%	2.808%
5	2.220	363	367	368	rBV3	277	217	0.01%	0.002%
6	2.387	414	419	422	rBV2	457	506	0.02%	0.006%
7	2.494	445	452	453	rBV2	256	275	0.01%	0.003%
8	2.561	460	473	478	rBV4	1973	3695	0.14%	0.041%
9	2.706	515	518	525	rVB2	351	419	0.02%	0.005%
10	2.773	536	539	543	rVB2	356	281	0.01%	0.003%
11	2.796	544	546	549	rBV2	271	177	0.01%	0.002%
12	2.860	561	566	568	rBV2	343	341	0.01%	0.004%
13	2.918	581	584	587	rBV	201	169	0.01%	0.002%
14	3.040	619	622	625	rBV2	302	248	0.01%	0.003%
15	3.098	635	640	643	rVB2	216	189	0.01%	0.002%
16	3.339	711	715	718	rBV2	241	195	0.01%	0.002%
17	3.407	732	736	738	rBV	238	190	0.01%	0.002%
18	3.439	743	746	749	rVV2	264	195	0.01%	0.002%
19	3.471	753	756	759	rBV	277	218	0.01%	0.002%
20	3.693	820	825	827	rBV	358	279	0.01%	0.003%
21	3.783	843	853	884	rBV	38078	105587	3.99%	1.181%
22	4.249	982	998	1027	rBV2	130999	336377	12.70%	3.761%
23	4.535	1084	1087	1089	rBV	210	164	0.01%	0.002%
24	4.564	1094	1096	1099	rVB	405	164	0.01%	0.002%
25	4.606	1105	1109	1112	rBV3	444	308	0.01%	0.003%
26	4.625	1112	1115	1118	rBV2	411	235	0.01%	0.003%
27	4.847	1180	1184	1191	rBV2	340	477	0.02%	0.005%
28	4.882	1191	1195	1200	rVB2	286	265	0.01%	0.003%
29	4.956	1201	1218	1250	rBV2	298952	802369	30.30%	8.972%
30	5.349	1337	1340	1342	rBV	483	218	0.01%	0.002%
31	5.407	1354	1358	1361	rBV3	360	239	0.01%	0.003%
32	5.442	1367	1369	1373	rBV	456	306	0.01%	0.003%
33	5.464	1373	1376	1379	rVB2	495	258	0.01%	0.003%
34	5.484	1380	1382	1385	rBV	367	260	0.01%	0.003%
35	5.532	1385	1397	1433	rBV	289231	599064	22.62%	6.699%
36	5.828	1482	1489	1500	rBV8	5120	10101	0.38%	0.113%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033259.D
 Acq On : 12 Dec 2023 13:20
 Operator : SY/MD
 Sample : 05752-04 20X
 Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.989	1526	1539	1558	rBV	161202	332988	12.58%	3.723%
38	6.223	1609	1612	1614	rBV	433	282	0.01%	0.003%
39	6.259	1619	1623	1625	rVV	282	173	0.01%	0.002%
40	6.278	1626	1629	1633	rVV2	500	265	0.01%	0.003%
41	6.323	1638	1643	1645	rBV2	368	277	0.01%	0.003%
42	6.461	1681	1686	1688	rVV2	182	193	0.01%	0.002%
43	6.554	1712	1715	1719	rBV2	300	216	0.01%	0.002%
44	6.828	1798	1800	1804	rVV	247	211	0.01%	0.002%
45	6.915	1816	1827	1845	rBV2	98114	183109	6.92%	2.048%
46	7.188	1909	1912	1914	rBV2	369	271	0.01%	0.003%
47	7.243	1917	1929	1953	rBV	381673	674406	25.47%	7.541%
48	7.500	2006	2009	2013	rBV2	466	312	0.01%	0.003%
49	7.554	2017	2026	2047	rBV	70214	123015	4.65%	1.376%
50	8.024	2159	2172	2214	rBV	138489	270068	10.20%	3.020%
51	8.538	2327	2332	2333	rBV	367	270	0.01%	0.003%
52	8.651	2363	2367	2370	rBV2	254	208	0.01%	0.002%
53	8.709	2381	2385	2389	rBV	226	166	0.01%	0.002%
54	8.786	2398	2409	2432	rBV	464891	842030	31.80%	9.416%
55	9.040	2484	2488	2491	rBV2	307	247	0.01%	0.003%
56	9.213	2538	2542	2545	rBB2	407	336	0.01%	0.004%
57	9.403	2597	2601	2603	rBV	342	258	0.01%	0.003%
58	9.464	2617	2620	2623	rVB2	274	209	0.01%	0.002%
59	9.500	2629	2631	2633	rVV2	540	295	0.01%	0.003%
60	9.564	2649	2651	2656	rVV	245	173	0.01%	0.002%
61	9.586	2656	2658	2662	rVV2	253	163	0.01%	0.002%
62	9.770	2711	2715	2716	rBV	212	169	0.01%	0.002%
63	9.812	2724	2728	2732	rBV2	280	295	0.01%	0.003%
64	9.834	2732	2735	2737	rVV2	239	165	0.01%	0.002%
65	10.152	2823	2834	2860	rVV	229504	362634	13.69%	4.055%
66	10.255	2864	2866	2870	rVB2	489	338	0.01%	0.004%
67	10.278	2870	2873	2877	rVB2	278	210	0.01%	0.002%
68	10.326	2883	2888	2898	rVB3	1229	1454	0.05%	0.016%
69	10.397	2905	2910	2913	rBV	228	254	0.01%	0.003%
70	10.567	2959	2963	2964	rBV	305	233	0.01%	0.003%
71	10.651	2986	2989	2993	rBV	293	251	0.01%	0.003%
72	10.712	3005	3008	3012	rVB2	188	172	0.01%	0.002%
73	10.763	3021	3024	3027	rVB2	257	163	0.01%	0.002%
74	10.844	3046	3049	3051	rBV	306	168	0.01%	0.002%
75	10.985	3090	3093	3095	rBV	327	181	0.01%	0.002%
76	11.078	3118	3122	3126	rVB2	377	376	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033259.D
 Acq On : 12 Dec 2023 13:20
 Operator : SY/MD
 Sample : 05752-04 20X
 Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.123	3126	3136	3145	rBV3	25266	40461	1.53%	0.452%
78	11.207	3145	3162	3189	rVV2	1262624	2647942	100.00%	29.609%
79	11.561	3260	3272	3296	rBV2	499098	977250	36.91%	10.928%
80	12.101	3438	3440	3444	rBV3	280	241	0.01%	0.003%
81	12.191	3460	3468	3470	rBV2	1124	1251	0.05%	0.014%
82	12.319	3504	3508	3511	rBV2	392	362	0.01%	0.004%
83	12.493	3560	3562	3565	rBV2	264	207	0.01%	0.002%
84	12.586	3589	3591	3597	rVB2	500	506	0.02%	0.006%
85	12.670	3615	3617	3621	rBV2	295	223	0.01%	0.002%
86	12.692	3621	3624	3626	rBV2	276	168	0.01%	0.002%
87	12.792	3652	3655	3658	rVV2	353	212	0.01%	0.002%
88	12.879	3680	3682	3685	rVB	342	202	0.01%	0.002%
89	12.934	3696	3699	3702	rBV	198	180	0.01%	0.002%
90	13.107	3748	3753	3755	rBV	346	338	0.01%	0.004%
91	13.200	3771	3782	3795	rBV2	62259	95866	3.62%	1.072%
92	13.287	3805	3809	3811	rBV2	213	222	0.01%	0.002%
93	13.454	3859	3861	3867	rVB2	804	545	0.02%	0.006%
94	13.593	3901	3904	3905	rBV2	360	189	0.01%	0.002%
95	13.651	3919	3922	3923	rBV	407	183	0.01%	0.002%
96	13.683	3923	3932	3944	rVV3	27960	43389	1.64%	0.485%
97	13.930	4005	4009	4012	rVB2	563	527	0.02%	0.006%
98	14.072	4049	4053	4054	rBV	463	272	0.01%	0.003%
99	14.265	4111	4113	4115	rVB2	655	255	0.01%	0.003%
100	14.763	4266	4268	4270	rBV2	704	363	0.01%	0.004%




Sum of corrected areas: 8942970

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033259.D
Acq On : 12 Dec 2023 13:20
Operator : SY/MD
Sample : 05752-04 20X
Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

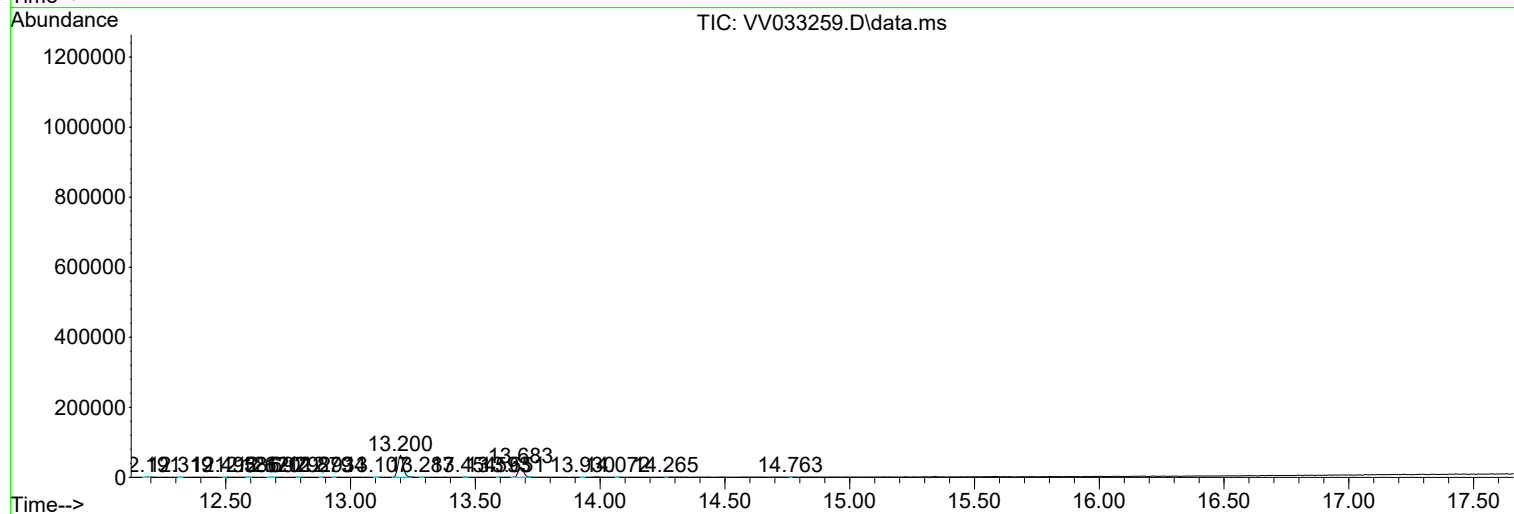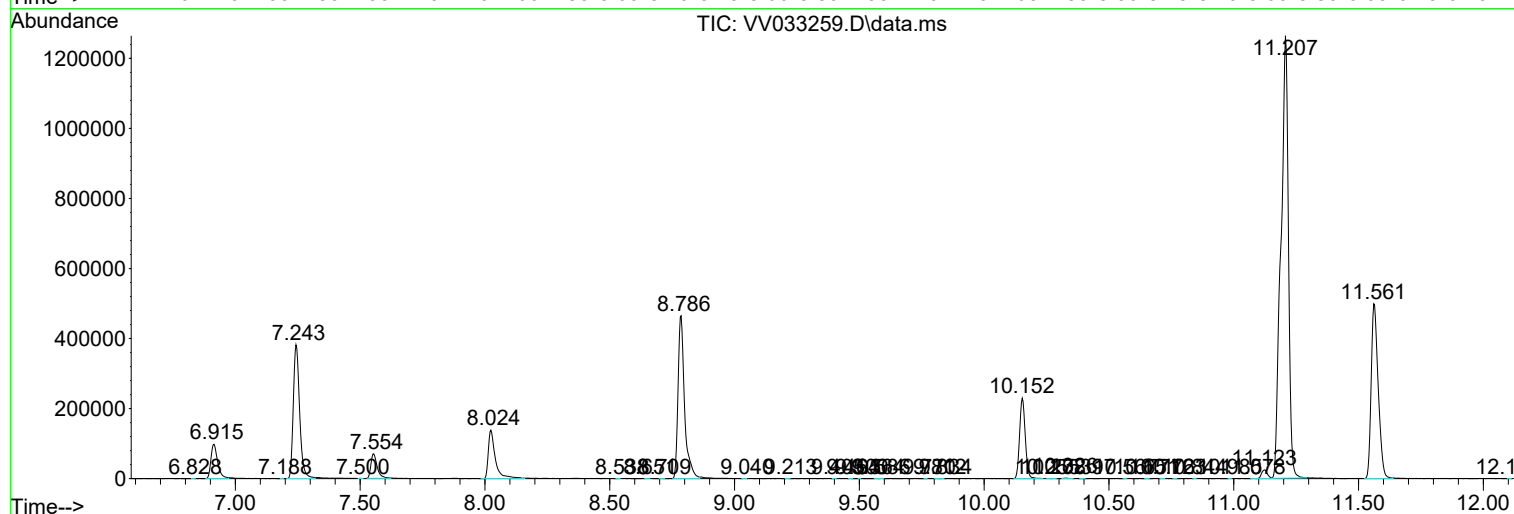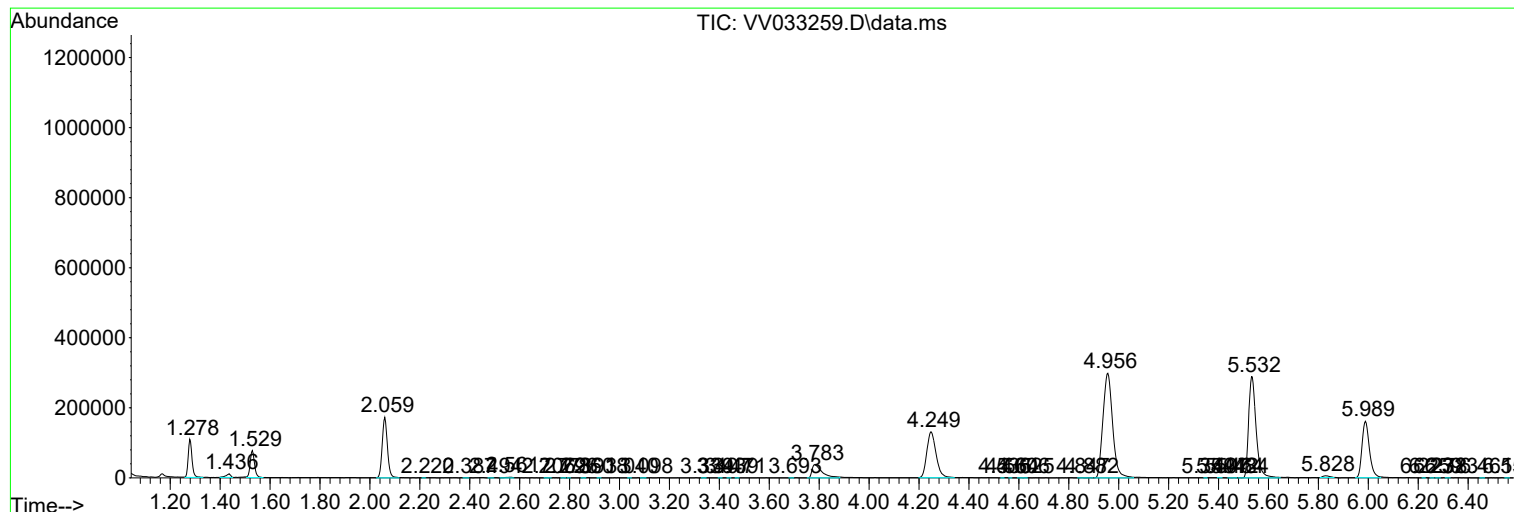

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033259.D
Acq On : 12 Dec 2023 13:20
Operator : SY/MD
Sample : 05752-04 20X
Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033259.D
Acq On : 12 Dec 2023 13:20
Operator : SY/MD
Sample : 05752-04 20X
Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc