

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033260.D
 Acq On : 12 Dec 2023 13:43
 Operator : SY/MD
 Sample : 05752-01 40X
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	35	39	47	rBV	9254	10105	0.36%	0.112%
2	1.278	68	74	88	rVB	105551	108461	3.88%	1.203%
3	1.529	145	152	167	rVB	76848	93100	3.33%	1.033%
4	1.944	277	281	285	rBV3	446	389	0.01%	0.004%
5	1.982	291	293	297	rVB	653	482	0.02%	0.005%
6	2.002	297	299	301	rBV2	674	368	0.01%	0.004%
7	2.059	307	317	341	rVB	167374	244254	8.75%	2.710%
8	2.236	368	372	379	rBV2	520	646	0.02%	0.007%
9	2.317	394	397	402	rBV	223	234	0.01%	0.003%
10	2.452	432	439	445	rBV4	1368	2055	0.07%	0.023%
11	2.564	464	474	484	rVB2	1347	2259	0.08%	0.025%
12	2.635	493	496	500	rBV2	235	203	0.01%	0.002%
13	2.719	518	522	525	rBV2	386	374	0.01%	0.004%
14	2.805	545	549	551	rVB	298	200	0.01%	0.002%
15	2.844	554	561	565	rBV2	350	527	0.02%	0.006%
16	2.979	598	603	605	rBV	365	317	0.01%	0.004%
17	3.121	643	647	650	rBV2	243	225	0.01%	0.002%
18	3.481	754	759	761	rBV	168	179	0.01%	0.002%
19	3.600	792	796	798	rVB2	310	245	0.01%	0.003%
20	3.629	799	805	808	rBV2	353	360	0.01%	0.004%
21	3.783	845	853	877	rBV	39854	103246	3.70%	1.145%
22	4.066	939	941	944	rBV2	392	272	0.01%	0.003%
23	4.249	982	998	1030	rBV2	127890	328849	11.78%	3.648%
24	4.474	1066	1068	1070	rBV	344	201	0.01%	0.002%
25	4.513	1077	1080	1083	rBV3	518	363	0.01%	0.004%
26	4.587	1099	1103	1111	rVB2	454	634	0.02%	0.007%
27	4.622	1111	1114	1116	rBV	293	187	0.01%	0.002%
28	4.702	1136	1139	1141	rBV2	422	266	0.01%	0.003%
29	4.789	1162	1166	1171	rVV2	244	226	0.01%	0.003%
30	4.957	1202	1218	1230	rBV3	296237	793180	28.40%	8.799%
31	5.307	1324	1327	1330	rBV2	566	369	0.01%	0.004%
32	5.477	1375	1380	1383	rBV3	382	379	0.01%	0.004%
33	5.535	1387	1398	1421	rBV	280525	574228	20.56%	6.370%
34	5.834	1482	1491	1511	rVV4	5663	13144	0.47%	0.146%
35	5.989	1526	1539	1563	rBV	159466	329855	11.81%	3.659%
36	6.223	1609	1612	1616	rBV2	282	223	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033260.D
 Acq On : 12 Dec 2023 13:43
 Operator : SY/MD
 Sample : 05752-01 40X
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.252	1619	1621	1624	rVV2	609	286	0.01%	0.003%
38	6.407	1664	1669	1674	rBV2	425	492	0.02%	0.005%
39	6.638	1739	1741	1743	rBV	429	217	0.01%	0.002%
40	6.911	1816	1826	1852	rBV2	96210	179743	6.44%	1.994%
41	7.098	1880	1884	1888	rVB3	572	395	0.01%	0.004%
42	7.153	1899	1901	1905	rVB	424	280	0.01%	0.003%
43	7.243	1918	1929	1955	rBV	385492	667540	23.91%	7.405%
44	7.554	2016	2026	2043	rBV	69991	124357	4.45%	1.380%
45	7.776	2093	2095	2097	rBV	265	185	0.01%	0.002%
46	7.918	2136	2139	2143	rBV	372	399	0.01%	0.004%
47	7.992	2160	2162	2164	rBV2	425	290	0.01%	0.003%
48	8.024	2164	2172	2207	rVV	137272	260442	9.33%	2.889%
49	8.371	2270	2280	2285	rBV3	1009	1301	0.05%	0.014%
50	8.458	2305	2307	2311	rVB2	401	283	0.01%	0.003%
51	8.484	2312	2315	2317	rBV	301	208	0.01%	0.002%
52	8.583	2342	2346	2349	rBV	279	271	0.01%	0.003%
53	8.718	2386	2388	2391	rBV2	359	182	0.01%	0.002%
54	8.812	2398	2417	2439	rBV2	1275268	2792439	100.00%	30.978%
55	9.046	2488	2490	2493	rVB2	422	184	0.01%	0.002%
56	9.185	2529	2533	2537	rBV2	214	202	0.01%	0.002%
57	9.246	2549	2552	2555	rBV2	392	308	0.01%	0.003%
58	9.268	2557	2559	2561	rVB	443	197	0.01%	0.002%
59	9.390	2591	2597	2598	rBV2	271	293	0.01%	0.003%
60	9.516	2630	2636	2639	rBV2	294	284	0.01%	0.003%
61	9.551	2644	2647	2650	rVB2	261	187	0.01%	0.002%
62	9.632	2669	2672	2675	rBV2	353	309	0.01%	0.003%
63	9.667	2681	2683	2690	rBV3	378	362	0.01%	0.004%
64	9.728	2698	2702	2704	rBV	558	394	0.01%	0.004%
65	9.847	2735	2739	2741	rBV	281	220	0.01%	0.002%
66	9.911	2757	2759	2764	rVB2	348	276	0.01%	0.003%
67	10.088	2810	2814	2817	rBV	210	239	0.01%	0.003%
68	10.152	2823	2834	2856	rBV	225718	355190	12.72%	3.940%
69	10.326	2883	2888	2892	rBV4	390	431	0.02%	0.005%
70	10.368	2896	2901	2909	rVB4	1577	1826	0.07%	0.020%
71	10.529	2949	2951	2959	rVB2	243	222	0.01%	0.002%
72	10.972	3085	3089	3093	rBV2	196	184	0.01%	0.002%
73	11.123	3125	3136	3145	rBV4	9612	15393	0.55%	0.171%
74	11.188	3145	3156	3185	rVB2	512686	1160839	41.57%	12.878%
75	11.561	3261	3272	3296	rBV	449489	728099	26.07%	8.077%
76	11.731	3322	3325	3331	rVB	760	669	0.02%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033260.D
 Acq On : 12 Dec 2023 13:43
 Operator : SY/MD
 Sample : 05752-01 40X
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.763	3332	3335	3338	rBV2	394	286	0.01%	0.003%
78	11.783	3338	3341	3344	rVV	551	382	0.01%	0.004%
79	11.815	3348	3351	3353	rBV	270	182	0.01%	0.002%
80	12.143	3450	3453	3457	rBV	319	282	0.01%	0.003%
81	12.197	3463	3470	3477	rVB3	1057	1638	0.06%	0.018%
82	12.233	3477	3481	3484	rBV2	309	233	0.01%	0.003%
83	12.297	3499	3501	3503	rBV	279	184	0.01%	0.002%
84	12.586	3585	3591	3596	rBV5	2268	2495	0.09%	0.028%
85	12.628	3602	3604	3608	rBV2	423	323	0.01%	0.004%
86	12.792	3652	3655	3659	rBV2	247	253	0.01%	0.003%
87	12.963	3704	3708	3710	rBV2	327	257	0.01%	0.003%
88	13.037	3729	3731	3733	rBV	323	209	0.01%	0.002%
89	13.133	3759	3761	3763	rBV	349	189	0.01%	0.002%
90	13.201	3772	3782	3799	rBV	41938	65760	2.35%	0.730%
91	13.300	3811	3813	3817	rBV	397	291	0.01%	0.003%
92	13.390	3836	3841	3846	rBV4	552	568	0.02%	0.006%
93	13.451	3857	3860	3866	rBV3	839	910	0.03%	0.010%
94	13.512	3876	3879	3881	rBV	466	268	0.01%	0.003%
95	13.683	3923	3932	3947	rBV2	18893	30670	1.10%	0.340%
96	13.988	4021	4027	4030	rBV4	1132	1208	0.04%	0.013%
97	14.419	4159	4161	4164	rBV2	578	361	0.01%	0.004%
98	14.493	4182	4184	4187	rVB2	545	231	0.01%	0.003%
99	14.898	4306	4310	4313	rBV2	507	507	0.02%	0.006%
100	15.226	4411	4412	4414	rBV2	710	381	0.01%	0.004%




Sum of corrected areas: 9014291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033260.D
Acq On : 12 Dec 2023 13:43
Operator : SY/MD
Sample : 05752-01 40X
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

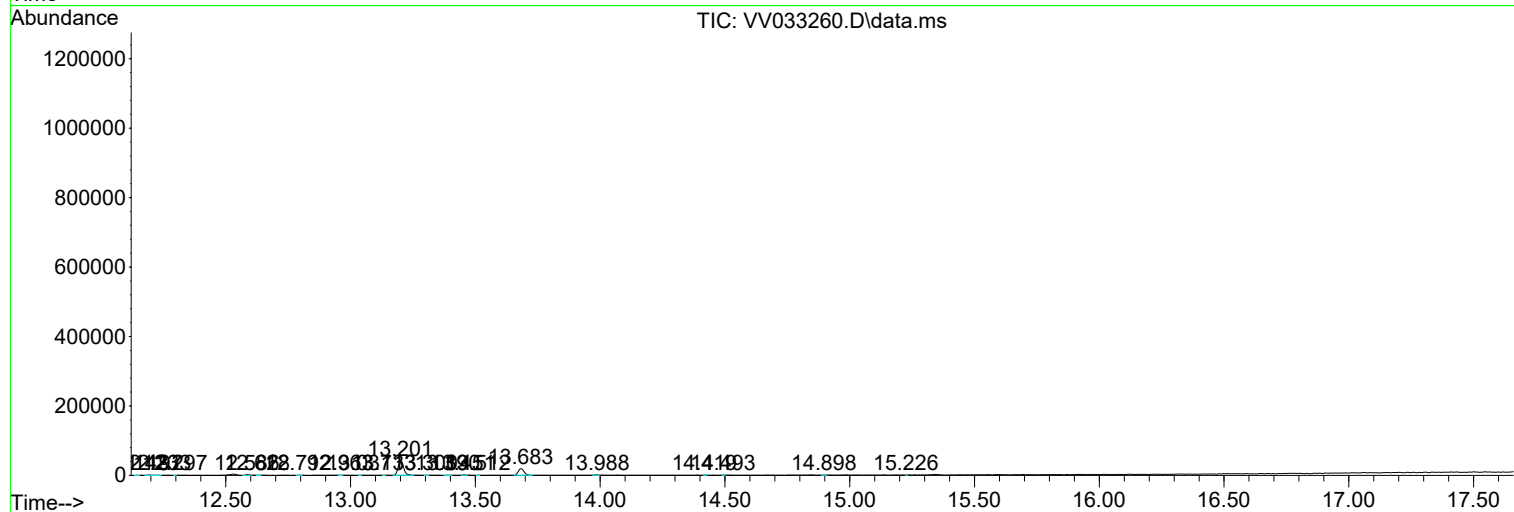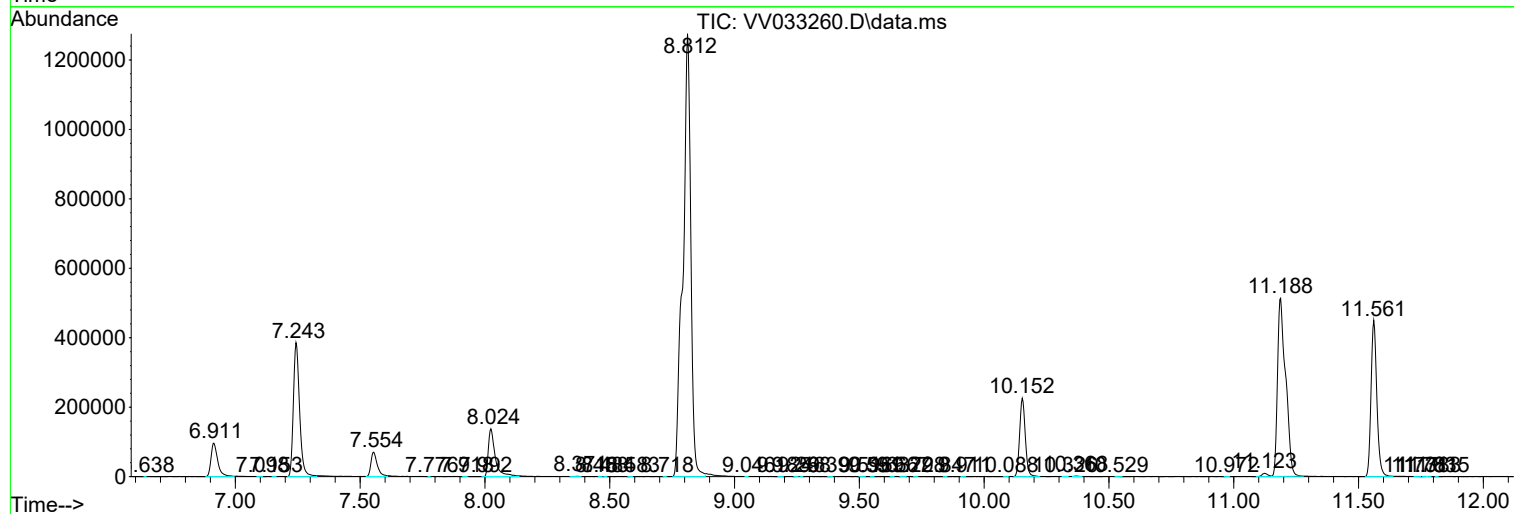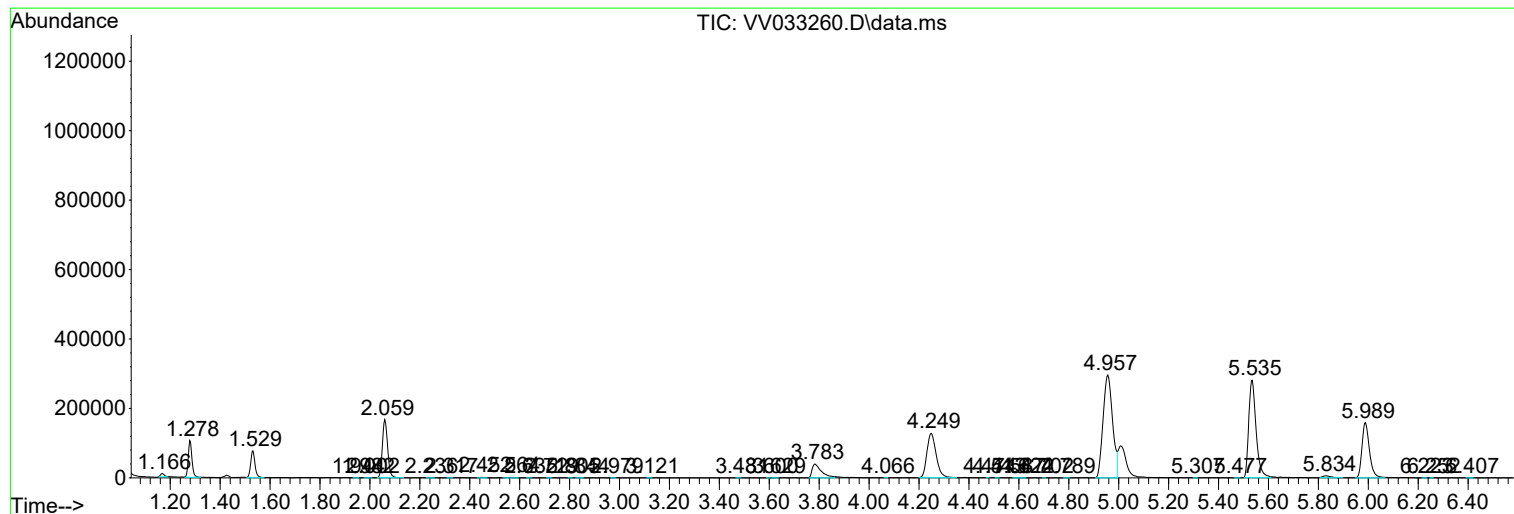

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033260.D
Acq On : 12 Dec 2023 13:43
Operator : SY/MD
Sample : 05752-01 40X
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033260.D
Acq On : 12 Dec 2023 13:43
Operator : SY/MD
Sample : 05752-01 40X
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc