

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033261.D
 Acq On : 12 Dec 2023 14:06
 Operator : SY/MD
 Sample : 05750-01 40X
 Misc : 5.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	35	39	58	rVB	8324	11500	1.45%	0.172%
2	1.278	68	74	89	rVB	106748	111007	13.98%	1.661%
3	1.529	145	152	166	rVB	76430	90729	11.42%	1.358%
4	1.967	284	288	292	rBV2	435	422	0.05%	0.006%
5	2.060	307	317	337	rVB	170670	249154	31.37%	3.729%
6	2.163	345	349	351	rBV	367	192	0.02%	0.003%
7	2.388	417	419	422	rBB2	351	196	0.02%	0.003%
8	2.446	432	437	451	rVB5	1149	1793	0.23%	0.027%
9	2.507	451	456	459	rBV3	401	345	0.04%	0.005%
10	2.558	464	472	477	rBV	1079	1757	0.22%	0.026%
11	2.712	516	520	523	rBB	240	179	0.02%	0.003%
12	2.732	523	526	530	rBV2	266	275	0.03%	0.004%
13	2.867	562	568	571	rBV2	356	406	0.05%	0.006%
14	2.912	579	582	584	rBV	285	172	0.02%	0.003%
15	3.169	659	662	664	rBV	265	175	0.02%	0.003%
16	3.204	670	673	676	rVB2	279	219	0.03%	0.003%
17	3.265	688	692	695	rBV2	343	327	0.04%	0.005%
18	3.343	714	716	721	rVB	276	194	0.02%	0.003%
19	3.507	762	767	768	rBV2	286	270	0.03%	0.004%
20	3.555	779	782	785	rVB2	283	185	0.02%	0.003%
21	3.748	840	842	845	rBV	258	174	0.02%	0.003%
22	3.783	845	853	883	rBV	40464	109934	13.84%	1.645%
23	4.249	981	998	1030	rVV2	129365	334954	42.17%	5.013%
24	4.474	1065	1068	1070	rBV2	306	187	0.02%	0.003%
25	4.529	1082	1085	1087	rVV3	454	258	0.03%	0.004%
26	4.555	1091	1093	1099	rVV2	472	358	0.05%	0.005%
27	4.581	1099	1101	1105	rVB2	391	218	0.03%	0.003%
28	4.645	1115	1121	1124	rBV3	294	307	0.04%	0.005%
29	4.674	1127	1130	1134	rVB	426	347	0.04%	0.005%
30	4.886	1190	1196	1199	rBV	381	335	0.04%	0.005%
31	4.957	1201	1218	1249	rBV2	296539	794215	100.00%	11.887%
32	5.217	1298	1299	1300	rBV	503	175	0.02%	0.003%
33	5.275	1315	1317	1321	rBV	304	237	0.03%	0.004%
34	5.294	1321	1323	1328	rVB	499	321	0.04%	0.005%
35	5.323	1328	1332	1334	rBV	368	257	0.03%	0.004%
36	5.410	1356	1359	1362	rBV2	247	233	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033261.D
 Acq On : 12 Dec 2023 14:06
 Operator : SY/MD
 Sample : 05750-01 40X
 Misc : 5.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.458	1369	1374	1376	rBV2	450	364	0.05%	0.005%
38	5.532	1386	1397	1425	rBV	276826	567620	71.47%	8.496%
39	5.828	1479	1489	1509	rBV9	6512	16013	2.02%	0.240%
40	5.989	1526	1539	1571	rBV2	161748	336800	42.41%	5.041%
41	6.182	1594	1599	1607	rBV4	685	854	0.11%	0.013%
42	6.490	1689	1695	1697	rBV	276	337	0.04%	0.005%
43	6.780	1782	1785	1790	rBB	311	334	0.04%	0.005%
44	6.806	1790	1793	1796	rBV	283	221	0.03%	0.003%
45	6.912	1816	1826	1853	rBV	97773	183786	23.14%	2.751%
46	7.101	1880	1885	1889	rVB2	332	374	0.05%	0.006%
47	7.243	1918	1929	1951	rBV	375503	667090	83.99%	9.985%
48	7.555	2015	2026	2047	rBV2	70513	128394	16.17%	1.922%
49	7.767	2088	2092	2095	rBV3	325	301	0.04%	0.005%
50	7.844	2114	2116	2119	rVB	408	222	0.03%	0.003%
51	7.863	2119	2122	2123	rBV	464	266	0.03%	0.004%
52	7.905	2124	2135	2156	rVV	145278	247039	31.10%	3.698%
53	8.024	2163	2172	2194	rBV	137310	253713	31.95%	3.797%
54	8.359	2271	2276	2277	rBV	601	518	0.07%	0.008%
55	8.535	2329	2331	2334	rVB2	444	183	0.02%	0.003%
56	8.558	2334	2338	2341	rBV	384	195	0.02%	0.003%
57	8.654	2364	2368	2371	rVB2	349	258	0.03%	0.004%
58	8.744	2393	2396	2397	rBV	276	170	0.02%	0.003%
59	8.783	2397	2408	2432	rBV	437604	730276	91.95%	10.930%
60	9.056	2490	2493	2497	rBV3	319	237	0.03%	0.004%
61	9.346	2580	2583	2587	rVB2	318	269	0.03%	0.004%
62	9.484	2624	2626	2630	rBV	240	197	0.02%	0.003%
63	9.516	2633	2636	2639	rVB2	298	237	0.03%	0.004%
64	9.658	2677	2680	2683	rVB	418	298	0.04%	0.004%
65	9.966	2771	2776	2778	rBB2	229	172	0.02%	0.003%
66	9.992	2779	2784	2787	rBB2	367	298	0.04%	0.004%
67	10.153	2820	2834	2858	rBV2	229115	364229	45.86%	5.452%
68	10.265	2866	2869	2874	rBV2	329	382	0.05%	0.006%
69	10.638	2981	2985	2987	rBV	369	341	0.04%	0.005%
70	10.677	2994	2997	2998	rBV	369	210	0.03%	0.003%
71	10.767	3023	3025	3028	rBV2	283	235	0.03%	0.004%
72	10.850	3046	3051	3054	rBV	355	404	0.05%	0.006%
73	10.905	3066	3068	3072	rVB	316	207	0.03%	0.003%
74	11.185	3144	3155	3178	rBV	486459	763284	96.11%	11.424%
75	11.355	3206	3208	3215	rBV3	304	308	0.04%	0.005%
76	11.419	3225	3228	3232	rVV2	348	274	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033261.D
 Acq On : 12 Dec 2023 14:06
 Operator : SY/MD
 Sample : 05750-01 40X
 Misc : 5.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.561	3260	3272	3295	rBV	439894	689886	86.86%	10.326%
78	12.001	3404	3409	3411	rBV2	336	337	0.04%	0.005%
79	12.159	3455	3458	3462	rBV	227	216	0.03%	0.003%
80	12.194	3462	3469	3477	rVV2	998	1619	0.20%	0.024%
81	12.355	3516	3519	3521	rBV2	349	233	0.03%	0.003%
82	12.403	3532	3534	3537	rVB2	390	237	0.03%	0.004%
83	12.432	3538	3543	3544	rBV3	424	356	0.04%	0.005%
84	12.645	3605	3609	3611	rVB	271	212	0.03%	0.003%
85	12.741	3635	3639	3642	rBV2	398	310	0.04%	0.005%
86	12.773	3647	3649	3653	rBV2	334	240	0.03%	0.004%
87	12.985	3711	3715	3721	rBV2	489	397	0.05%	0.006%
88	13.021	3721	3726	3733	rVB	290	351	0.04%	0.005%
89	13.072	3740	3742	3745	rVV2	364	170	0.02%	0.003%
90	13.207	3775	3784	3797	rVB7	2367	4412	0.56%	0.066%
91	13.255	3797	3799	3803	rBV2	285	211	0.03%	0.003%
92	13.284	3803	3808	3812	rBV2	720	654	0.08%	0.010%
93	13.342	3824	3826	3828	rBV2	267	172	0.02%	0.003%
94	13.529	3881	3884	3886	rBV	294	202	0.03%	0.003%
95	13.548	3887	3890	3892	rBV2	363	226	0.03%	0.003%
96	13.606	3904	3908	3911	rBV2	274	249	0.03%	0.004%
97	13.661	3919	3925	3927	rBV4	572	629	0.08%	0.009%
98	13.841	3980	3981	3986	rBV2	336	272	0.03%	0.004%
99	13.927	4004	4008	4010	rBV2	439	445	0.06%	0.007%
100	14.551	4199	4202	4204	rBV3	406	258	0.03%	0.004%

Sum of corrected areas: 6681211




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033261.D
Acq On : 12 Dec 2023 14:06
Operator : SY/MD
Sample : 05750-01 40X
Misc : 5.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

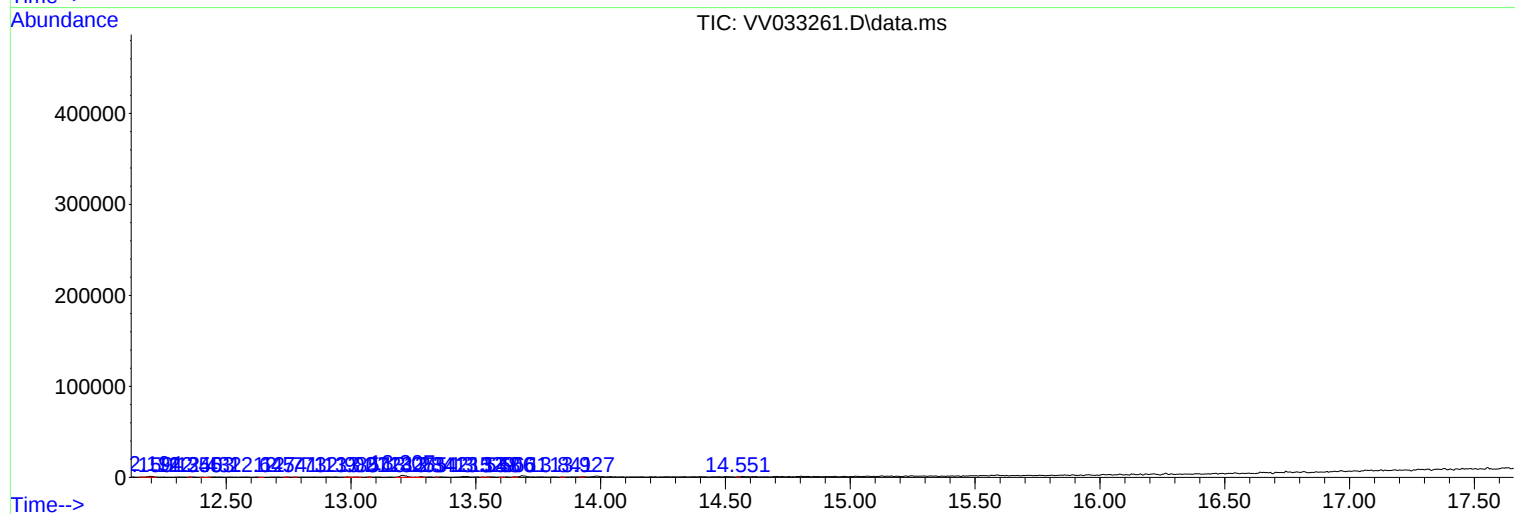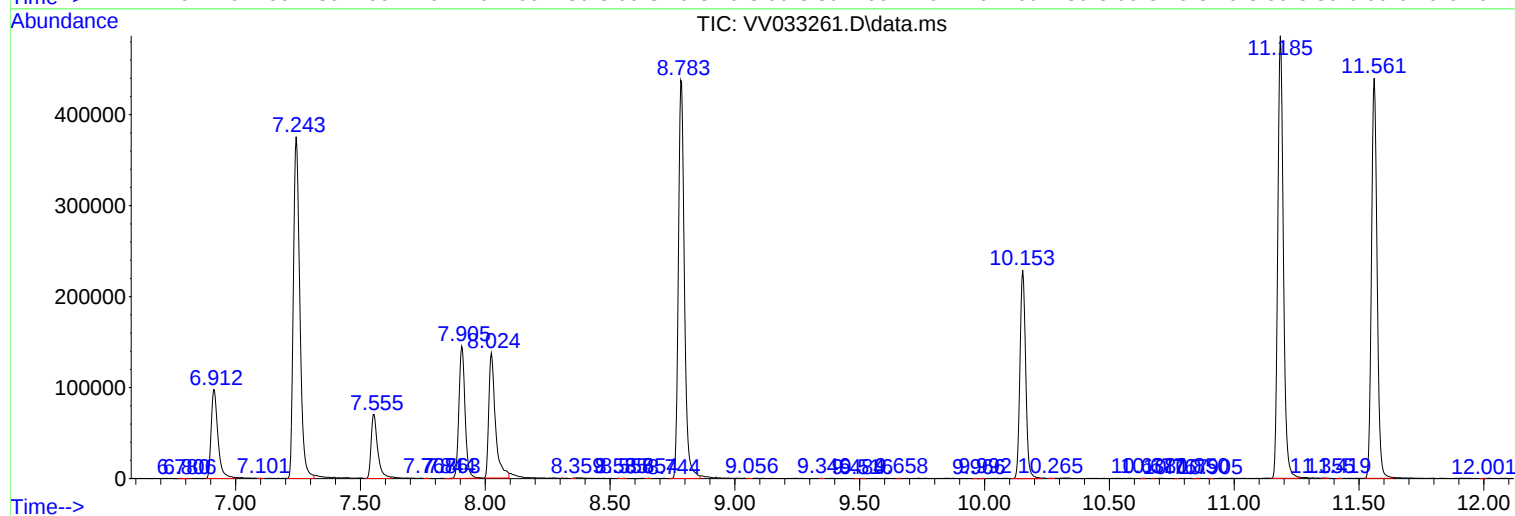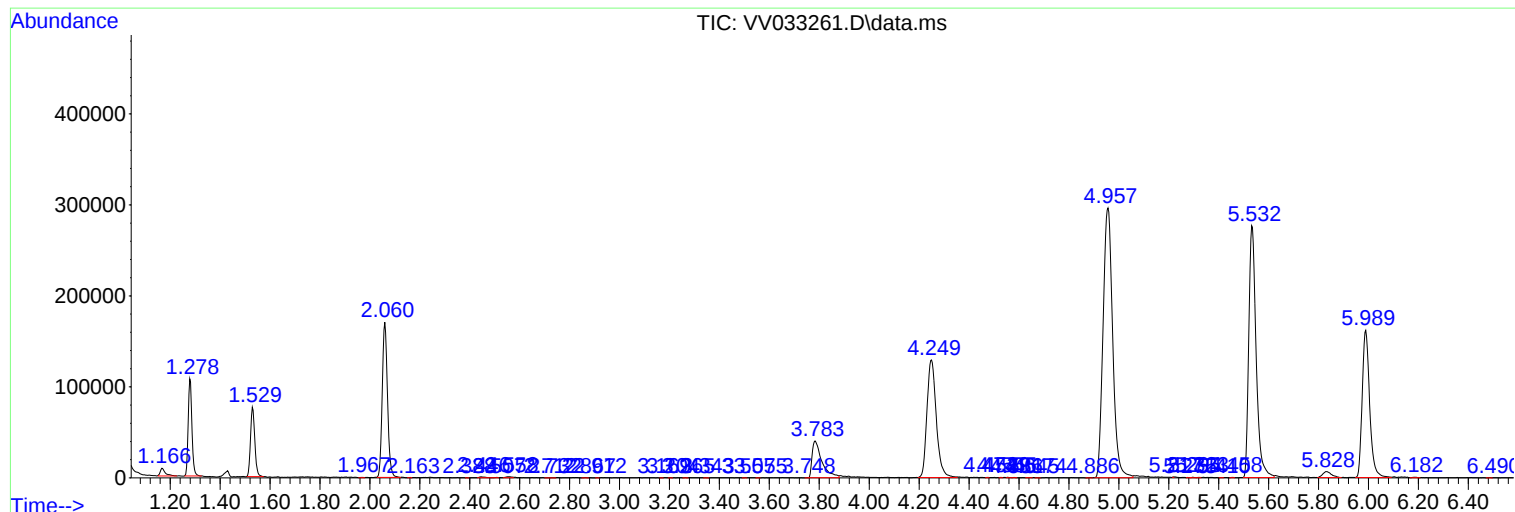

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033261.D
Acq On : 12 Dec 2023 14:06
Operator : SY/MD
Sample : 05750-01 40X
Misc : 5.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033261.D
Acq On : 12 Dec 2023 14:06
Operator : SY/MD
Sample : 05750-01 40X
Misc : 5.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------