

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033262.D
 Acq On : 12 Dec 2023 14:56
 Operator : SY/MD
 Sample : 05750-02ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	117465	146020	14.69%	1.673%
2	1.471	110	134	139	rBV	28921	92003	9.25%	1.054%
3	1.812	237	240	243	rBV2	441	377	0.04%	0.004%
4	1.947	275	282	285	rBV2	251	238	0.02%	0.003%
5	1.976	288	291	293	rBV	699	447	0.04%	0.005%
6	2.002	296	299	301	rBV3	621	353	0.04%	0.004%
7	2.043	302	312	332	rVB	225229	339225	34.12%	3.888%
8	2.214	363	365	366	rBV	355	153	0.02%	0.002%
9	2.326	397	400	403	rBV2	294	226	0.02%	0.003%
10	2.404	421	424	427	rBB2	418	249	0.03%	0.003%
11	2.445	427	437	450	rBV5	3107	5950	0.60%	0.068%
12	2.503	453	455	458	rBV2	235	176	0.02%	0.002%
13	2.555	458	471	484	rBV3	4763	10412	1.05%	0.119%
14	2.638	492	497	498	rBV3	378	255	0.03%	0.003%
15	2.683	508	511	515	rBV2	356	271	0.03%	0.003%
16	2.741	527	529	532	rBV2	427	234	0.02%	0.003%
17	2.863	565	567	571	rBV	156	147	0.01%	0.002%
18	3.056	621	627	631	rBV2	213	241	0.02%	0.003%
19	3.227	677	680	683	rBV2	206	164	0.02%	0.002%
20	3.346	714	717	720	rBV2	276	213	0.02%	0.002%
21	3.439	743	746	750	rBB2	246	204	0.02%	0.002%
22	3.461	750	753	756	rBB2	284	194	0.02%	0.002%
23	3.481	756	759	762	rBV2	249	215	0.02%	0.002%
24	3.551	779	781	785	rVB	290	179	0.02%	0.002%
25	3.793	847	856	879	rBV	26749	88840	8.94%	1.018%
26	4.243	979	996	1029	rBV	155645	419243	42.17%	4.805%
27	4.397	1039	1044	1046	rBV3	447	396	0.04%	0.005%
28	4.429	1050	1054	1057	rBV2	258	202	0.02%	0.002%
29	4.542	1086	1089	1091	rBV	365	214	0.02%	0.002%
30	4.564	1094	1096	1099	rVB2	375	190	0.02%	0.002%
31	4.635	1116	1118	1121	rVB	256	150	0.02%	0.002%
32	4.760	1155	1157	1161	rBB	220	165	0.02%	0.002%
33	4.793	1162	1167	1169	rBV	303	219	0.02%	0.003%
34	4.947	1199	1215	1245	rBV2	381459	994174	100.00%	11.394%
35	5.146	1274	1277	1278	rBV2	426	197	0.02%	0.002%
36	5.214	1295	1298	1300	rBV	527	283	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033262.D
 Acq On : 12 Dec 2023 14:56
 Operator : SY/MD
 Sample : 05750-02ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.252	1306	1310	1314	rBV2	354	277	0.03%	0.003%
38	5.323	1329	1332	1334	rBV	356	217	0.02%	0.002%
39	5.371	1345	1347	1351	rVB	289	172	0.02%	0.002%
40	5.529	1383	1396	1423	rBV	308330	662399	66.63%	7.591%
41	5.738	1459	1461	1464	rBV2	369	185	0.02%	0.002%
42	5.834	1479	1491	1508	rBV5	18490	42394	4.26%	0.486%
43	5.985	1525	1538	1568	rVB2	189596	415125	41.76%	4.757%
44	6.230	1610	1614	1615	rBV2	238	159	0.02%	0.002%
45	6.339	1642	1648	1649	rBV2	247	241	0.02%	0.003%
46	6.419	1670	1673	1677	rBB	298	212	0.02%	0.002%
47	6.465	1684	1687	1690	rVB	290	186	0.02%	0.002%
48	6.510	1699	1701	1704	rBV	267	170	0.02%	0.002%
49	6.587	1721	1725	1726	rBV	231	143	0.01%	0.002%
50	6.622	1732	1736	1738	rVV2	263	172	0.02%	0.002%
51	6.680	1750	1754	1757	rBV2	203	180	0.02%	0.002%
52	6.754	1775	1777	1778	rBV	272	150	0.02%	0.002%
53	6.776	1781	1784	1788	rVV	186	163	0.02%	0.002%
54	6.802	1788	1792	1796	rVB	398	366	0.04%	0.004%
55	6.828	1796	1800	1803	rBV	331	261	0.03%	0.003%
56	6.911	1816	1826	1854	rBV	118653	241070	24.25%	2.763%
57	7.137	1894	1896	1899	rVB	307	192	0.02%	0.002%
58	7.169	1901	1906	1907	rBV2	890	605	0.06%	0.007%
59	7.239	1916	1928	1959	rBV	477560	868816	87.39%	9.957%
60	7.461	1994	1997	2003	rVB	681	579	0.06%	0.007%
61	7.493	2003	2007	2009	rBV2	447	338	0.03%	0.004%
62	7.551	2016	2025	2053	rBV2	80419	164088	16.50%	1.881%
63	7.902	2122	2134	2159	rVV	353140	607886	61.14%	6.967%
64	8.046	2166	2179	2206	rBV2	97309	265421	26.70%	3.042%
65	8.333	2265	2268	2274	rVB4	695	517	0.05%	0.006%
66	8.371	2274	2280	2282	rBV4	1060	1047	0.11%	0.012%
67	8.493	2314	2318	2322	rVB2	365	342	0.03%	0.004%
68	8.516	2322	2325	2327	rBV	378	287	0.03%	0.003%
69	8.529	2327	2329	2333	rVB3	482	355	0.04%	0.004%
70	8.606	2345	2353	2357	rVV4	925	1153	0.12%	0.013%
71	8.628	2357	2360	2366	rVB2	243	234	0.02%	0.003%
72	8.712	2382	2386	2388	rBV3	574	493	0.05%	0.006%
73	8.786	2397	2409	2440	rBV	475809	856545	86.16%	9.816%
74	9.034	2480	2486	2488	rBV4	840	937	0.09%	0.011%
75	9.095	2494	2505	2513	rBV8	3992	7608	0.77%	0.087%
76	9.214	2537	2542	2545	rBV2	391	320	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033262.D
 Acq On : 12 Dec 2023 14:56
 Operator : SY/MD
 Sample : 05750-02ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	9.239	2547	2550	2553	rBV	202	188	0.02%	0.002%
78	9.255	2553	2555	2557	rBV	361	143	0.01%	0.002%
79	9.352	2583	2585	2588	rBB	324	153	0.02%	0.002%
80	9.387	2592	2596	2598	rBV2	852	729	0.07%	0.008%
81	9.452	2612	2616	2618	rBB	374	277	0.03%	0.003%
82	9.490	2621	2628	2634	rBV4	1778	2973	0.30%	0.034%
83	9.567	2651	2652	2654	rBV	344	157	0.02%	0.002%
84	9.603	2661	2663	2666	rBV	367	190	0.02%	0.002%
85	9.651	2668	2678	2684	rBV7	2170	3300	0.33%	0.038%
86	9.741	2696	2706	2715	rBV8	3072	5858	0.59%	0.067%
87	9.825	2730	2732	2733	rBV8	459	230	0.02%	0.003%
88	9.844	2735	2738	2740	rBV2	552	394	0.04%	0.005%
89	9.931	2764	2765	2768	rVB2	357	161	0.02%	0.002%
90	9.960	2768	2774	2778	rBV5	1327	1786	0.18%	0.020%
91	10.001	2781	2787	2789	rBV4	1300	1447	0.15%	0.017%
92	10.027	2790	2795	2800	rBV6	2311	3118	0.31%	0.036%
93	10.101	2816	2818	2822	rBV	257	164	0.02%	0.002%
94	10.159	2822	2836	2856	rBV	258695	440452	44.30%	5.048%
95	10.390	2901	2908	2922	rBV2	11876	26977	2.71%	0.309%
96	10.779	3018	3029	3032	rBV9	2738	4526	0.46%	0.052%
97	10.860	3048	3054	3065	rVB2	27507	39461	3.97%	0.452%
98	10.976	3083	3090	3093	rBV6	3246	3680	0.37%	0.042%
99	11.188	3146	3156	3176	rBV	622607	970332	97.60%	11.120%
100	11.564	3264	3273	3293	rVB	591182	974590	98.03%	11.169%

Sum of corrected areas: 8725710




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033262.D
Acq On : 12 Dec 2023 14:56
Operator : SY/MD
Sample : 05750-02ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

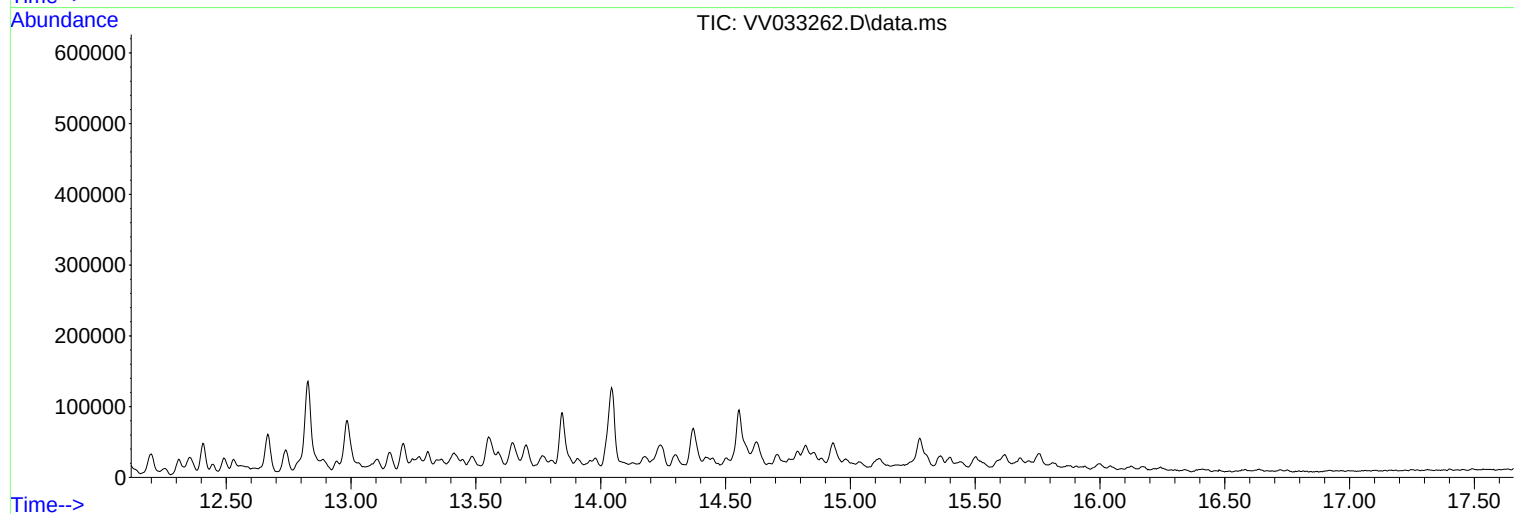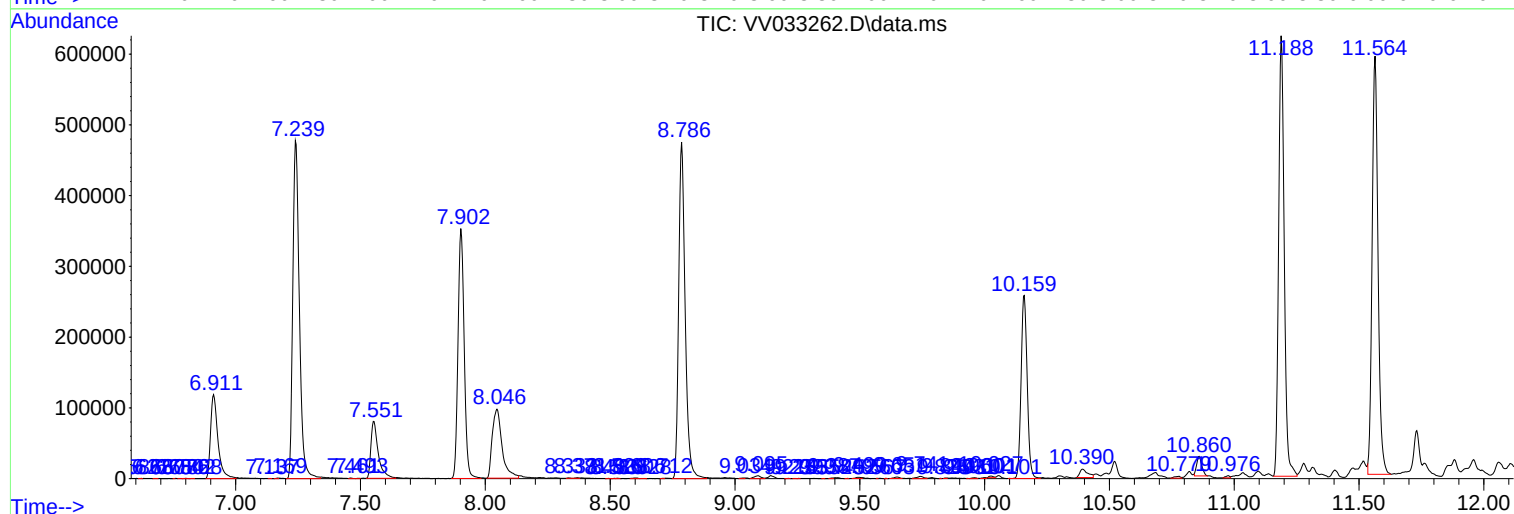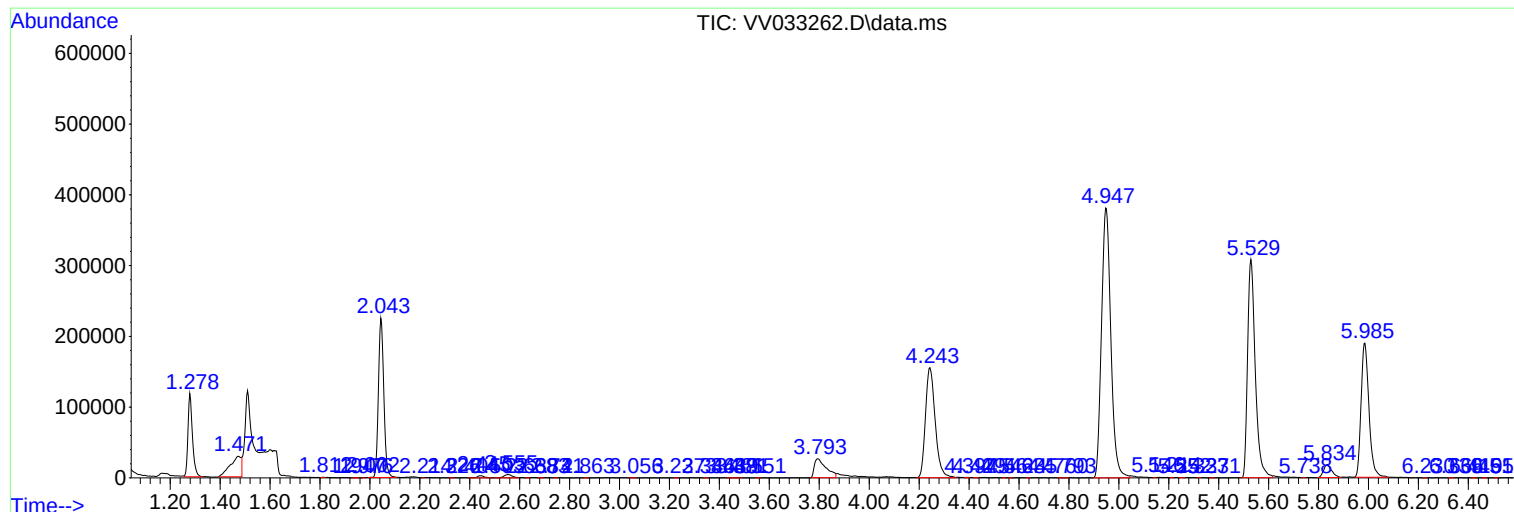

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033262.D
Acq On : 12 Dec 2023 14:56
Operator : SY/MD
Sample : 05750-02ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033262.D
Acq On : 12 Dec 2023 14:56
Operator : SY/MD
Sample : 05750-02ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------