

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033264.D
 Acq On : 12 Dec 2023 15:47
 Operator : SY/MD
 Sample : 05750-03ME
 Misc : 5.65g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	95831	121567	14.04%	1.714%
2	1.452	111	128	129	rBV4	22135	40383	4.66%	0.570%
3	1.963	282	287	289	rBV4	566	425	0.05%	0.006%
4	1.989	289	295	297	rBV4	951	1028	0.12%	0.014%
5	2.043	301	312	330	rVB	171733	255661	29.52%	3.606%
6	2.269	374	382	384	rBV3	324	377	0.04%	0.005%
7	2.391	417	420	423	rBV	250	198	0.02%	0.003%
8	2.439	429	435	447	rVB6	2669	4942	0.57%	0.070%
9	2.484	447	449	453	rVB2	374	233	0.03%	0.003%
10	2.506	454	456	459	rBB	312	188	0.02%	0.003%
11	2.558	459	472	480	rBV2	5333	11648	1.34%	0.164%
12	2.693	511	514	516	rBV	375	258	0.03%	0.004%
13	2.773	536	539	541	rBV	316	207	0.02%	0.003%
14	2.818	547	553	557	rBV2	352	410	0.05%	0.006%
15	2.934	585	589	590	rBV2	392	231	0.03%	0.003%
16	2.957	594	596	599	rVB	363	182	0.02%	0.003%
17	2.986	602	605	607	rBV	290	238	0.03%	0.003%
18	3.178	659	665	668	rBB2	333	342	0.04%	0.005%
19	3.288	695	699	705	rBB2	348	321	0.04%	0.005%
20	3.391	729	731	736	rVB2	267	213	0.02%	0.003%
21	3.471	755	756	759	rBV	359	194	0.02%	0.003%
22	3.523	768	772	776	rBB	271	251	0.03%	0.004%
23	3.551	777	781	784	rBV	179	183	0.02%	0.003%
24	3.571	785	787	791	rVV2	338	226	0.03%	0.003%
25	3.703	825	828	830	rBV	306	239	0.03%	0.003%
26	3.725	830	835	838	rVB2	186	232	0.03%	0.003%
27	3.796	849	857	888	rBV	26640	96356	11.13%	1.359%
28	4.156	967	969	972	rBV2	311	193	0.02%	0.003%
29	4.246	981	997	1030	rBV	134362	367013	42.38%	5.176%
30	4.641	1117	1120	1122	rBV	435	254	0.03%	0.004%
31	4.950	1201	1216	1251	rBV2	332770	866053	100.00%	12.214%
32	5.230	1300	1303	1305	rVV2	560	343	0.04%	0.005%
33	5.259	1309	1312	1315	rBV2	557	365	0.04%	0.005%
34	5.326	1330	1333	1335	rBV	325	213	0.02%	0.003%
35	5.532	1386	1397	1425	rBV	298410	639863	73.88%	9.024%
36	5.838	1480	1492	1505	rBV8	12221	29074	3.36%	0.410%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033264.D
 Acq On : 12 Dec 2023 15:47
 Operator : SY/MD
 Sample : 05750-03ME
 Misc : 5.65g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.989	1527	1539	1564	rBV	164557	355910	41.10%	5.019%
38	6.522	1702	1705	1707	rVB2	361	201	0.02%	0.003%
39	6.545	1711	1712	1715	rVB	370	182	0.02%	0.003%
40	6.561	1715	1717	1721	rBV	272	235	0.03%	0.003%
41	6.915	1816	1827	1862	rVV2	99747	207835	24.00%	2.931%
42	7.162	1901	1904	1905	rBV	450	224	0.03%	0.003%
43	7.243	1916	1929	1961	rBV	409958	747842	86.35%	10.547%
44	7.554	2017	2026	2057	rBV	70274	145172	16.76%	2.047%
45	7.908	2125	2136	2155	rVB	75446	131986	15.24%	1.861%
46	8.053	2167	2181	2214	rBV2	90228	259755	29.99%	3.663%
47	8.371	2276	2280	2281	rBV3	614	469	0.05%	0.007%
48	8.670	2371	2373	2376	rVB	334	190	0.02%	0.003%
49	8.786	2397	2409	2438	rBV	430982	803136	92.74%	11.327%
50	9.149	2516	2522	2526	rBV2	355	498	0.06%	0.007%
51	9.320	2571	2575	2579	rVB2	373	299	0.03%	0.004%
52	9.471	2618	2622	2626	rVB2	404	365	0.04%	0.005%
53	9.513	2631	2635	2637	rVB2	277	223	0.03%	0.003%
54	9.603	2662	2663	2666	rBV	340	192	0.02%	0.003%
55	9.619	2666	2668	2673	rVV2	340	346	0.04%	0.005%
56	9.651	2676	2678	2682	rVB2	268	216	0.02%	0.003%
57	9.744	2704	2707	2712	rBV	335	346	0.04%	0.005%
58	9.886	2747	2751	2753	rBV	397	271	0.03%	0.004%
59	10.037	2795	2798	2801	rVB2	262	197	0.02%	0.003%
60	10.062	2801	2806	2809	rBV2	299	354	0.04%	0.005%
61	10.159	2824	2836	2856	rBV	216562	373845	43.17%	5.272%
62	10.329	2881	2889	2897	rVB4	961	1327	0.15%	0.019%
63	10.397	2908	2910	2913	rVB	370	190	0.02%	0.003%
64	10.419	2913	2917	2921	rBV2	330	371	0.04%	0.005%
65	10.519	2945	2948	2951	rBV	329	278	0.03%	0.004%
66	10.776	3026	3028	3032	rVB	261	183	0.02%	0.003%
67	10.834	3043	3046	3050	rBB	361	309	0.04%	0.004%
68	10.860	3050	3054	3055	rBV	274	249	0.03%	0.004%
69	10.895	3063	3065	3068	rVV	357	219	0.03%	0.003%
70	11.191	3144	3157	3182	rBV	549338	856282	98.87%	12.076%
71	11.564	3262	3273	3300	rBV	476948	744062	85.91%	10.493%
72	11.808	3345	3349	3350	rBV	298	194	0.02%	0.003%
73	11.995	3402	3407	3411	rVB2	222	269	0.03%	0.004%
74	12.236	3478	3482	3484	rBV2	256	215	0.02%	0.003%
75	12.580	3585	3589	3590	rVB	559	272	0.03%	0.004%
76	12.596	3591	3594	3596	rBV	341	200	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033264.D
 Acq On : 12 Dec 2023 15:47
 Operator : SY/MD
 Sample : 05750-03ME
 Misc : 5.65g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LQ6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.831	3661	3667	3675	rBV4	2071	2185	0.25%	0.031%
78	12.930	3693	3698	3702	rBV3	451	476	0.05%	0.007%
79	12.950	3702	3704	3708	rVB3	457	229	0.03%	0.003%
80	13.043	3730	3733	3735	rBV	262	186	0.02%	0.003%
81	13.114	3752	3755	3757	rBV	302	216	0.02%	0.003%
82	13.127	3757	3759	3764	rVB	321	248	0.03%	0.003%
83	13.146	3764	3765	3769	rBV	254	191	0.02%	0.003%
84	13.217	3781	3787	3795	rBV5	813	956	0.11%	0.013%
85	13.358	3828	3831	3833	rBV3	391	229	0.03%	0.003%
86	13.371	3833	3835	3838	rBV2	339	180	0.02%	0.003%
87	13.554	3890	3892	3894	rBV2	482	241	0.03%	0.003%
88	13.628	3913	3915	3917	rBV3	454	210	0.02%	0.003%
89	13.731	3941	3947	3949	rBV3	504	418	0.05%	0.006%
90	13.844	3976	3982	3993	rVB6	3578	4814	0.56%	0.068%
91	13.895	3996	3998	4000	rBV3	507	208	0.02%	0.003%
92	13.921	4003	4006	4008	rBV	374	279	0.03%	0.004%
93	14.030	4037	4040	4042	rBV2	621	339	0.04%	0.005%
94	14.284	4116	4119	4121	rBV	462	253	0.03%	0.004%
95	14.345	4135	4138	4140	rBV	429	271	0.03%	0.004%
96	14.397	4153	4154	4157	rVB	559	239	0.03%	0.003%
97	14.455	4170	4172	4175	rVB4	837	330	0.04%	0.005%
98	14.593	4208	4215	4220	rBV8	1839	2316	0.27%	0.033%
99	14.866	4298	4300	4302	rBV2	505	249	0.03%	0.004%
100	15.188	4398	4400	4402	rBV2	673	462	0.05%	0.007%

Sum of corrected areas: 7090738




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033264.D
Acq On : 12 Dec 2023 15:47
Operator : SY/MD
Sample : 05750-03ME
Misc : 5.65g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

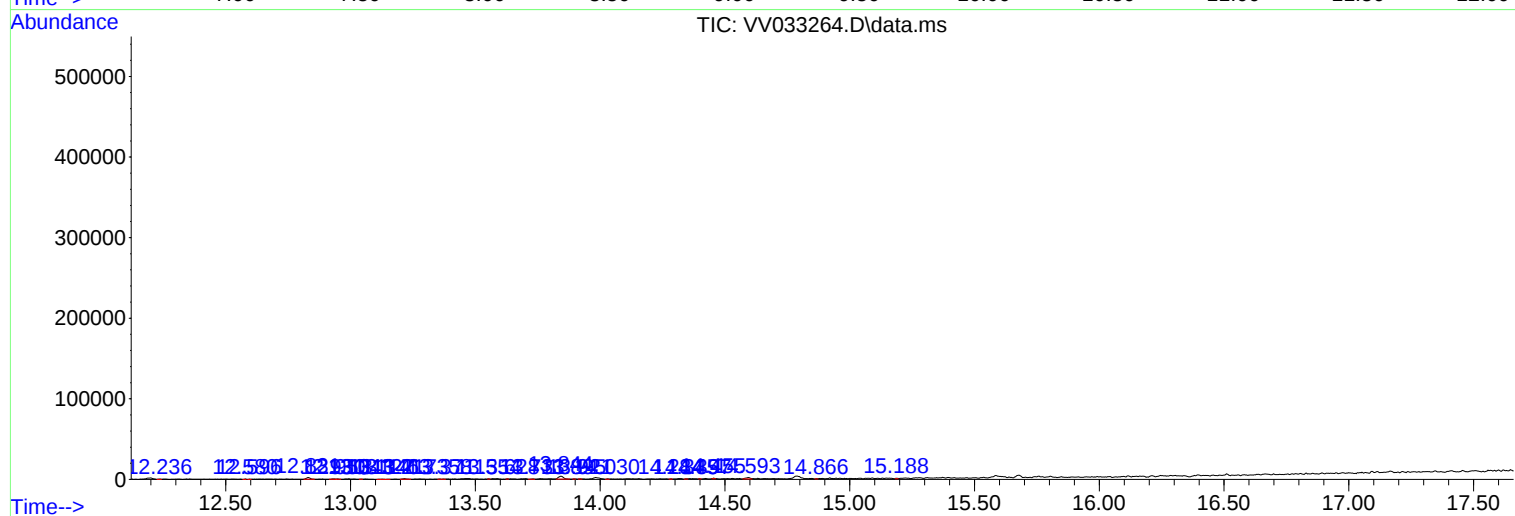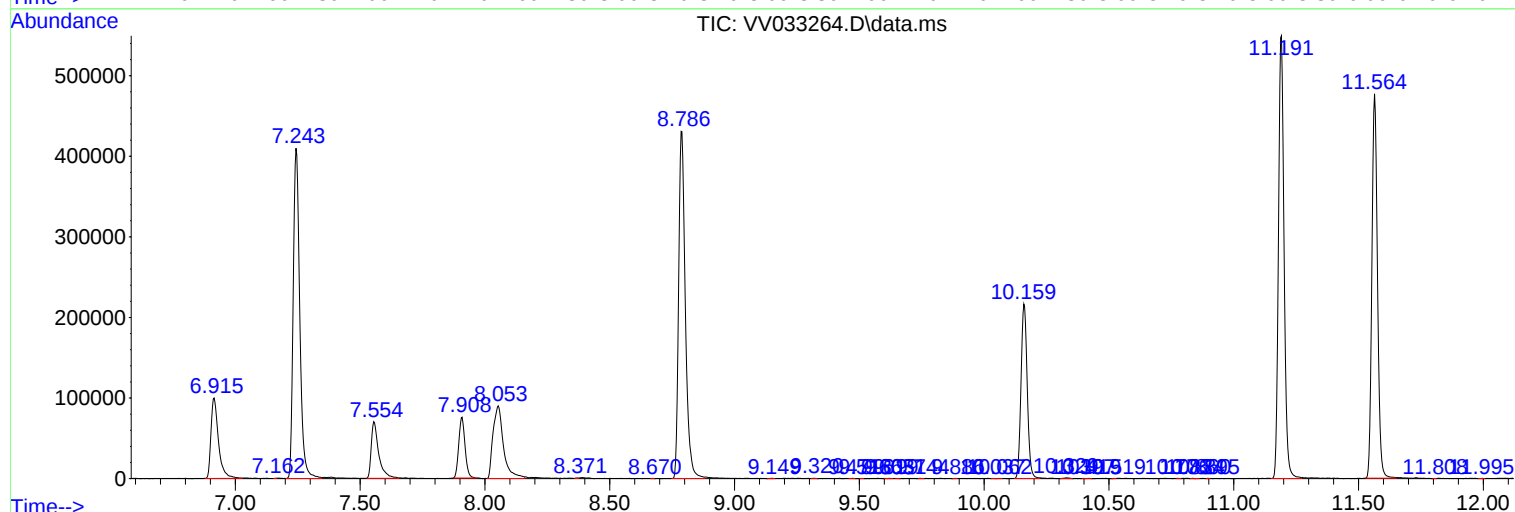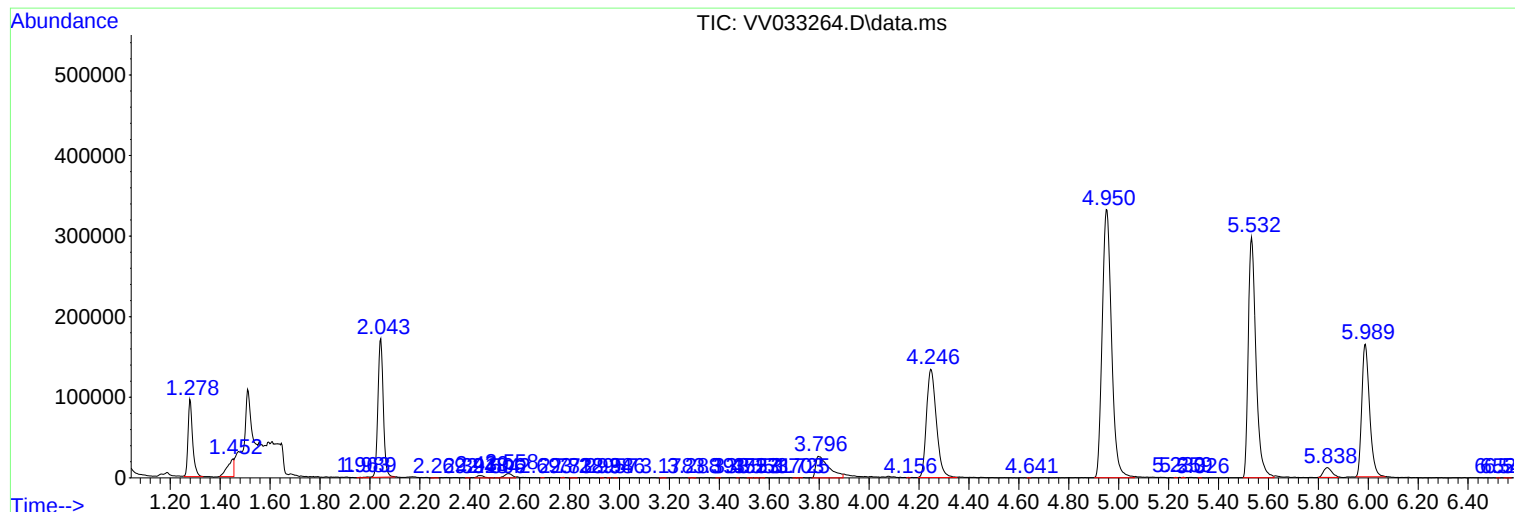

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033264.D
Acq On : 12 Dec 2023 15:47
Operator : SY/MD
Sample : 05750-03ME
Misc : 5.65g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033264.D
Acq On : 12 Dec 2023 15:47
Operator : SY/MD
Sample : 05750-03ME
Misc : 5.65g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LQ6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------