

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033266.D
 Acq On : 12 Dec 2023 16:33
 Operator : SY/MD
 Sample : 05751-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033266.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	125414	132353	13.97%	1.907%
2	1.532	146	153	169	rVB	91282	107535	11.35%	1.549%
3	2.060	307	317	332	rBV	198867	290977	30.72%	4.192%
4	2.240	370	373	376	rBV2	373	317	0.03%	0.005%
5	2.326	397	400	401	rBV2	231	92	0.01%	0.001%
6	2.362	409	411	413	rVB	286	129	0.01%	0.002%
7	2.378	413	416	419	rBV2	293	251	0.03%	0.004%
8	2.452	432	439	445	rBB4	1176	1455	0.15%	0.021%
9	2.484	445	449	451	rBV2	354	291	0.03%	0.004%
10	2.603	483	486	489	rBB	270	226	0.02%	0.003%
11	2.625	489	493	495	rBV	238	177	0.02%	0.003%
12	2.661	503	504	506	rBB	234	70	0.01%	0.001%
13	2.680	507	510	512	rBB	138	94	0.01%	0.001%
14	2.709	517	519	521	rBB	273	127	0.01%	0.002%
15	2.728	522	525	527	rBV	250	143	0.02%	0.002%
16	2.831	555	557	559	rBB	107	60	0.01%	0.001%
17	2.841	559	560	561	rBV	124	46	0.00%	0.001%
18	2.915	582	583	586	rVB2	173	69	0.01%	0.001%
19	2.953	592	595	596	rBV	257	148	0.02%	0.002%
20	2.982	601	604	606	rBV	345	292	0.03%	0.004%
21	3.031	616	619	621	rBV	144	122	0.01%	0.002%
22	3.060	625	628	632	rBB	308	282	0.03%	0.004%
23	3.085	633	636	641	rBB	242	203	0.02%	0.003%
24	3.117	644	646	647	rBV	282	136	0.01%	0.002%
25	3.201	668	672	677	rBV	157	216	0.02%	0.003%
26	3.281	696	697	699	rBV	229	90	0.01%	0.001%
27	3.352	716	719	720	rBV	137	100	0.01%	0.001%
28	3.500	762	765	767	rBV	119	108	0.01%	0.002%
29	3.535	774	776	778	rBV	152	106	0.01%	0.002%
30	3.574	784	788	789	rBB	114	63	0.01%	0.001%
31	3.600	792	796	798	rBV	176	170	0.02%	0.002%
32	3.651	809	812	814	rBB2	257	143	0.02%	0.002%
33	3.677	818	820	822	rBB	123	65	0.01%	0.001%
34	3.744	838	841	843	rBV	284	189	0.02%	0.003%
35	3.780	843	852	884	rBV	47086	128588	13.58%	1.853%
36	4.674	1128	1130	1131	rBV	426	194	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121223\
 Data File : VW033266.D
 Acq On : 12 Dec 2023 16:33
 Operator : SY/MD
 Sample : 05751-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.873	1189	1192	1193	rBV	205	133	0.01%	0.002%
38	4.957	1201	1218	1250	rBV3	355180	947096	100.00%	13.645%
39	5.532	1386	1397	1429	rBV	292021	598066	63.15%	8.617%
40	5.738	1460	1461	1463	rBV	629	264	0.03%	0.004%
41	5.989	1528	1539	1558	rBV2	188866	385955	40.75%	5.561%
42	6.355	1649	1653	1657	rBV	315	290	0.03%	0.004%
43	6.493	1693	1696	1698	rBV	172	138	0.01%	0.002%
44	6.674	1750	1752	1753	rBV	348	136	0.01%	0.002%
45	6.789	1786	1788	1789	rBV	161	47	0.00%	0.001%
46	6.911	1816	1826	1846	rBV	114632	211877	22.37%	3.053%
47	7.243	1918	1929	1964	rBV	454843	805331	85.03%	11.603%
48	7.551	2016	2025	2046	rBV	86389	153937	16.25%	2.218%
49	7.841	2111	2115	2118	rBV	170	200	0.02%	0.003%
50	7.963	2150	2153	2155	rBV	280	204	0.02%	0.003%
51	8.024	2163	2172	2208	rBV	172817	324498	34.26%	4.675%
52	8.445	2302	2303	2305	rBV	217	91	0.01%	0.001%
53	8.526	2325	2328	2330	rBV	177	155	0.02%	0.002%
54	8.783	2397	2408	2436	rBV	460947	760257	80.27%	10.954%
55	9.098	2503	2506	2507	rBV	323	144	0.02%	0.002%
56	9.175	2528	2530	2533	rBV	269	168	0.02%	0.002%
57	9.233	2547	2548	2551	rBB	132	72	0.01%	0.001%
58	9.271	2556	2560	2564	rBB2	478	432	0.05%	0.006%
59	9.291	2564	2566	2567	rBV	137	72	0.01%	0.001%
60	9.374	2590	2592	2593	rBV	117	66	0.01%	0.001%
61	9.583	2655	2657	2659	rBV	166	119	0.01%	0.002%
62	9.657	2678	2680	2681	rBV	123	65	0.01%	0.001%
63	9.725	2696	2701	2706	rBV2	271	380	0.04%	0.005%
64	9.767	2712	2714	2715	rBV2	259	113	0.01%	0.002%
65	9.805	2724	2726	2727	rBV	210	45	0.00%	0.001%
66	9.857	2738	2742	2744	rBV	246	164	0.02%	0.002%
67	9.918	2756	2761	2765	rBB2	320	297	0.03%	0.004%
68	9.937	2766	2767	2770	rBV	255	119	0.01%	0.002%
69	10.098	2815	2817	2819	rBV	275	198	0.02%	0.003%
70	10.152	2823	2834	2855	rVV	277568	434514	45.88%	6.260%
71	10.381	2904	2905	2906	rBV	207	68	0.01%	0.001%
72	10.497	2938	2941	2945	rBB2	264	206	0.02%	0.003%
73	10.519	2945	2948	2951	rBB	173	137	0.01%	0.002%
74	10.542	2952	2955	2959	rBV3	372	352	0.04%	0.005%
75	10.699	3000	3004	3007	rBB	292	268	0.03%	0.004%
76	10.731	3008	3014	3016	rBV	171	191	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
 Data File : VV033266.D
 Acq On : 12 Dec 2023 16:33
 Operator : SY/MD
 Sample : 05751-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.824	3040	3043	3045	rBV	133	116	0.01%	0.002%
78	10.870	3055	3057	3059	rBV	254	159	0.02%	0.002%
79	10.934	3074	3077	3078	rBV	247	168	0.02%	0.002%
80	11.082	3121	3123	3125	rBV	150	105	0.01%	0.002%
81	11.185	3144	3155	3179	rBV	524476	806232	85.13%	11.616%
82	11.471	3243	3244	3245	rBB	127	49	0.01%	0.001%
83	11.561	3260	3272	3296	rBV	544605	837173	88.39%	12.062%
84	11.844	3358	3360	3363	rVB2	313	140	0.01%	0.002%
85	11.895	3372	3376	3377	rBV	262	172	0.02%	0.002%
86	12.085	3428	3435	3440	rBV2	257	386	0.04%	0.006%
87	12.307	3500	3504	3507	rBB2	311	255	0.03%	0.004%
88	12.323	3507	3509	3510	rBV2	419	192	0.02%	0.003%
89	12.558	3577	3582	3586	rBV	308	386	0.04%	0.006%
90	12.625	3601	3603	3605	rBB	372	142	0.01%	0.002%
91	12.648	3605	3610	3611	rBV2	286	227	0.02%	0.003%
92	12.763	3642	3646	3653	rBB2	508	758	0.08%	0.011%
93	12.799	3654	3657	3658	rBV	130	72	0.01%	0.001%
94	12.847	3671	3672	3675	rBV	258	134	0.01%	0.002%
95	12.959	3706	3707	3711	rVB	216	74	0.01%	0.001%
96	13.162	3767	3770	3774	rBV3	325	273	0.03%	0.004%
97	13.204	3781	3783	3784	rBV	377	133	0.01%	0.002%
98	13.509	3874	3878	3881	rBV2	507	510	0.05%	0.007%
99	13.686	3931	3933	3935	rBV2	380	139	0.01%	0.002%
100	13.744	3948	3951	3955	rBV2	391	246	0.03%	0.004%




Sum of corrected areas: 6940733

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033266.D
Acq On : 12 Dec 2023 16:33
Operator : SY/MD
Sample : 05751-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

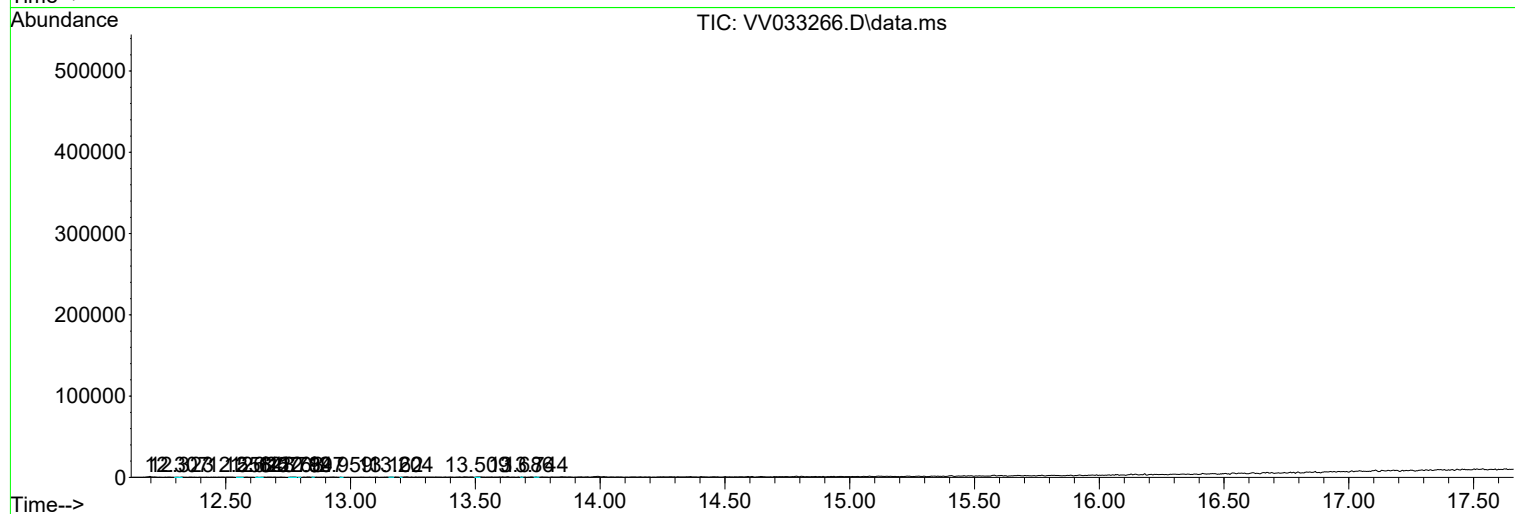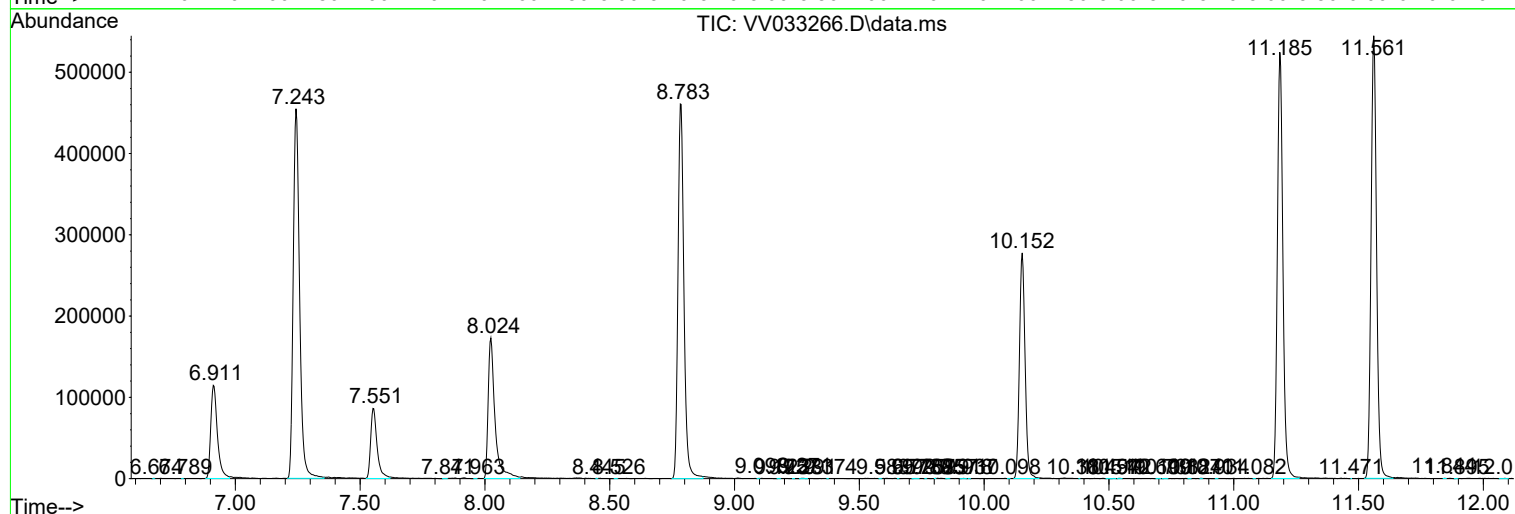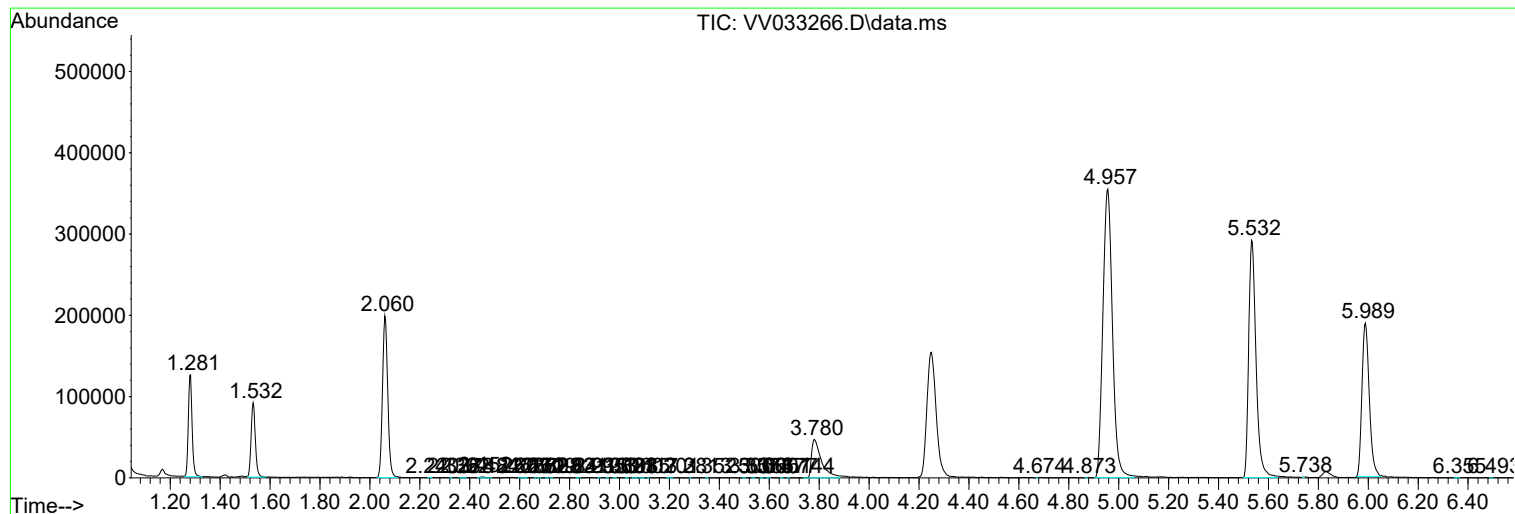

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033266.D
Acq On : 12 Dec 2023 16:33
Operator : SY/MD
Sample : 05751-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033266.D
Acq On : 12 Dec 2023 16:33
Operator : SY/MD
Sample : 05751-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc