


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121223\
Data File : VV033252.D
Acq On : 12 Dec 2023 08:50
Operator : SY/MD
Sample : BFB245
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB245

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis
Last Update : Fri Dec 08 21:51:12 2023

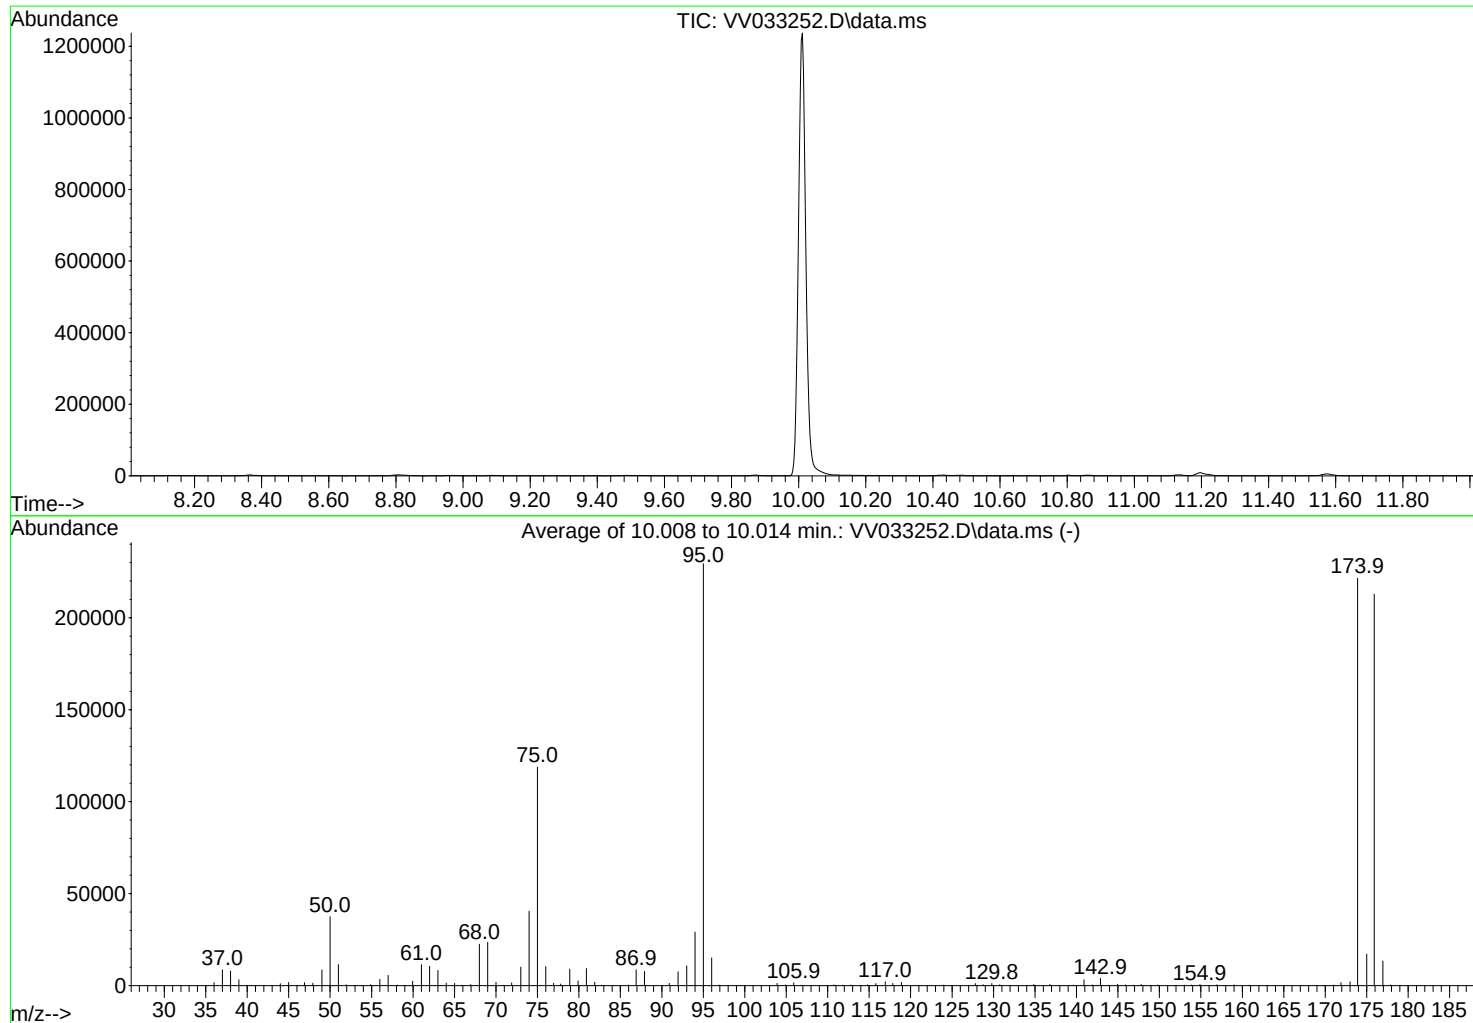

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	37477	PASS
75	95	30	80	51.8	118843	PASS
95	95	100	100	100.0	229397	PASS
96	95	5	9	6.6	15041	PASS
173	174	0.00	2	0.9	2024	PASS
174	95	50	120	96.6	221525	PASS
175	174	5	9	7.7	17133	PASS
176	174	95	105	96.1	212864	PASS
177	176	5	10	6.3	13344	PASS

m/z	Abundance
40.10	121.0
44.00	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.00	1577.0
37.00	9154.0
38.00	8363.0
39.00	3290.0
39.90	269.0
44.10	1175.0
45.00	1712.0
45.90	203.0
46.90	1656.0
47.90	1279.0
49.00	8849.0
50.00	38896.0
51.00	11609.0
52.00	474.0
52.80	152.0
53.80	117.0
54.90	610.0
56.00	3337.0
57.00	5551.0
58.00	350.0
59.90	2402.0
61.00	12011.0
62.00	10621.0
63.00	8776.0
64.00	1412.0
65.00	1374.0
65.90	142.0
66.90	666.0
68.00	23032.0
69.00	24072.0
70.00	1839.0
70.90	118.0
71.90	1637.0
73.00	10057.0
74.00	41568.0
75.00	122784.0
76.00	10547.0
76.90	1356.0
77.80	765.0
78.90	8938.0
79.90	2456.0
80.90	9603.0
81.90	1884.0
82.70	198.0
83.10	152.0
85.90	336.0
86.90	8826.0
87.90	7646.0
90.90	1162.0
92.00	7822.0
93.00	11107.0
94.00	29080.0
95.00	235136.0
96.00	15938.0
96.90	310.0
103.90	1221.0
104.90	414.0
105.90	1526.0
106.80	240.0
109.90	146.0
110.70	427.0
111.90	258.0
112.80	344.0
114.80	408.0
115.80	1009.0
116.90	1942.0
117.80	1158.0
118.90	1735.0
123.90	334.0
127.00	123.0
127.80	1084.0
128.70	494.0
129.80	1102.0
130.80	558.0
134.90	620.0
136.80	638.0
139.70	207.0
140.90	3003.0
141.90	371.0
142.90	4033.0
143.90	249.0
145.00	879.0
145.90	352.0
146.80	198.0
147.80	575.0
148.90	166.0
149.80	326.0
151.80	177.0
152.90	201.0
153.80	325.0
154.90	643.0
157.00	513.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

157.80	115.0
159.00	445.0
160.70	286.0
170.10	168.0
171.10	387.0
171.90	1648.0
173.00	2957.0
173.90	223488.0
175.00	17408.0
175.90	213376.0
177.00	13420.0
177.80	470.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.00	1623.0
37.00	8914.0
38.00	8225.0
39.00	3243.0
39.90	272.0
44.00	1200.0
45.00	1770.0
45.90	165.0
46.90	1690.0
47.90	1319.0
49.00	8733.0
50.00	38952.0
51.00	11808.0
51.90	487.0
52.90	145.0
53.80	124.0
54.90	573.0
56.00	3543.0
57.00	5742.0
58.10	306.0
60.00	2471.0
61.00	11822.0
62.00	10915.0
63.00	8469.0
64.00	1480.0
65.00	1248.0
65.90	171.0
66.90	597.0
68.00	23200.0
69.00	24296.0
70.00	1953.0
70.90	135.0
71.90	1537.0
73.00	10429.0
74.00	41856.0
75.00	123016.0
76.00	10555.0
77.00	1318.0
77.80	838.0
78.90	9261.0
79.90	2536.0
80.90	9617.0
81.90	1807.0
82.70	238.0
86.00	365.0
86.90	8853.0
87.90	8060.0
90.90	1239.0
91.90	7912.0
93.00	11275.0
94.00	30376.0
95.00	237312.0
96.00	15481.0
96.90	299.0
103.90	1231.0
104.90	450.0
105.90	1627.0
106.80	253.0
109.90	156.0
110.70	419.0
111.80	251.0
112.80	314.0
114.80	463.0
115.80	1155.0
116.90	2139.0
117.90	1181.0
118.90	1757.0
123.00	134.0
123.90	295.0
127.00	135.0
127.80	1136.0
128.70	541.0
129.80	1149.0
130.80	479.0
134.90	594.0
136.80	732.0
139.70	185.0
140.90	3218.0
141.90	421.0
142.90	3991.0
143.80	238.0
145.00	771.0
145.90	416.0
146.90	232.0
147.80	648.0
148.80	164.0
149.80	324.0
151.80	193.0
153.00	306.0
153.80	327.0
154.90	717.0
156.90	532.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

157.80	109.0
159.00	418.0
160.90	301.0
169.10	101.0
170.00	134.0
171.00	350.0
171.90	1724.0
173.00	3116.0
173.90	229632.0
175.00	17760.0
175.90	220544.0
176.90	13754.0
177.90	343.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.00	1583.0
37.00	7740.0
38.00	7154.0
39.00	2887.0
40.00	303.0
44.00	1151.0
45.00	1618.0
46.10	149.0
46.90	1401.0
47.90	1253.0
49.00	7770.0
50.00	34584.0
51.00	11015.0
51.90	438.0
53.00	156.0
54.90	503.0
56.00	3225.0
57.00	5258.0
58.20	207.0
60.00	2250.0
61.00	10305.0
62.00	9914.0
63.00	7468.0
64.00	1184.0
65.00	985.0
65.90	184.0
67.00	498.0
68.00	21168.0
69.00	21936.0
70.00	1857.0
70.90	105.0
71.90	1274.0
73.00	9680.0
74.00	37912.0
75.00	110728.0
76.00	9759.0
77.00	1130.0
77.80	828.0
78.90	8491.0
79.90	2407.0
80.90	8648.0
81.90	1578.0
82.80	248.0
86.00	356.0
86.90	8022.0
87.90	7540.0
90.90	1027.0
91.90	6984.0
93.00	9871.0
94.00	27976.0
95.00	215744.0
96.00	13704.0
96.90	248.0
103.90	1057.0
104.90	451.0
105.90	1423.0
106.80	228.0
109.80	171.0
110.80	319.0
111.70	253.0
112.80	254.0
114.80	429.0
115.80	1130.0
117.00	2106.0
117.90	1087.0
118.90	1590.0
123.00	117.0
123.90	183.0
126.90	119.0
127.80	1060.0
128.80	461.0
129.80	1071.0
130.70	380.0
134.80	479.0
136.80	661.0
139.60	202.0
140.90	3187.0
141.90	410.0
142.90	3630.0
143.80	214.0
144.90	635.0
145.90	438.0
146.90	229.0
147.80	637.0
148.80	167.0
149.80	320.0
151.80	162.0
153.10	317.0
153.90	282.0
154.90	701.0
156.90	518.0
159.00	314.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

160.90	319.0
169.80	141.0
171.00	263.0
171.90	1501.0
173.90	211456.0
175.00	16230.0
175.90	204672.0
176.90	12857.0
178.00	277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245