

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121318\
 Data File : VV008913.D
 Acq On : 13 Dec 2018 17:01
 Operator : SY/MD
 Sample : J6367-03
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL38

Quant Time: Dec 14 01:28:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 14 01:09:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	111770	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	103049	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42582	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	63038	96.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	193.16%#
7) Chloroethane-d5	1.57	69	47622	115.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	231.86%#
11) 1,1-Dichloroethene-d2	2.13	63	118937	77.16	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	154.32%#
21) 2-Butanone-d5	3.93	46	95229	218.51	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	218.51%#
24) Chloroform-d	4.41	84	140452	100.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	201.70%#
26) 1,2-Dichloroethane-d4	5.08	65	95977	108.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	216.38%#
32) Benzene-d6	5.10	84	293143	105.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	211.12%#
36) 1,2-Dichloropropane-d6	6.12	67	87939	105.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	210.76%#
41) Toluene-d8	7.36	98	269874	103.53	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	207.06%#
43) trans-1,3-Dichloropropene-	7.67	79	42361	100.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	200.18%#
47) 2-Hexanone-d5	8.13	63	61595	199.43	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	199.43%#
57) 1,1,2,2-Tetrachloroethane-	10.26	84	108134	100.37	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	200.74%#
64) 1,2-Dichlorobenzene-d4	11.68	152	92735	105.59	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	211.18%#


Target Compounds					Ovalue
13) Acetone	2.19	43	2868	4.376 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121318\
Data File : VV008913.D
Acq On : 13 Dec 2018 17:01
Operator : SY/MD
Sample : J6367-03
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL38

Quant Time: Dec 14 01:28:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 14 01:09:42 2018
Response via : Initial Calibration

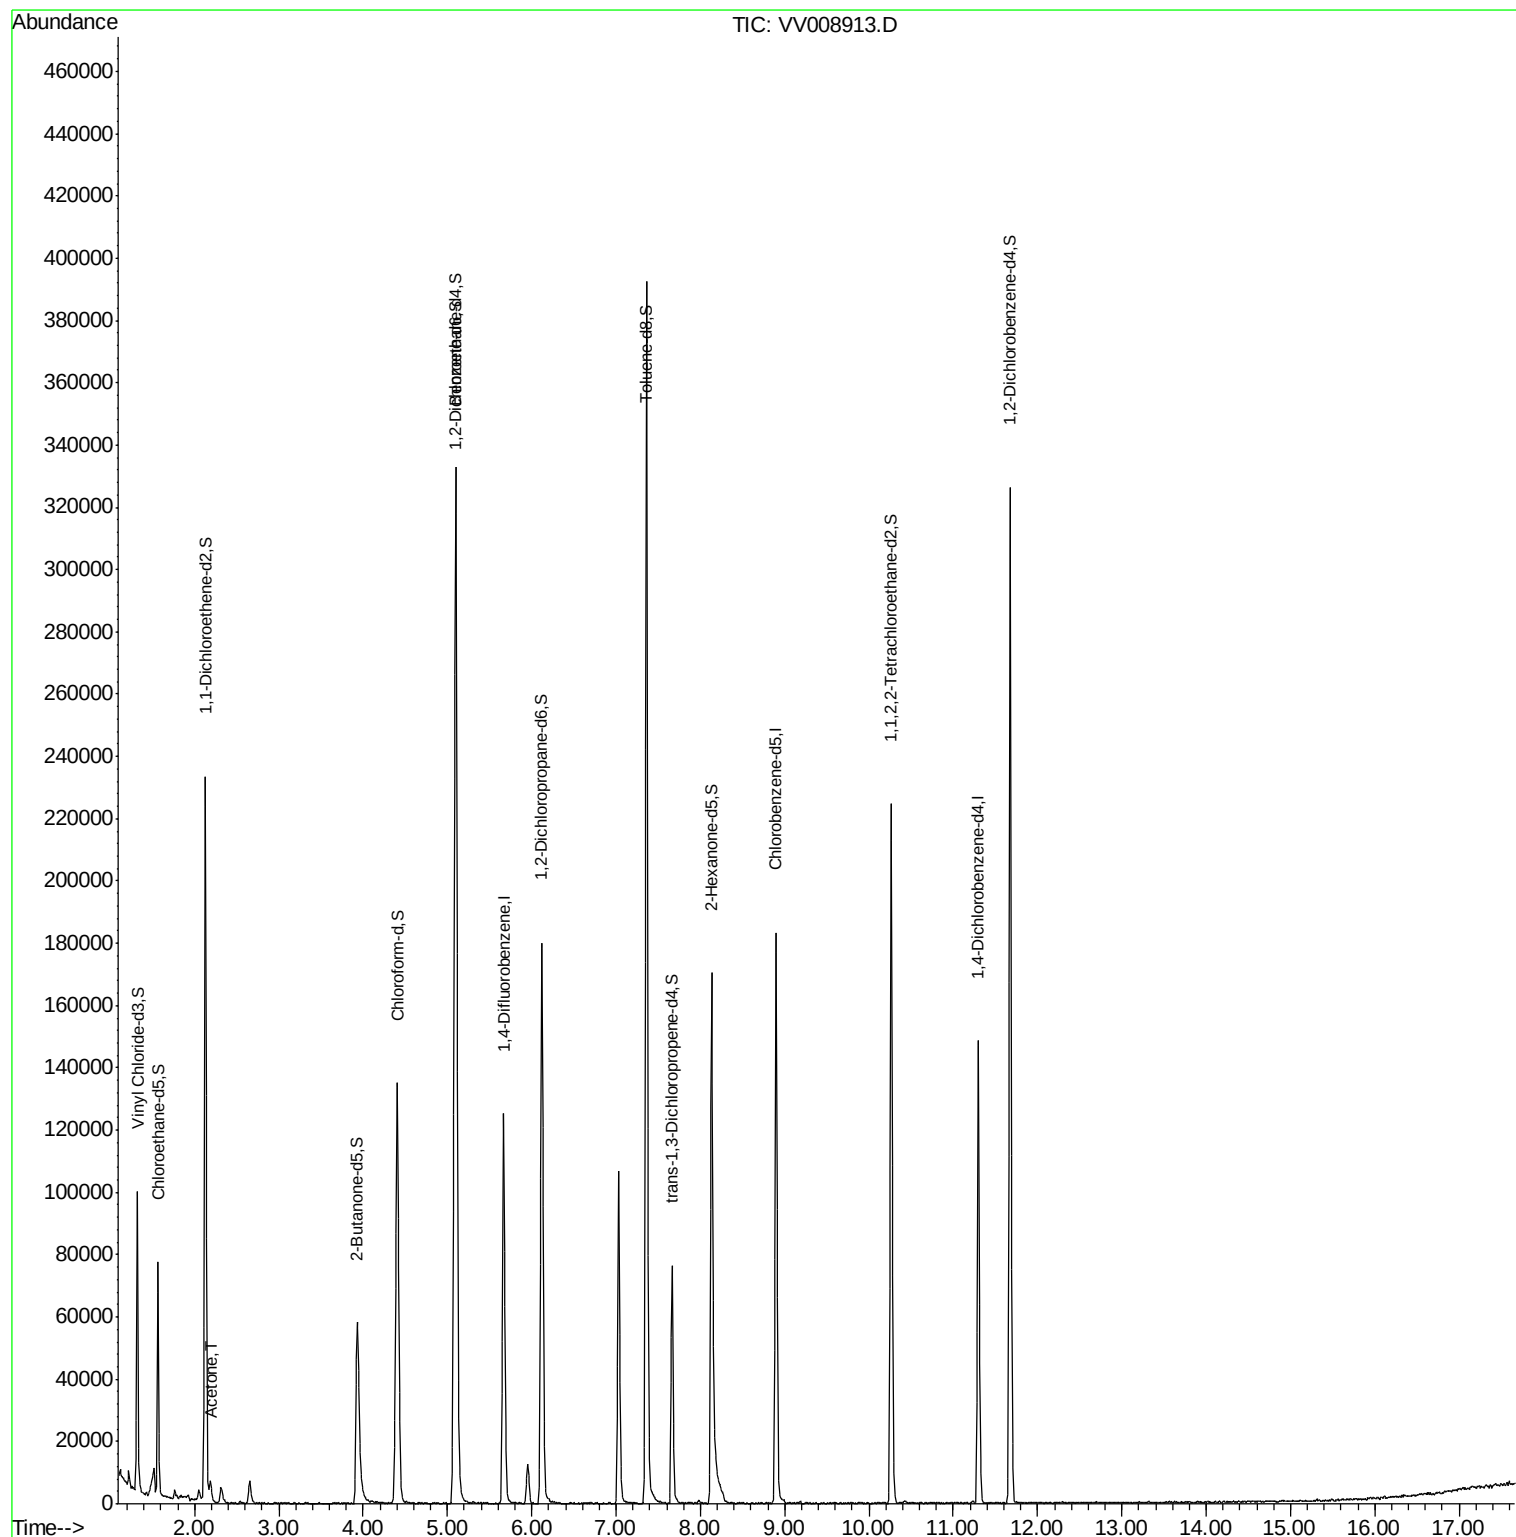

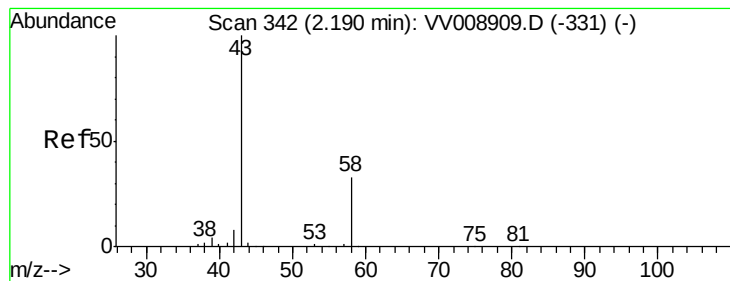

#13
 Acetone
 Concen: 4.376 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. 0.00 min
 Lab File: VV008913.D
 Acq: 13 Dec 2018 17:01

Instrument :
 MSVOA_V
 ClientSampleId :
 COL38

Tot Ion: 43 Resp: 2868
 Ion Ratio Lower Upper
 43 100
 58 31.5 0.0 61.8

