

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121318\
 Data File : VV008914.D
 Acq On : 13 Dec 2018 17:25
 Operator : SY/MD
 Sample : J6367-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL40

Quant Time: Dec 14 01:31:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 14 01:09:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	159826	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	145145	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	59075	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58059	62.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	124.40%
7) Chloroethane-d5	1.57	69	44356	75.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	151.02%#
11) 1,1-Dichloroethene-d2	2.13	63	109786	49.81	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.62%
21) 2-Butanone-d5	3.93	46	83094	133.34	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	133.34%#
24) Chloroform-d	4.40	84	128411	64.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	128.96%#
26) 1,2-Dichloroethane-d4	5.08	65	84870	66.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	133.80%#
32) Benzene-d6	5.10	84	266925	68.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	136.48%#
36) 1,2-Dichloropropane-d6	6.12	67	79778	67.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	135.76%#
41) Toluene-d8	7.36	98	243516	66.32	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	132.64%#
43) trans-1,3-Dichloropropene-	7.67	79	38342	64.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	128.64%#
47) 2-Hexanone-d5	8.13	63	52548	120.80	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	120.80%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	97505	64.25	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	128.50%#
64) 1,2-Dichlorobenzene-d4	11.68	152	83676	68.68	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	137.36%#


Target Compounds					Ovalue
13) Acetone	2.19	43	3048	3.253 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121318\
Data File : VV008914.D
Acq On : 13 Dec 2018 17:25
Operator : SY/MD
Sample : J6367-04
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL40

Quant Time: Dec 14 01:31:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 14 01:09:42 2018
Response via : Initial Calibration

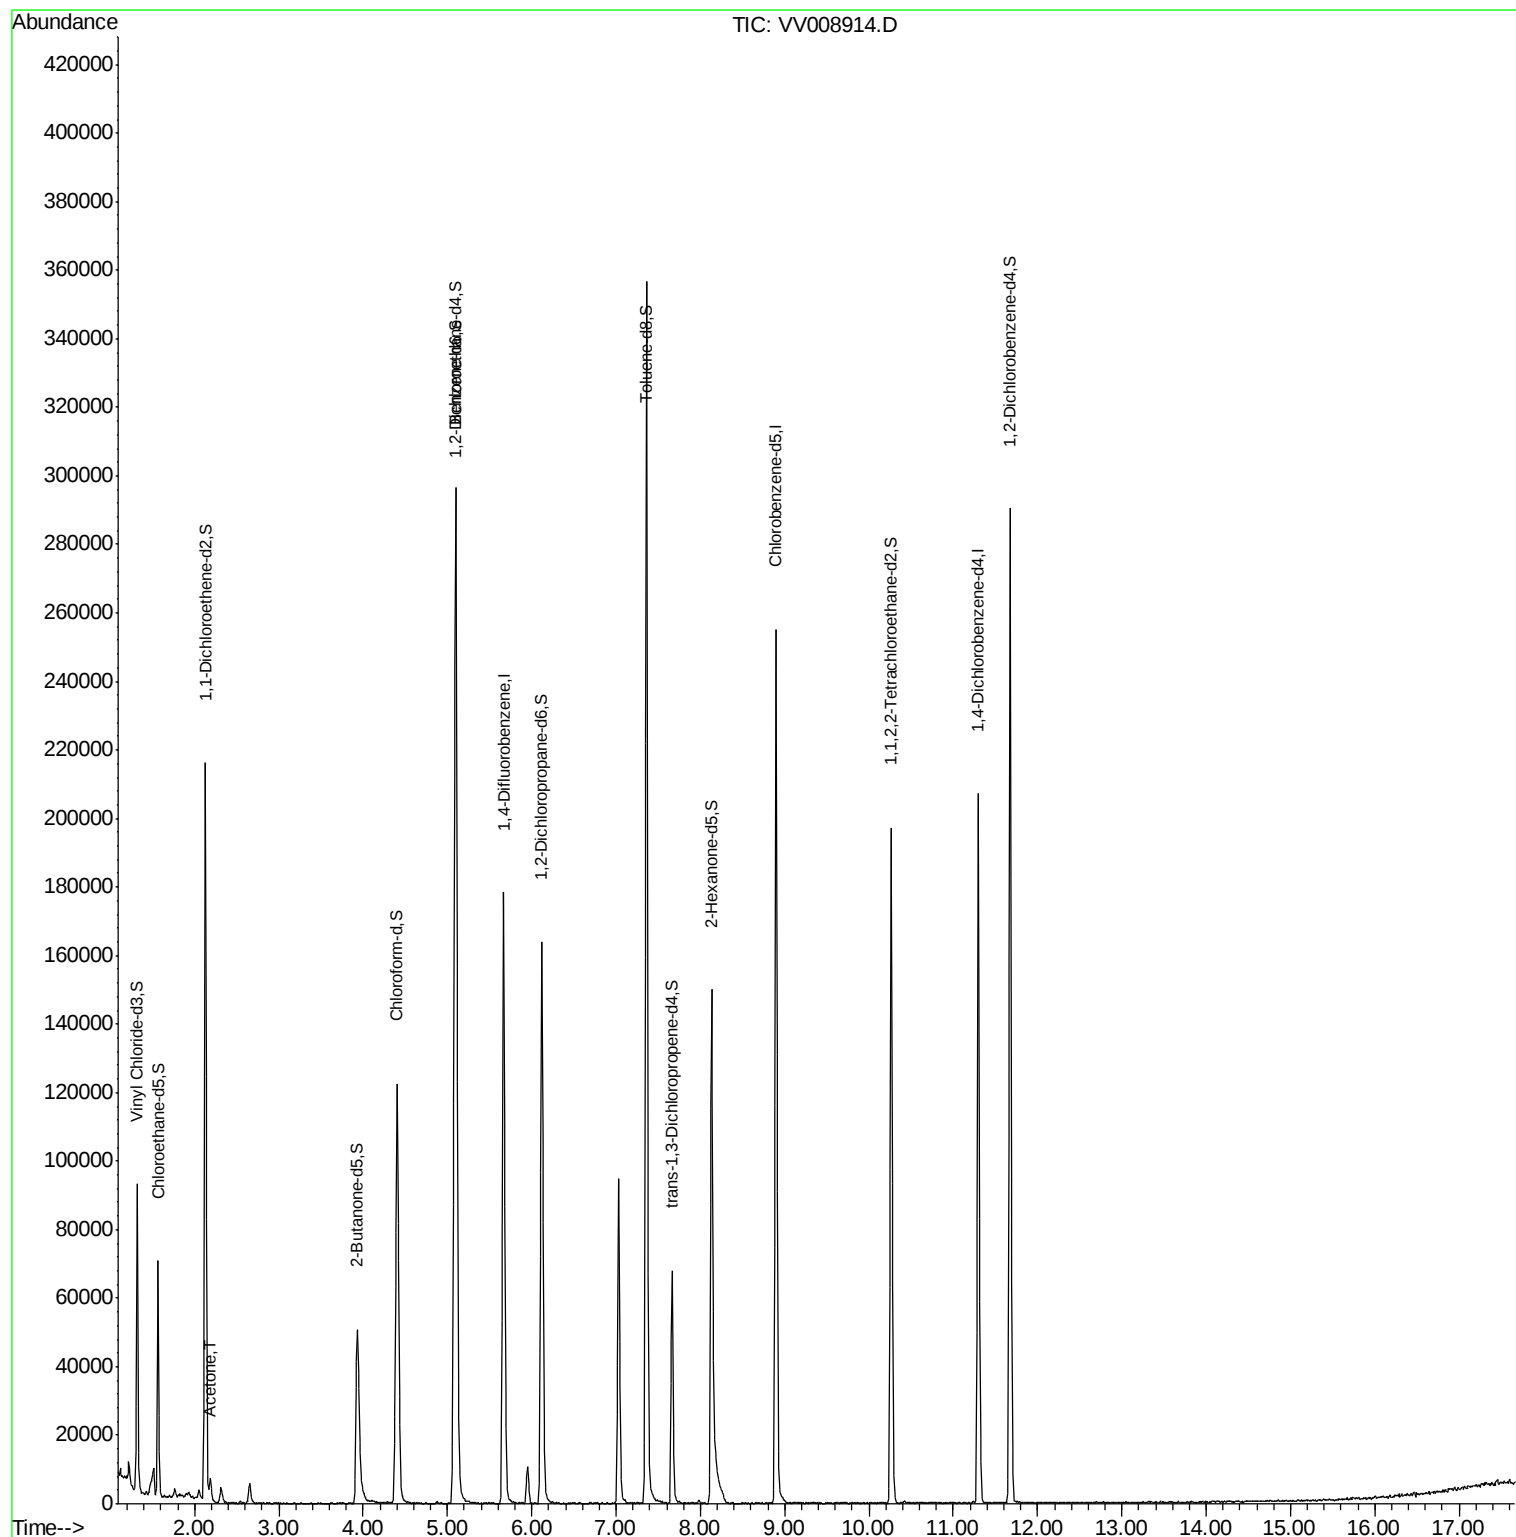

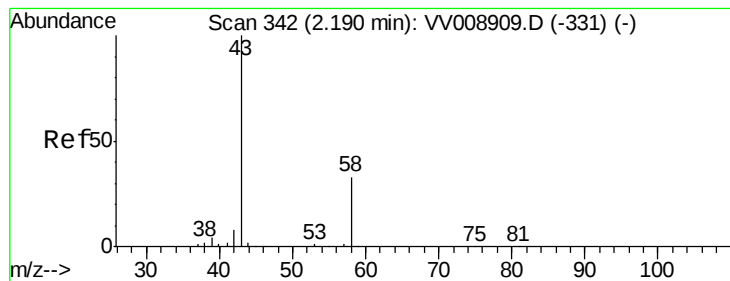

#13

Acetone

Concen: 3.253 ug/L

RT: 2.19 min Scan# 342

Delta R.T. 0.00 min

Lab File: VV008914.D

Acq: 13 Dec 2018 17:25

Instrument :
MSVOA_V
ClientSampleId :
COL40

Tot Ion: 43 Resp: 3048

Ion Ratio Lower Upper

43 100

58 32.5 0.0 61.8

