

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
 Data File : VV008915.D
 Acq On : 13 Dec 2018 17:49
 Operator : SY/MD
 Sample : J6367-05
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	92	rVB	85615	95101	12.69%	1.691%
2	1.566	141	148	163	rVB	67157	77909	10.40%	1.385%
3	2.042	292	296	297	rBV3	2780	1685	0.22%	0.030%
4	2.129	313	323	335	rBV	213841	300626	40.13%	5.346%
5	2.318	372	382	400	rBV3	4098	9206	1.23%	0.164%
6	2.437	413	419	422	rBV2	243	269	0.04%	0.005%
7	2.540	445	451	453	rBV2	586	564	0.08%	0.010%
8	2.653	474	486	502	rBV2	5276	11409	1.52%	0.203%
9	2.788	525	528	531	rBV	244	170	0.02%	0.003%
10	3.087	616	621	623	rBV	284	219	0.03%	0.004%
11	3.261	673	675	676	rBV	351	143	0.02%	0.003%
12	3.286	681	683	685	rVB	377	149	0.02%	0.003%
13	3.309	685	690	692	rBV	206	216	0.03%	0.004%
14	3.318	692	693	701	rVB	369	302	0.04%	0.005%
15	3.357	701	705	706	rBV	231	188	0.03%	0.003%
16	3.479	739	743	746	rBV	222	257	0.03%	0.005%
17	3.595	777	779	781	rVB2	251	137	0.02%	0.002%
18	3.611	782	784	788	rBB	186	152	0.02%	0.003%
19	3.637	789	792	794	rBB	184	114	0.02%	0.002%
20	3.659	795	799	802	rBV	280	238	0.03%	0.004%
21	3.736	819	823	825	rBB	144	128	0.02%	0.002%
22	3.797	840	842	845	rBV	159	92	0.01%	0.002%
23	3.862	860	862	866	rVB	186	96	0.01%	0.002%
24	3.933	870	884	916	rBV	51297	145069	19.36%	2.580%
25	4.267	985	988	993	rBV2	307	314	0.04%	0.006%
26	4.405	1013	1031	1054	rBV	120847	293100	39.12%	5.212%
27	4.650	1105	1107	1109	rBV	179	111	0.01%	0.002%
28	4.691	1118	1120	1122	rVB	239	112	0.01%	0.002%
29	4.717	1125	1128	1131	rBB	293	196	0.03%	0.003%
30	4.743	1131	1136	1139	rBB	353	268	0.04%	0.005%
31	4.778	1145	1147	1148	rBV	136	74	0.01%	0.001%
32	4.849	1167	1169	1171	rBV	278	181	0.02%	0.003%
33	4.904	1183	1186	1188	rBV	160	127	0.02%	0.002%
34	4.916	1188	1190	1193	rVV	209	119	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
 Data File : VV008915.D
 Acq On : 13 Dec 2018 17:49
 Operator : SY/MD
 Sample : J6367-05
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Title : VOC Analysis

35	4.958	1202	1203	1205	rVB	218	83	0.01%	0.001%
36	4.981	1206	1210	1212	rBV	155	132	0.02%	0.002%
37	5.035	1224	1227	1228	rBV	153	106	0.01%	0.002%
38	5.096	1228	1246	1277	rVV2	297526	749169	100.00%	13.322%
39	5.328	1316	1318	1322	rVB	424	261	0.03%	0.005%
40	5.367	1327	1330	1333	rVB	331	225	0.03%	0.004%
41	5.415	1343	1345	1349	rVB	266	152	0.02%	0.003%
42	5.441	1350	1353	1355	rBV	196	163	0.02%	0.003%
43	5.518	1373	1377	1381	rBV2	297	360	0.05%	0.006%
44	5.598	1399	1402	1404	rBV	213	149	0.02%	0.003%
45	5.666	1409	1423	1452	rBV	235687	469856	62.72%	8.355%
46	5.871	1485	1487	1491	rBV2	143	122	0.02%	0.002%
47	5.958	1500	1514	1532	rVB5	21078	46986	6.27%	0.836%
48	6.119	1546	1564	1590	rBV	160999	331593	44.26%	5.896%
49	6.248	1600	1604	1606	rBV2	634	462	0.06%	0.008%
50	6.318	1622	1626	1627	rBV3	246	183	0.02%	0.003%
51	6.360	1636	1639	1642	rBV2	142	103	0.01%	0.002%
52	6.469	1668	1673	1676	rBV2	391	377	0.05%	0.007%
53	6.627	1720	1722	1725	rBB	246	119	0.02%	0.002%
54	6.656	1728	1731	1737	rBV	193	273	0.04%	0.005%
55	6.698	1739	1744	1749	rBV3	500	499	0.07%	0.009%
56	6.823	1781	1783	1786	rVB	315	155	0.02%	0.003%
57	6.852	1786	1792	1794	rBV	270	277	0.04%	0.005%
58	6.868	1795	1797	1799	rVV	230	102	0.01%	0.002%
59	6.884	1799	1802	1807	rVB	307	238	0.03%	0.004%
60	6.932	1815	1817	1818	rVB	250	81	0.01%	0.001%
61	6.949	1819	1822	1823	rBV	183	130	0.02%	0.002%
62	7.032	1835	1848	1866	rBV	97322	170248	22.72%	3.027%
63	7.225	1905	1908	1911	rBV2	293	185	0.02%	0.003%
64	7.312	1932	1935	1937	rBV	184	101	0.01%	0.002%
65	7.360	1937	1950	1968	rBV	351968	618310	82.53%	10.995%
66	7.665	2033	2045	2062	rBV	68881	113715	15.18%	2.022%
67	7.788	2080	2083	2084	rBV	162	89	0.01%	0.002%
68	7.829	2092	2096	2100	rBV2	290	344	0.05%	0.006%
69	7.865	2104	2107	2110	rVV	257	141	0.02%	0.003%
70	8.135	2179	2191	2240	rBV	153277	325764	43.48%	5.793%
71	8.379	2265	2267	2269	rVB	225	90	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
Data File : VV008915.D
Acq On : 13 Dec 2018 17:49
Operator : SY/MD
Sample : J6367-05
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL41

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Title : VOC Analysis

72	8.415	2276	2278	2281	rBV	278	136	0.02%	0.002%
73	8.434	2281	2284	2290	rVB2	303	266	0.04%	0.005%
74	8.784	2389	2393	2396	rVB	227	166	0.02%	0.003%
75	8.836	2407	2409	2411	rBV	155	102	0.01%	0.002%
76	8.897	2416	2428	2464	rVV	336868	558957	74.61%	9.939%
77	9.058	2473	2478	2483	rVB2	423	425	0.06%	0.008%
78	9.093	2484	2489	2493	rVB	249	264	0.04%	0.005%
79	9.116	2493	2496	2497	rBV	155	89	0.01%	0.002%
80	9.588	2641	2643	2649	rVB2	328	177	0.02%	0.003%
81	9.688	2672	2674	2677	rVB	194	81	0.01%	0.001%
82	9.903	2738	2741	2746	rBV	164	105	0.01%	0.002%
83	10.026	2776	2779	2786	rVB2	259	246	0.03%	0.004%
84	10.077	2793	2795	2801	rVB2	217	231	0.03%	0.004%
85	10.128	2808	2811	2814	rBV	231	145	0.02%	0.003%
86	10.263	2841	2853	2874	rVB	199869	327875	43.77%	5.830%
87	10.653	2972	2974	2976	rBV	226	122	0.02%	0.002%
88	10.964	3068	3071	3077	rBV	204	163	0.02%	0.003%
89	11.193	3140	3142	3146	rBV	220	111	0.01%	0.002%
90	11.299	3163	3175	3198	rVB	280713	465340	62.11%	8.275%
91	11.379	3198	3200	3202	rBV2	249	140	0.02%	0.002%
92	11.517	3240	3243	3246	rBV	181	102	0.01%	0.002%
93	11.675	3279	3292	3310	rBV	294873	496697	66.30%	8.832%
94	11.816	3334	3336	3340	rBV	177	82	0.01%	0.001%
95	12.074	3413	3416	3418	rVB	315	155	0.02%	0.003%
96	12.415	3519	3522	3524	rVB	204	96	0.01%	0.002%
97	12.443	3525	3531	3534	rBV2	280	303	0.04%	0.005%
98	12.990	3698	3701	3704	rBV	328	200	0.03%	0.004%
99	13.977	4005	4008	4010	rBV2	386	273	0.04%	0.005%
100	15.035	4335	4337	4340	rVB2	561	213	0.03%	0.004%


Sum of corrected areas: 5623646

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
Data File : VV008915.D
Acq On : 13 Dec 2018 17:49
Operator : SY/MD
Sample : J6367-05
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

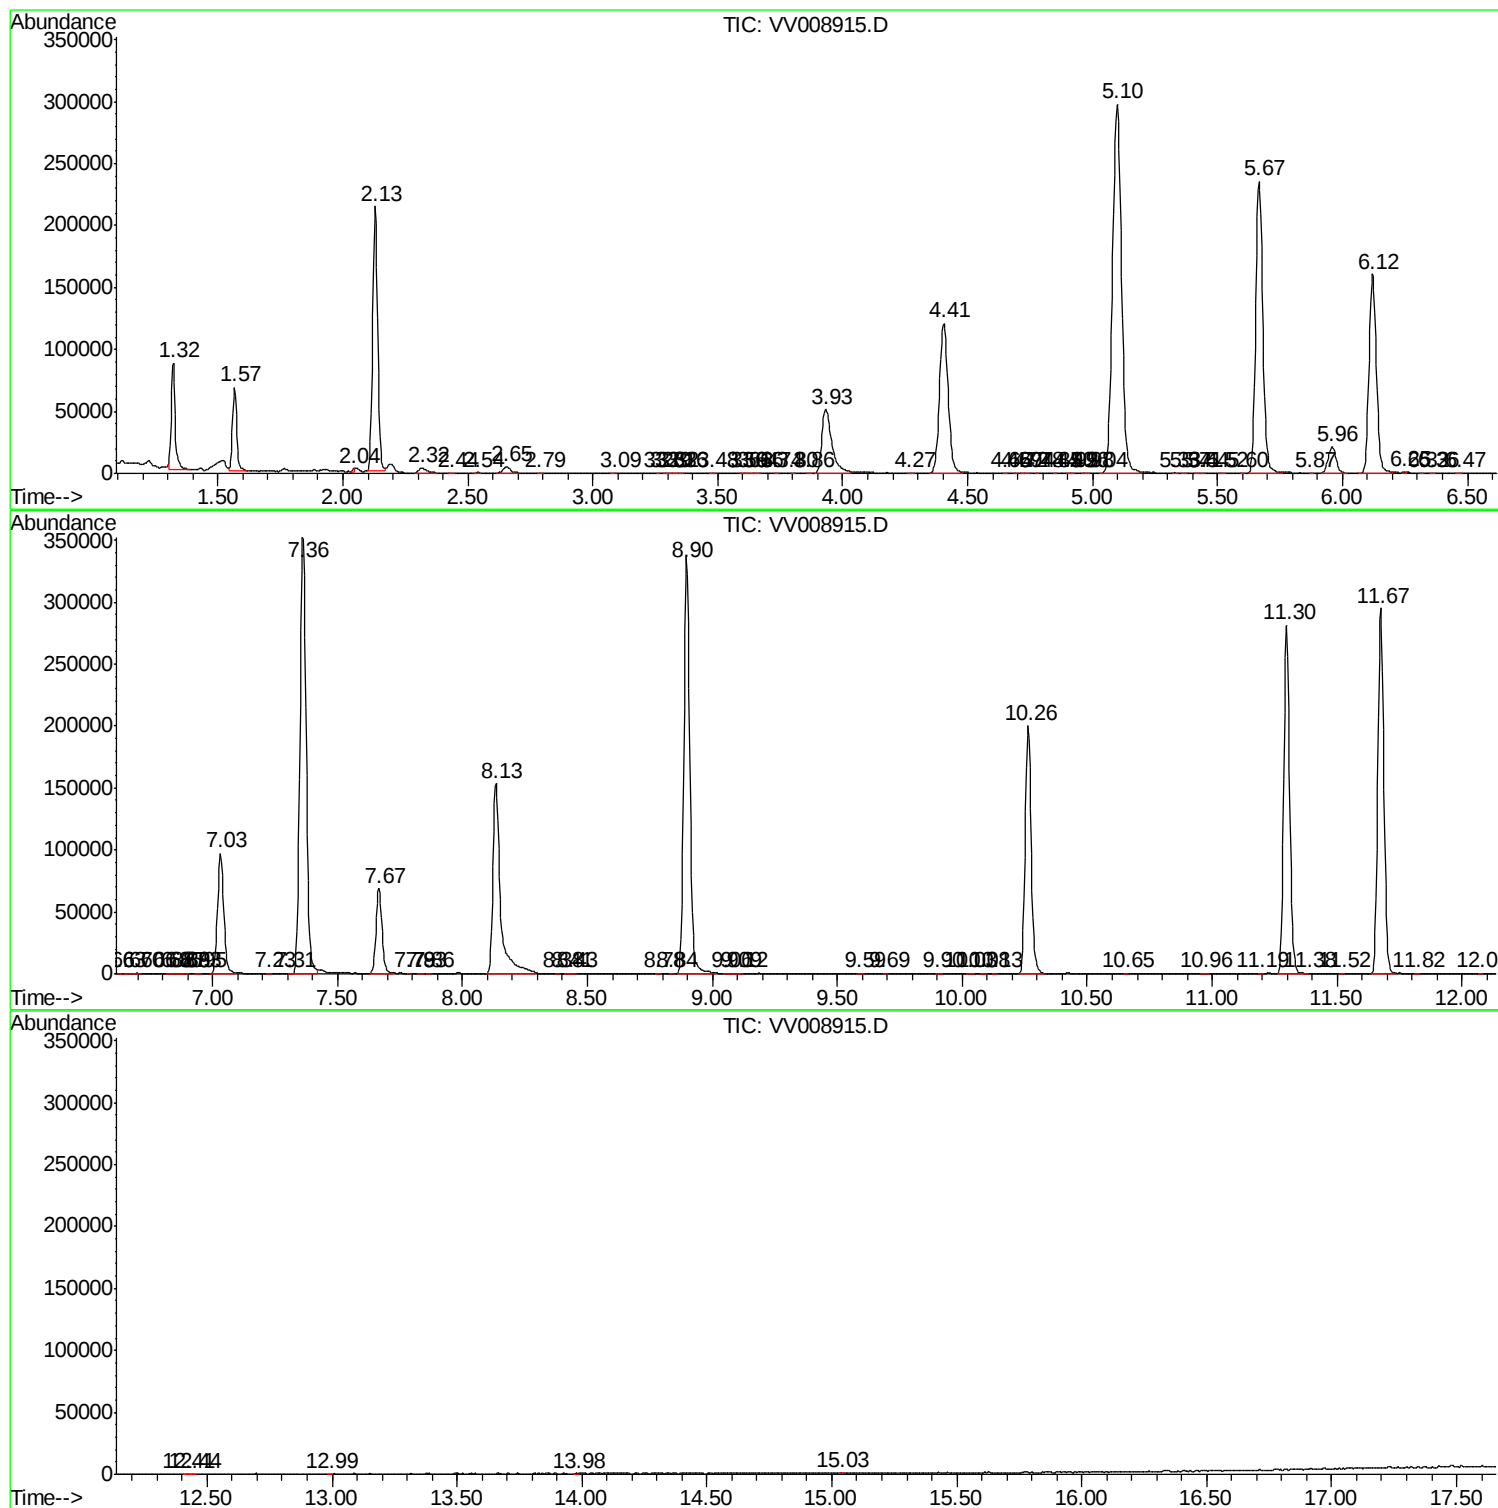

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
Data File : VV008915.D
Acq On : 13 Dec 2018 17:49
Operator : SY/MD
Sample : J6367-05
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
Data File : VV008915.D
Acq On : 13 Dec 2018 17:49
Operator : SY/MD
Sample : J6367-05
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc