

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
 Data File : VV008917.D
 Acq On : 13 Dec 2018 18:37
 Operator : SY/MD
 Sample : J6367-07
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	92	rVB	85283	95907	13.18%	1.752%
2	1.563	141	147	163	rVB	64317	74458	10.23%	1.360%
3	2.129	313	323	335	rBV	208182	298484	41.02%	5.452%
4	2.315	374	381	382	rBV2	3508	3404	0.47%	0.062%
5	2.563	455	458	461	rVB	180	80	0.01%	0.001%
6	2.653	473	486	502	rBV2	8163	17506	2.41%	0.320%
7	2.740	510	513	514	rBV2	150	70	0.01%	0.001%
8	2.862	544	551	554	rBV	226	324	0.04%	0.006%
9	2.881	554	557	561	rVB	170	110	0.02%	0.002%
10	2.917	566	568	571	rVB2	234	148	0.02%	0.003%
11	2.994	589	592	593	rBV	124	52	0.01%	0.001%
12	3.174	647	648	650	rBV	146	62	0.01%	0.001%
13	3.222	661	663	665	rBV	231	84	0.01%	0.002%
14	3.364	702	707	709	rBV	290	294	0.04%	0.005%
15	3.409	718	721	724	rVB2	185	105	0.01%	0.002%
16	3.537	759	761	763	rBV	208	68	0.01%	0.001%
17	3.640	790	793	795	rBV	170	138	0.02%	0.003%
18	3.708	811	814	815	rBV	129	55	0.01%	0.001%
19	3.743	822	825	829	rBV	177	195	0.03%	0.004%
20	3.766	830	832	834	rVV	125	62	0.01%	0.001%
21	3.856	858	860	863	rVB	167	75	0.01%	0.001%
22	3.933	868	884	921	rBV2	53352	163222	22.43%	2.981%
23	4.261	981	986	989	rBV2	246	327	0.04%	0.006%
24	4.402	1013	1030	1061	rBV	116234	282809	38.87%	5.166%
25	4.573	1081	1083	1085	rVB	139	55	0.01%	0.001%
26	4.618	1095	1097	1100	rBV	167	89	0.01%	0.002%
27	4.659	1100	1110	1115	rBV4	1115	2053	0.28%	0.037%
28	4.717	1124	1128	1129	rBV	159	134	0.02%	0.002%
29	4.791	1145	1151	1156	rBB2	299	379	0.05%	0.007%
30	4.827	1159	1162	1165	rBB	352	234	0.03%	0.004%
31	4.846	1166	1168	1171	rBV	263	188	0.03%	0.003%
32	5.010	1213	1219	1222	rBV	206	265	0.04%	0.005%
33	5.097	1228	1246	1273	rBV3	290390	727599	100.00%	13.290%
34	5.364	1326	1329	1330	rBV	246	103	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
 Data File : VV008917.D
 Acq On : 13 Dec 2018 18:37
 Operator : SY/MD
 Sample : J6367-07
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Title : VOC Analysis

35	5.376	1330	1333	1336	rVB2	293	205	0.03%	0.004%
36	5.415	1342	1345	1347	rVB	280	158	0.02%	0.003%
37	5.447	1348	1355	1358	rBV	334	372	0.05%	0.007%
38	5.528	1376	1380	1384	rBV2	225	144	0.02%	0.003%
39	5.666	1408	1423	1447	rBV	233077	462976	63.63%	8.456%
40	5.907	1495	1498	1500	rVB	396	193	0.03%	0.004%
41	5.949	1500	1511	1526	rVB3	10222	20398	2.80%	0.373%
42	6.026	1533	1535	1539	rVB2	207	115	0.02%	0.002%
43	6.055	1542	1544	1545	rBV2	234	97	0.01%	0.002%
44	6.119	1550	1564	1586	rBV	159362	321009	44.12%	5.863%
45	6.222	1595	1596	1599	rBV2	324	104	0.01%	0.002%
46	6.290	1614	1617	1620	rVB	161	99	0.01%	0.002%
47	6.315	1623	1625	1628	rVV	155	70	0.01%	0.001%
48	6.457	1666	1669	1671	rBV2	193	132	0.02%	0.002%
49	6.515	1685	1687	1690	rVB	153	87	0.01%	0.002%
50	6.544	1693	1696	1700	rVB2	146	91	0.01%	0.002%
51	6.637	1724	1725	1726	rVB	261	50	0.01%	0.001%
52	6.656	1726	1731	1732	rBV	196	113	0.02%	0.002%
53	6.958	1820	1825	1827	rBV	191	196	0.03%	0.004%
54	7.032	1835	1848	1867	rBV	93646	163908	22.53%	2.994%
55	7.267	1919	1921	1925	rVB	246	164	0.02%	0.003%
56	7.299	1925	1931	1934	rBV	189	249	0.03%	0.005%
57	7.360	1936	1950	1970	rBV	343127	598167	82.21%	10.926%
58	7.611	2025	2028	2030	rBV	283	189	0.03%	0.003%
59	7.666	2034	2045	2060	rBV	66107	109435	15.04%	1.999%
60	7.794	2082	2085	2086	rVB	219	104	0.01%	0.002%
61	7.807	2087	2089	2091	rBV	240	100	0.01%	0.002%
62	7.900	2116	2118	2123	rVB	166	60	0.01%	0.001%
63	7.926	2124	2126	2132	rVB	290	243	0.03%	0.004%
64	7.955	2132	2135	2137	rBV	198	158	0.02%	0.003%
65	7.978	2137	2142	2145	rBV2	575	573	0.08%	0.010%
66	8.029	2157	2158	2161	rVB	172	48	0.01%	0.001%
67	8.064	2166	2169	2171	rBV	150	94	0.01%	0.002%
68	8.135	2178	2191	2219	rBV	155502	318857	43.82%	5.824%
69	8.351	2254	2258	2263	rBV2	219	214	0.03%	0.004%
70	8.415	2275	2278	2281	rVB	140	77	0.01%	0.001%
71	8.566	2322	2325	2328	rVB	251	137	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
 Data File : VV008917.D
 Acq On : 13 Dec 2018 18:37
 Operator : SY/MD
 Sample : J6367-07
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Title : VOC Analysis

72	8.614	2338	2340	2343	rBV	183	76	0.01%	0.001%
73	8.659	2353	2354	2356	rBB	117	44	0.01%	0.001%
74	8.698	2363	2366	2370	rVB	253	130	0.02%	0.002%
75	8.897	2415	2428	2452	rBV	329148	541123	74.37%	9.884%
76	9.116	2494	2496	2497	rVB	257	70	0.01%	0.001%
77	9.177	2513	2515	2521	rBV2	199	179	0.02%	0.003%
78	9.244	2534	2536	2540	rVB	210	114	0.02%	0.002%
79	9.264	2540	2542	2544	rBV	185	95	0.01%	0.002%
80	9.466	2602	2605	2606	rBV	254	80	0.01%	0.001%
81	9.563	2633	2635	2638	rBV	160	76	0.01%	0.001%
82	9.727	2684	2686	2687	rBV	308	147	0.02%	0.003%
83	9.765	2695	2698	2702	rBV	137	130	0.02%	0.002%
84	10.087	2795	2798	2800	rBV	182	142	0.02%	0.003%
85	10.222	2837	2840	2841	rVB	145	58	0.01%	0.001%
86	10.264	2841	2853	2873	rBV2	197400	323045	44.40%	5.901%
87	10.415	2897	2900	2901	rBV	451	240	0.03%	0.004%
88	10.723	2994	2996	2998	rBV	230	94	0.01%	0.002%
89	10.778	3011	3013	3017	rBV	270	123	0.02%	0.002%
90	11.231	3150	3154	3155	rBV	365	188	0.03%	0.003%
91	11.296	3162	3174	3196	rBV	277019	456509	62.74%	8.338%
92	11.608	3268	3271	3273	rBV	240	120	0.02%	0.002%
93	11.675	3280	3292	3315	rVB	281457	482402	66.30%	8.811%
94	11.775	3322	3323	3325	rBV	215	89	0.01%	0.002%
95	11.826	3336	3339	3342	rBV2	169	158	0.02%	0.003%
96	12.170	3444	3446	3448	rBV	195	73	0.01%	0.001%
97	12.698	3607	3610	3613	rVB	329	248	0.03%	0.005%
98	12.717	3613	3616	3619	rBV	293	201	0.03%	0.004%
99	12.936	3682	3684	3687	rBV	184	84	0.01%	0.002%
100	13.325	3802	3805	3808	rBV2	302	269	0.04%	0.005%


Sum of corrected areas: 5474831

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
Data File : VV008917.D
Acq On : 13 Dec 2018 18:37
Operator : SY/MD
Sample : J6367-07
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
COL43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

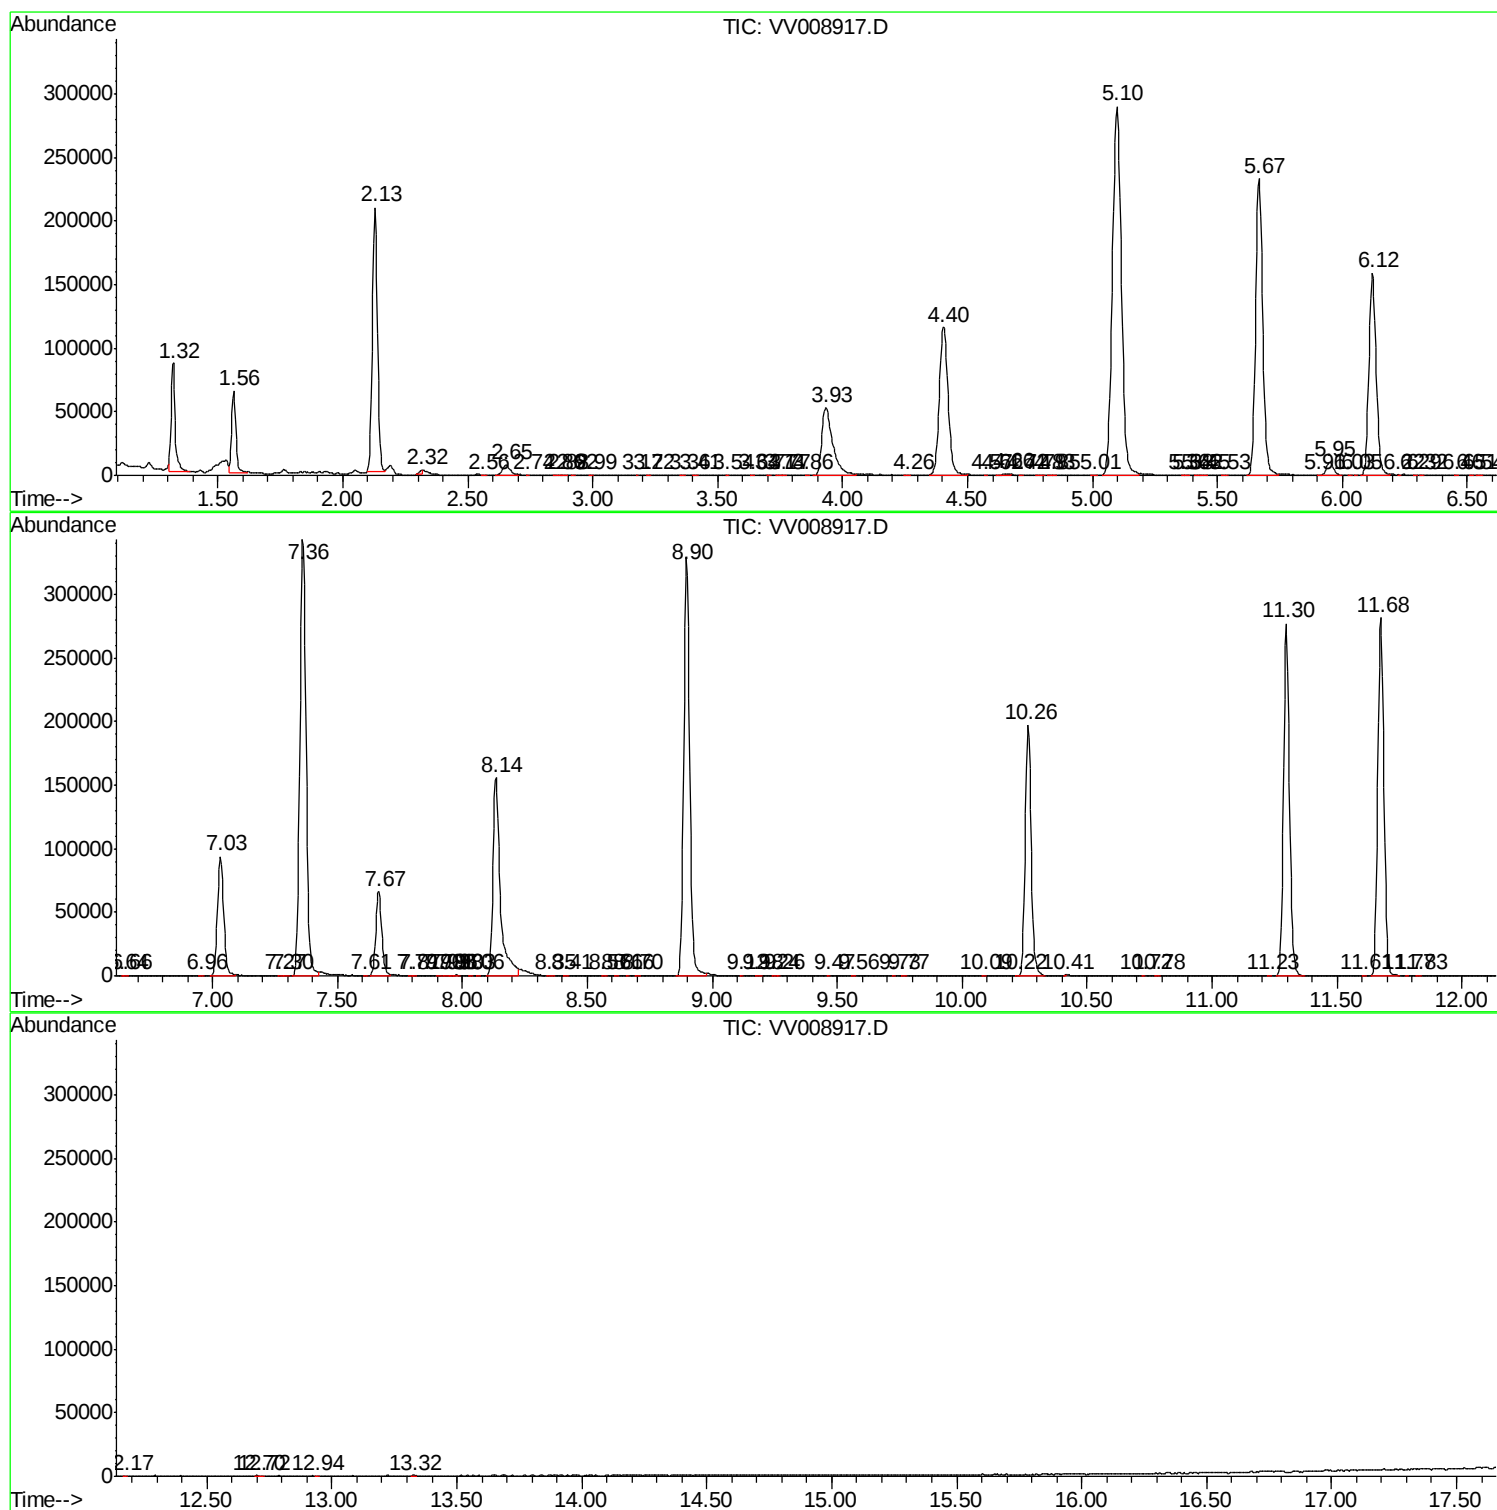

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
Data File : VV008917.D
Acq On : 13 Dec 2018 18:37
Operator : SY/MD
Sample : J6367-07
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
Data File : VV008917.D
Acq On : 13 Dec 2018 18:37
Operator : SY/MD
Sample : J6367-07
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL43

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc