


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121318\
Data File : VV008901.D
Acq On : 13 Dec 2018 11:00
Operator : SY/MD
Sample : BFB59
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB59

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
Title : VOC Analysis
Last Update : Fri Dec 14 01:09:42 2018

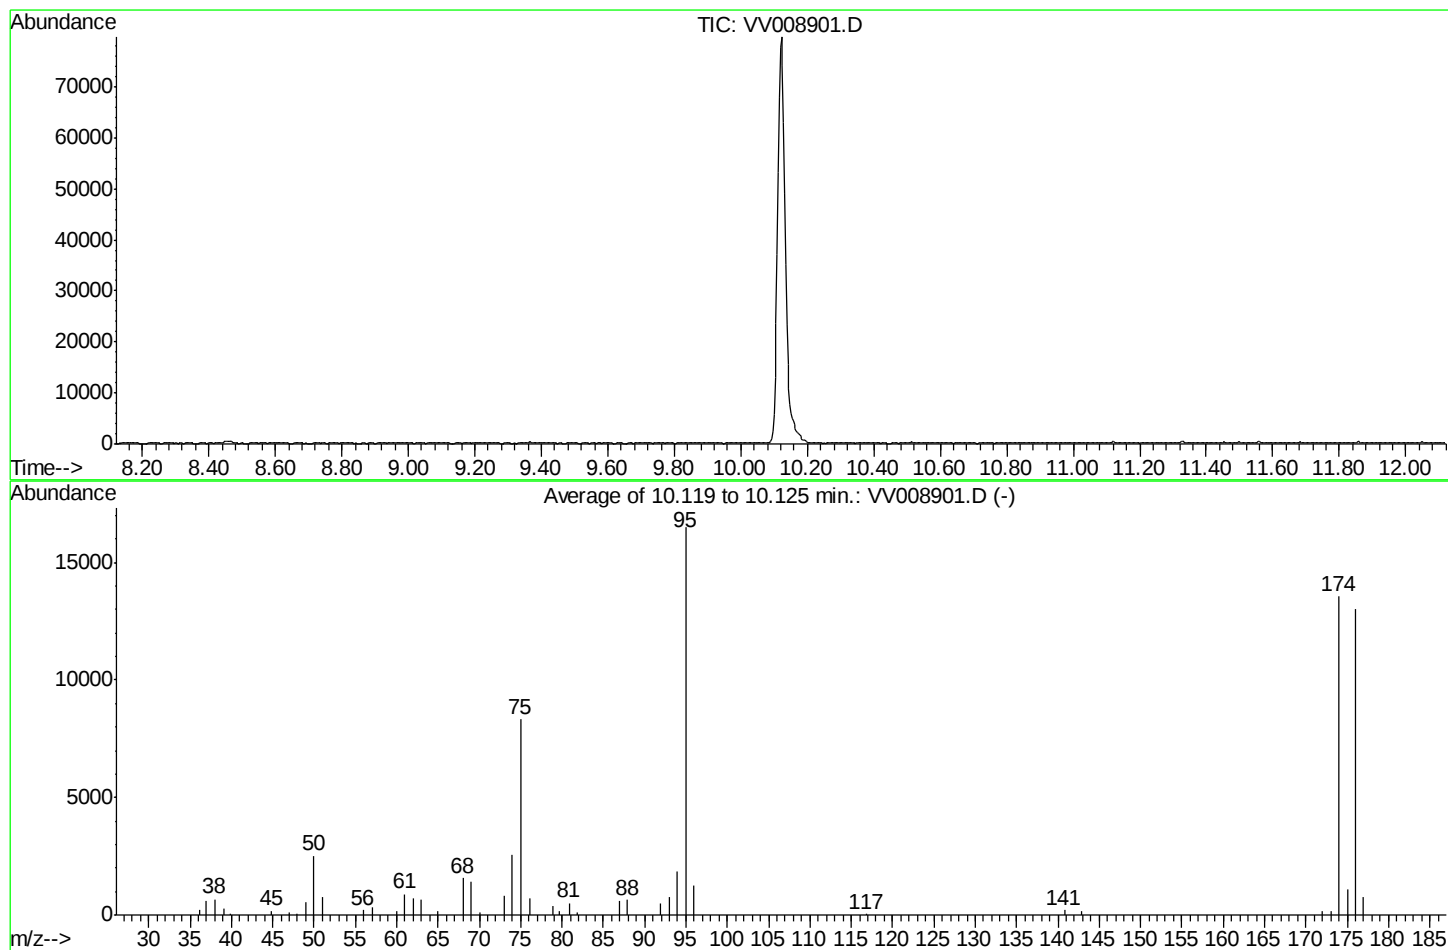

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	2513	PASS
75	95	30	80	50.4	8316	PASS
95	95	100	100	100.0	16494	PASS
96	95	5	9	7.6	1248	PASS
173	174	0.00	2	1.1	148	PASS
174	95	50	120	82.2	13557	PASS
175	174	5	9	7.9	1067	PASS
176	174	95	101	96.0	13016	PASS
177	176	5	9	5.8	757	PASS

m/z	Abundance
44.00	254.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

m/z	Abundance
36.10	183.0
37.00	581.0
38.00	637.0
39.00	241.0
44.00	226.0
44.90	175.0
46.90	116.0
48.00	108.0
49.00	541.0
50.00	2347.0
51.00	787.0
56.00	194.0
57.00	280.0
60.00	142.0
61.00	841.0
62.00	694.0
63.00	597.0
64.90	148.0
68.00	1522.0
69.00	1276.0
70.00	119.0
73.00	822.0
74.00	2582.0
75.00	7897.0
76.00	609.0
78.90	399.0
79.70	158.0
80.90	500.0
81.90	106.0
86.90	560.0
87.90	616.0
91.90	422.0
93.00	750.0
94.00	1784.0
95.00	15650.0
96.00	1296.0
116.90	102.0
140.80	158.0
142.90	169.0
171.90	144.0
174.00	12952.0
175.00	948.0
176.00	13193.0
177.00	721.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

m/z	Abundance
36.10	206.0
37.00	635.0
38.00	684.0
39.00	285.0
44.00	242.0
44.90	173.0
46.90	132.0
48.00	113.0
49.00	565.0
50.00	2577.0
51.00	794.0
55.90	211.0
57.00	327.0
60.00	195.0
61.00	901.0
62.10	764.0
63.00	684.0
64.90	160.0
68.00	1600.0
69.00	1424.0
70.00	144.0
73.00	883.0
74.00	2653.0
75.00	8638.0
76.10	744.0
78.80	389.0
79.80	188.0
80.90	540.0
81.90	116.0
86.90	621.0
87.90	665.0
91.90	497.0
93.00	755.0
94.00	1919.0
95.00	17120.0
96.00	1290.0
140.90	208.0
142.90	185.0
171.90	161.0
173.10	205.0
174.00	13904.0
175.00	1108.0
176.00	13372.0
177.00	784.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

m/z	Abundance
36.10	191.0
37.00	640.0
37.90	651.0
39.10	316.0
39.90	121.0
44.00	235.0
44.90	182.0
47.00	161.0
49.00	564.0
50.00	2616.0
51.00	743.0
55.90	226.0
57.00	301.0
60.00	211.0
61.00	875.0
62.10	723.0
63.00	681.0
65.00	155.0
68.00	1556.0
69.00	1527.0
70.00	144.0
73.00	791.0
74.00	2493.0
75.00	8414.0
76.10	745.0
78.90	403.0
79.80	171.0
80.90	502.0
81.90	107.0
87.00	606.0
87.90	649.0
91.90	522.0
92.90	749.0
94.00	1828.0
95.00	16712.0
96.00	1158.0
140.90	230.0
142.80	197.0
171.90	171.0
173.10	240.0
174.00	13816.0
175.00	1146.0
176.00	12483.0
177.00	767.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59