
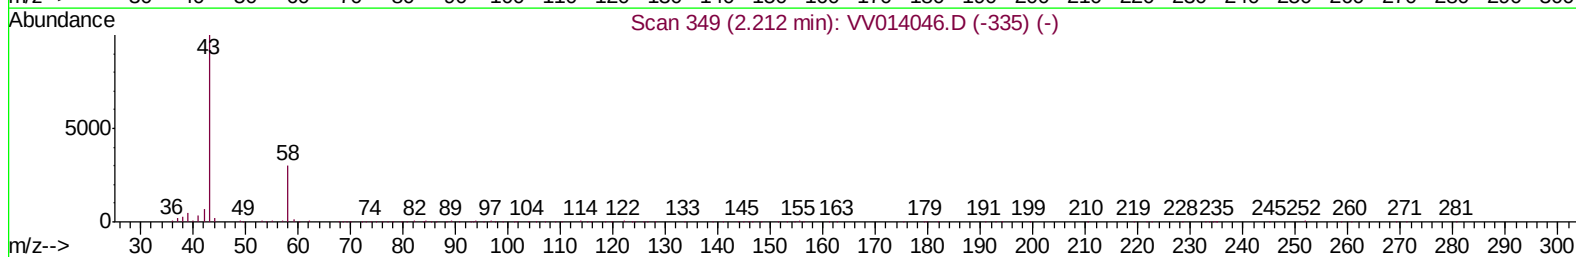
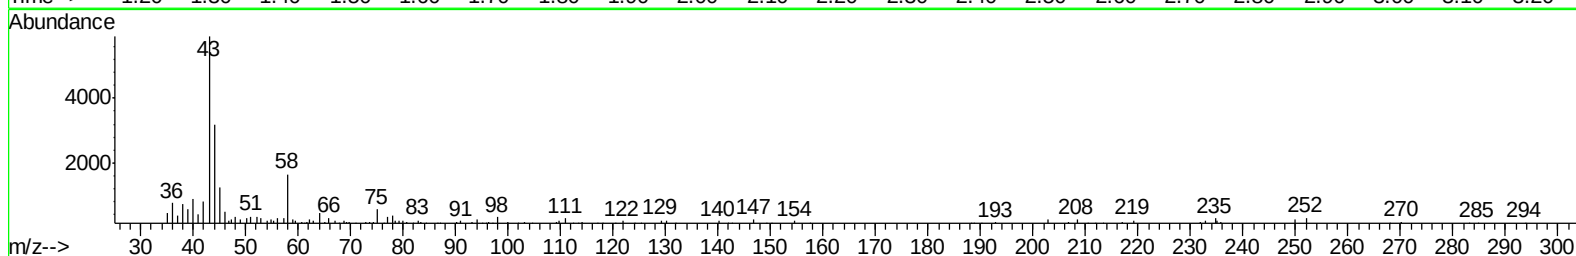


Data File : VV014051.D
Acq On : 13 Dec 2019 14:14
Operator : SY/MD
Sample : K6281-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 14 03:28:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 14 03:25:09 2019
Response via : Initial Calibration

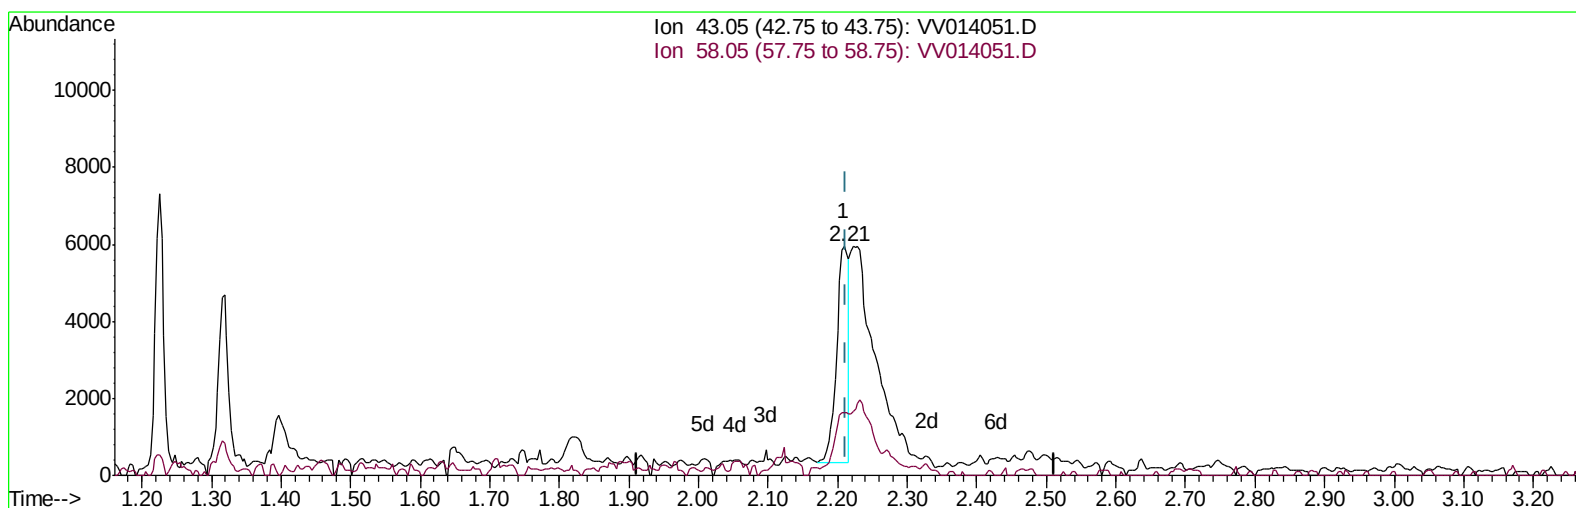

TIC: VV014051.D

(13) Acetone (T)

2.209min (-0.003) 2.14ug/L

response 6783

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	31.05#
0.00	0.00	0.00
0.00	0.00	0.00