


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121319\
 Data File : VV014045.D
 Acq On : 13 Dec 2019 09:47
 Operator : SY/MD
 Sample : BFB41
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Dec 16 13:26:15 2019

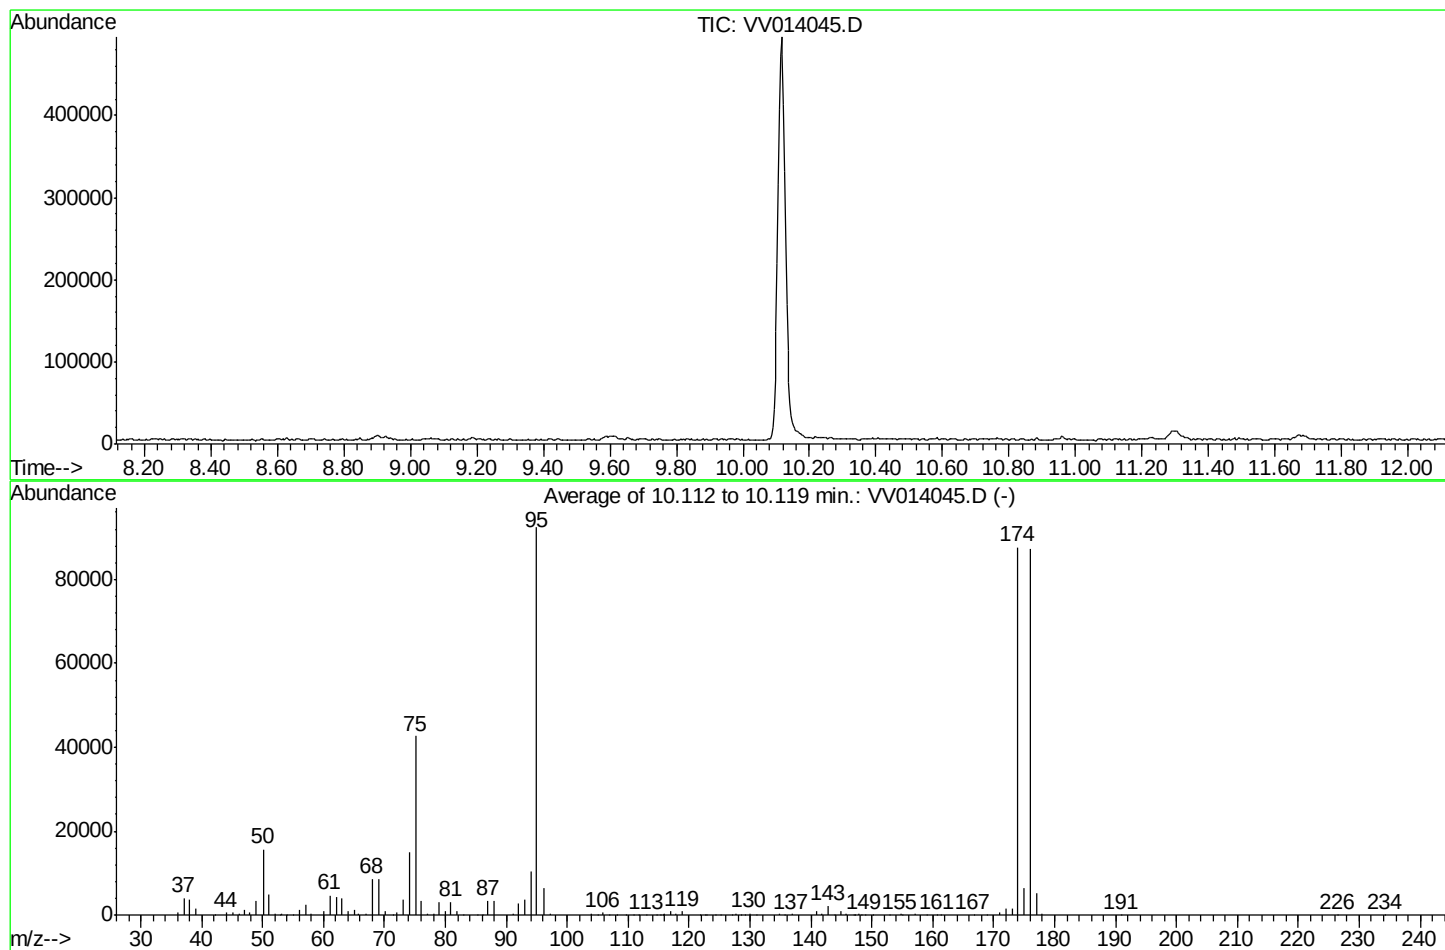

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	15627	PASS
75	95	30	80	46.2	42716	PASS
95	95	100	100	100.0	92434	PASS
96	95	5	9	6.8	6294	PASS
173	174	0.00	2	1.6	1442	PASS
174	95	50	120	94.9	87752	PASS
175	174	5	9	7.4	6464	PASS
176	174	95	101	99.4	87248	PASS
177	176	5	9	6.1	5336	PASS

m/z	Abundance
36.00	924.0
37.10	4097.0
38.10	3810.0
39.10	1838.0
40.00	878.0
40.70	102.0
41.50	120.0
42.20	126.0
42.90	105.0
44.00	1319.0
45.10	897.0
46.00	355.0
47.10	1140.0
47.90	667.0
49.00	3160.0
50.10	15593.0
51.10	4911.0
52.00	501.0
53.10	249.0
54.10	174.0
55.00	257.0
56.00	1297.0
57.00	2404.0
57.90	142.0
60.10	983.0
61.00	4443.0
62.00	4287.0
63.00	3898.0
64.00	874.0
65.00	966.0
65.70	206.0
66.90	308.0
68.00	8776.0
69.10	8943.0
70.10	842.0
71.30	121.0
72.00	518.0
73.00	4096.0
74.00	14679.0
75.10	43160.0
76.00	3513.0
77.00	480.0
78.10	444.0
78.90	2959.0
80.00	966.0
80.90	3140.0
81.90	769.0
83.00	155.0
85.20	127.0
86.10	155.0
87.00	3692.0
87.90	3408.0
91.00	373.0
92.00	2876.0
93.00	3690.0
94.10	10175.0
95.00	90832.0
96.10	6199.0
97.20	239.0
104.00	375.0
105.00	155.0
105.90	500.0
107.00	129.0
108.10	136.0
109.60	168.0
111.00	160.0
111.70	107.0
113.00	124.0
114.60	119.0
115.70	264.0
116.90	732.0
117.80	267.0
118.90	840.0
121.90	159.0
122.90	115.0
125.10	115.0
127.10	114.0
127.80	278.0
130.00	466.0
131.00	136.0
134.90	164.0
136.90	238.0
140.90	842.0
141.90	165.0
142.90	2041.0
143.80	192.0
145.00	1016.0
145.80	127.0
147.00	103.0
147.80	211.0
148.20	147.0
148.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

150.20	109.0
152.90	199.0
154.90	320.0
157.10	283.0
158.90	130.0
160.80	202.0
166.70	144.0
168.90	105.0
171.00	458.0
171.90	1242.0
173.00	1342.0
174.00	83504.0
175.00	6684.0
176.00	84536.0
177.00	5387.0
177.90	244.0
226.50	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.00	864.0
37.10	4266.0
38.10	3715.0
39.00	1857.0
40.00	921.0
42.10	157.0
42.80	104.0
44.00	1283.0
45.10	909.0
46.10	308.0
47.00	1094.0
47.90	643.0
49.00	3295.0
50.10	16334.0
51.10	4995.0
52.00	437.0
52.90	224.0
53.10	225.0
54.00	197.0
55.00	223.0
56.00	1361.0
57.00	2412.0
58.00	184.0
60.10	963.0
61.00	4699.0
62.10	4274.0
63.00	4027.0
64.00	903.0
65.00	1173.0
65.80	197.0
66.90	245.0
68.00	9014.0
69.00	8797.0
70.00	752.0
71.30	166.0
72.10	553.0
73.00	4066.0
74.00	15635.0
75.10	43656.0
76.00	3634.0
77.10	500.0
78.00	485.0
78.90	3148.0
80.00	1042.0
80.90	3178.0
81.90	868.0
82.90	149.0
86.20	302.0
87.00	3545.0
87.90	3685.0
91.00	370.0
92.00	2928.0
93.00	3992.0
94.10	10750.0
95.00	95256.0
96.10	6538.0
97.20	228.0
104.00	371.0
105.00	126.0
105.90	518.0
106.90	167.0
108.00	163.0
109.60	142.0
110.90	169.0
113.00	137.0
114.70	121.0
115.20	104.0
116.00	325.0
117.00	814.0
117.90	267.0
118.90	908.0
121.90	149.0
122.80	120.0
124.30	103.0
127.00	115.0
127.80	375.0
128.50	189.0
129.20	102.0
129.90	469.0
131.00	161.0
134.90	173.0
136.90	257.0
140.90	901.0
141.80	186.0
142.90	2318.0
145.00	971.0
145.90	185.0
147.20	117.0
147.80	246.0
148.90	139.0
150.20	130.0
152.80	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

154.70	292.0
157.10	280.0
158.90	123.0
160.70	121.0
161.20	164.0
166.70	120.0
168.80	101.0
171.10	559.0
171.90	1462.0
173.00	1465.0
174.00	90240.0
175.00	6683.0
176.00	90464.0
177.00	5539.0
177.90	231.0
226.40	113.0
234.30	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.00	733.0
37.10	4132.0
38.00	3360.0
39.00	1654.0
40.00	849.0
42.10	165.0
42.70	114.0
44.00	1128.0
45.00	723.0
46.20	276.0
47.00	1078.0
47.90	547.0
49.00	3263.0
50.10	15342.0
51.10	4711.0
52.10	313.0
52.80	243.0
54.00	228.0
55.20	188.0
56.00	1236.0
57.00	2194.0
58.10	237.0
60.10	772.0
61.10	4634.0
62.10	3962.0
63.00	3847.0
64.00	804.0
65.00	1279.0
65.80	180.0
66.90	169.0
68.00	8272.0
69.00	8288.0
70.00	736.0
71.30	142.0
72.10	585.0
73.10	3595.0
74.10	14662.0
75.10	41712.0
76.00	3376.0
77.10	552.0
78.00	439.0
78.90	3086.0
80.00	1077.0
80.90	2965.0
81.90	803.0
82.80	179.0
87.00	3274.0
88.00	3598.0
91.10	301.0
92.00	2674.0
93.00	3785.0
94.10	10356.0
95.00	91216.0
96.10	6147.0
97.10	228.0
103.90	351.0
104.90	124.0
105.90	455.0
106.90	186.0
108.00	186.0
110.90	129.0
113.10	108.0
114.70	132.0
116.00	422.0
117.00	845.0
117.90	262.0
118.90	853.0
121.90	113.0
122.60	106.0
127.00	115.0
127.80	405.0
128.50	151.0
129.20	141.0
129.90	352.0
131.10	167.0
134.90	180.0
135.60	105.0
136.90	216.0
140.90	844.0
141.80	147.0
142.90	2229.0
144.80	823.0
145.90	241.0
147.20	177.0
147.90	277.0
148.80	114.0
150.30	136.0
154.70	297.0
155.10	192.0
157.00	246.0
158.90	142.0
161.20	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

171.10	520.0
172.00	1574.0
173.00	1520.0
174.00	89512.0
175.00	6026.0
176.00	86744.0
177.00	5082.0
177.90	209.0
191.00	115.0
234.30	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.00	168.0
37.20	131.0
37.80	178.0
38.90	159.0
39.90	994.0
40.70	200.0
41.60	173.0
42.80	135.0
44.00	665.0
45.10	149.0
45.80	135.0
48.40	154.0
48.70	127.0
49.40	130.0
50.30	129.0
51.20	101.0
54.00	122.0
55.40	173.0
61.30	127.0
67.50	131.0
68.30	121.0
73.10	121.0
75.10	126.0
75.90	116.0
76.70	144.0
77.10	126.0
87.80	165.0
127.60	111.0
151.30	119.0
221.80	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41