

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121321\
 Data File : VV023944.D
 Acq On : 13 Dec 2021 13:10
 Operator : SY/MD
 Sample : M4971-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 14 01:07:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 23 02:04:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7287	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.864	117	7420	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.244	152	4312	0.500	ug/L	-0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	3747	0.506	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 102.000%			
4) 1,2-Dichloroethane-d4	5.043	65	2631	0.523	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 104.000%			
7) 1,2-Dichloropropane-d6	6.069	67	2812	0.436	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 88.000%			
8) Toluene-d8	7.317	98	9622	0.577	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 116.000%			
10) 1,1,2,2-Tetrachloroeth...	10.216	84	1957	0.500	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 100.000%			
Target Compounds					Qvalue	
13) 1,2-Dibromo-3-chloropr...	12.238	75	29	0.044	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121321\
Data File : VV023944.D
Acq On : 13 Dec 2021 13:10
Operator : SY/MD
Sample : M4971-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 14 01:07:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 23 02:04:29 2021
Response via : Initial Calibration

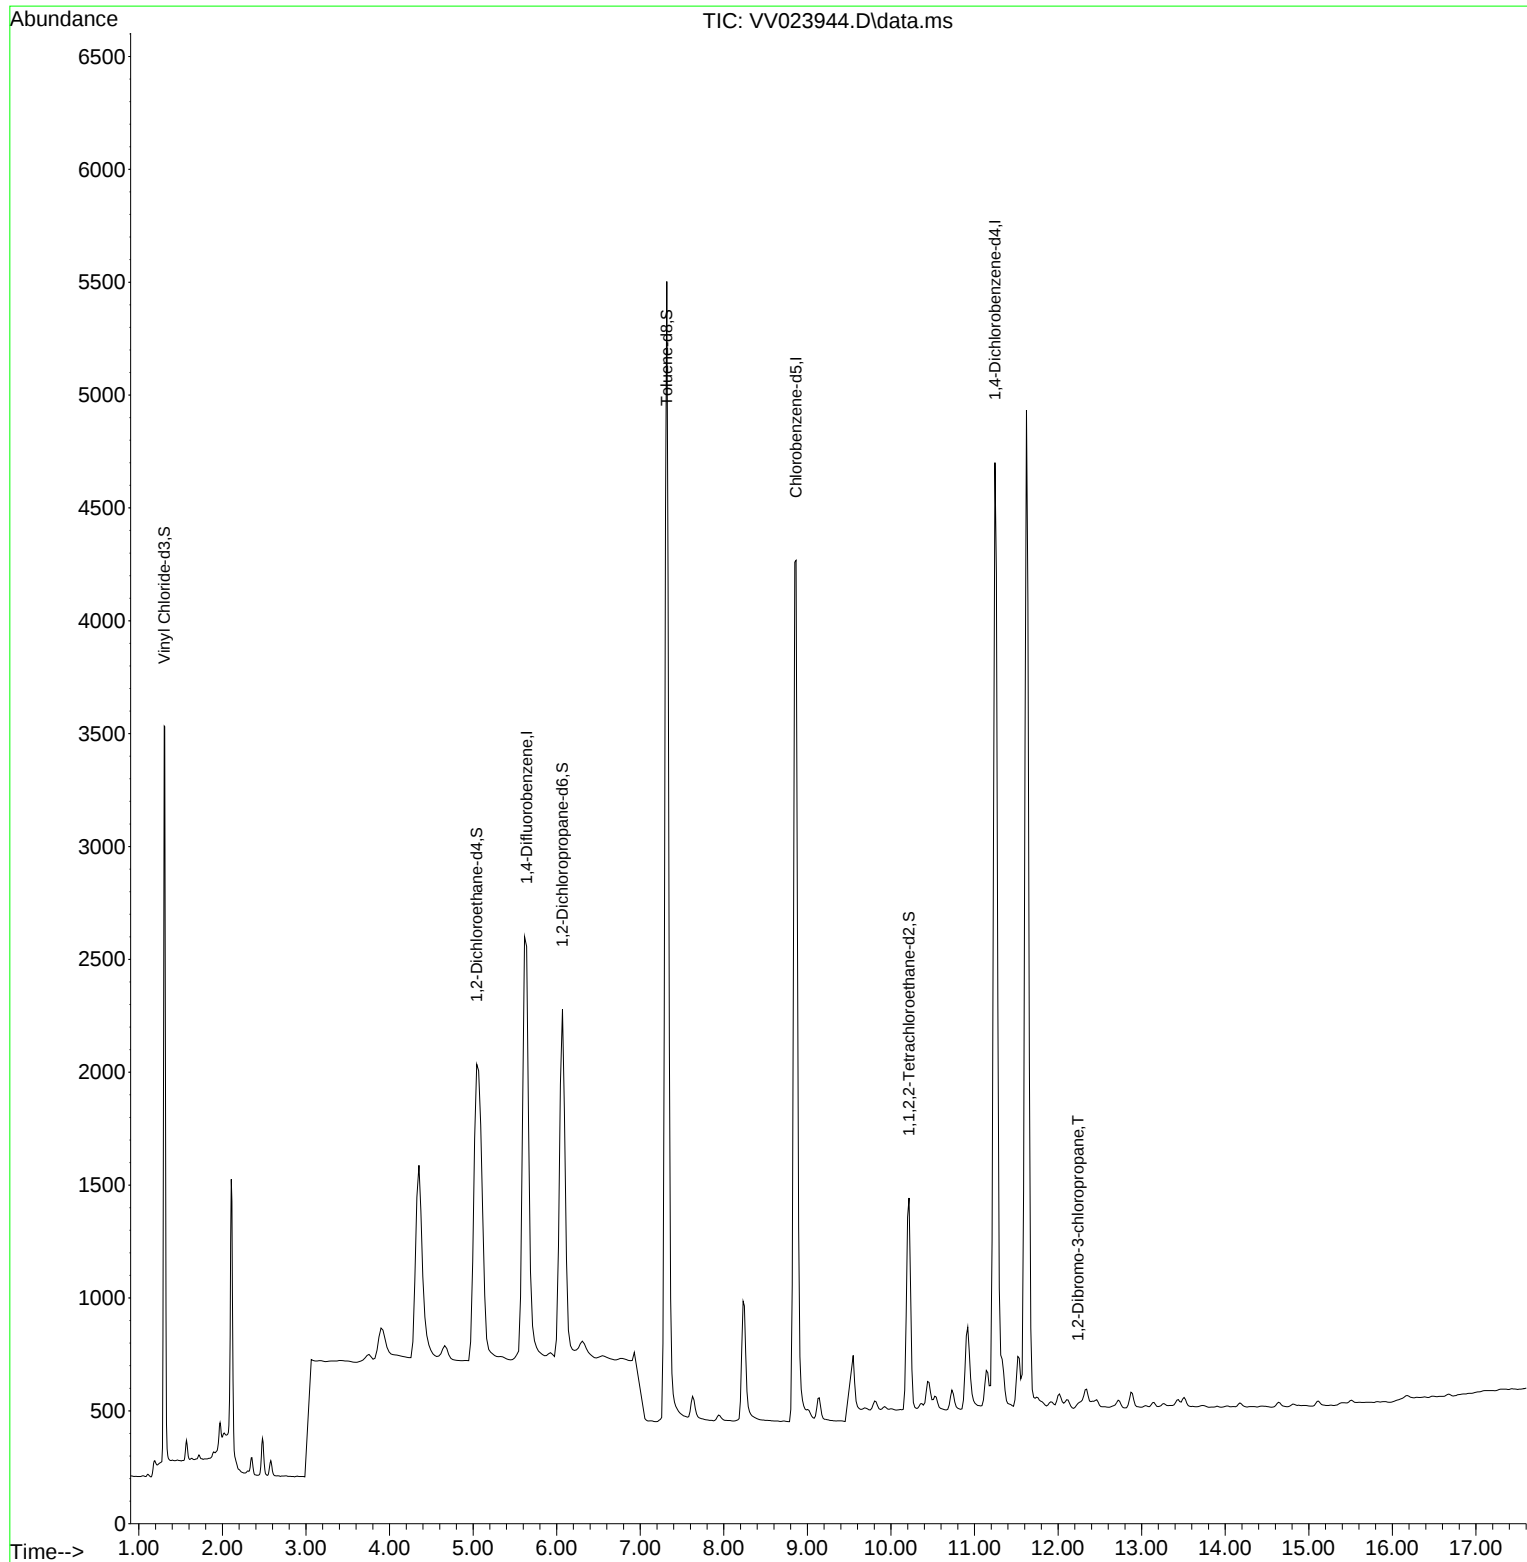

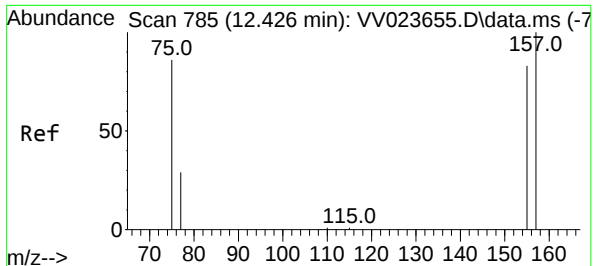

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.044 ug/L
 RT: 12.238 min Scan# 71
 Delta R.T. -0.188 min
 Lab File: VV023944.D
 Acq: 13 Dec 2021 13:10

Instrument :
 MSVOA_V
 ClientSampleId :

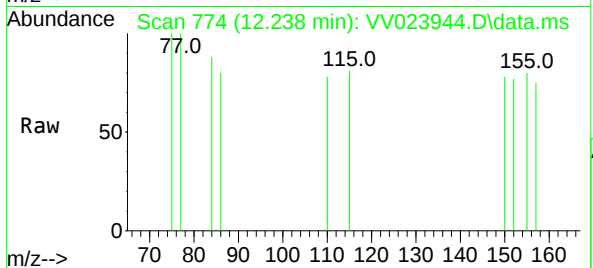

Tgt Ion: 75 Resp: 29
 Ion Ratio Lower Upper
 75 100
 157 75.0 85.7 128.5#
 155 79.7 74.3 111.5

