

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121321\
 Data File : VV023948.D
 Acq On : 13 Dec 2021 14:45
 Operator : SY/MD
 Sample : M4971-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 14 01:08:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 23 02:04:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7640	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.864	117	7570	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.244	152	4475	0.500	ug/L	-0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	4659	0.600	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	120.000%
4) 1,2-Dichloroethane-d4	5.042	65	2852	0.541	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	6.069	67	3144	0.478	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	96.000%
8) Toluene-d8	7.317	98	9918	0.583	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	116.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2150	0.538	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.000%
Target Compounds						
3) Vinyl chloride	1.310	62	18010	2.104	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121321\
Data File : VV023948.D
Acq On : 13 Dec 2021 14:45
Operator : SY/MD
Sample : M4971-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 14 01:08:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 23 02:04:29 2021
Response via : Initial Calibration

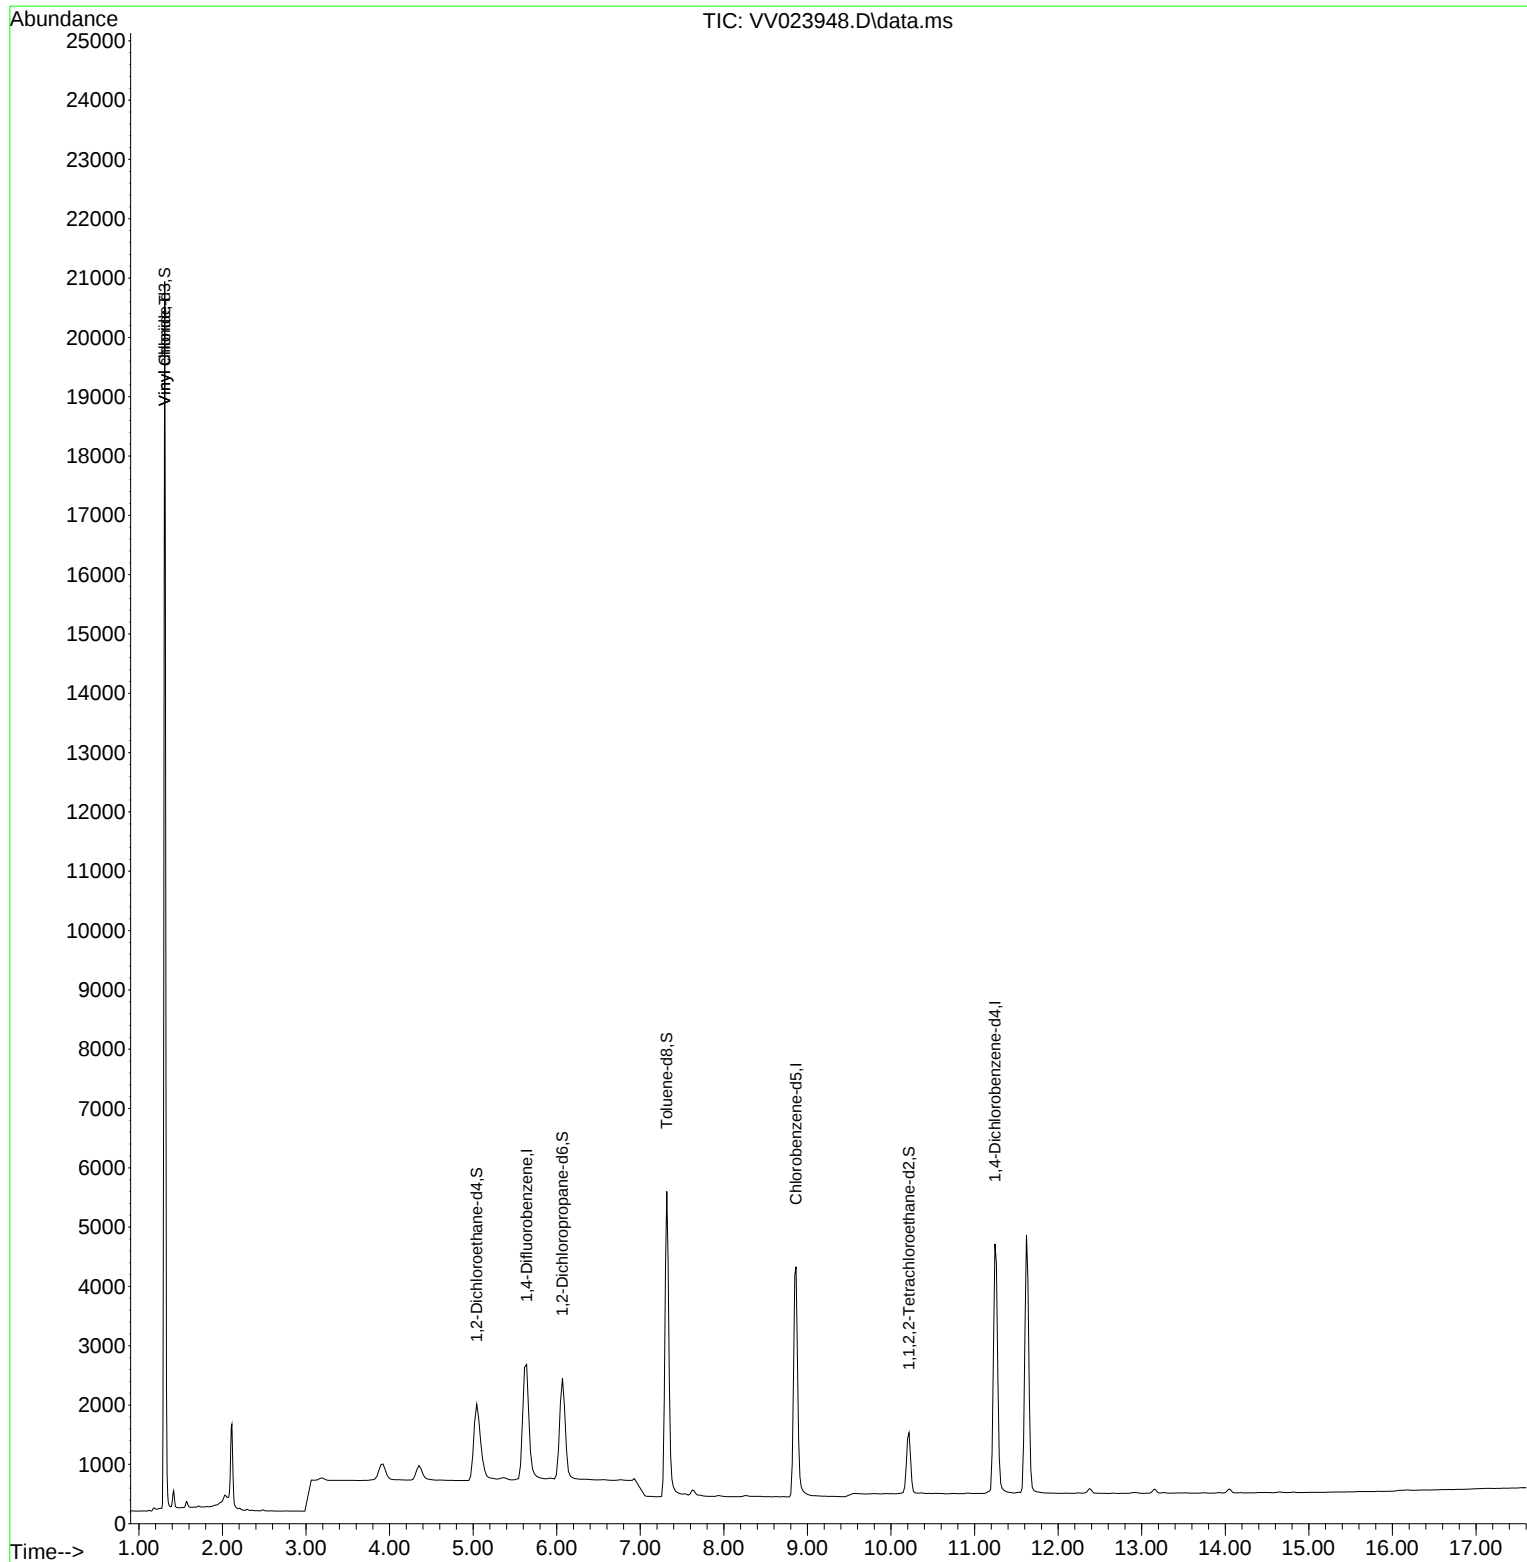

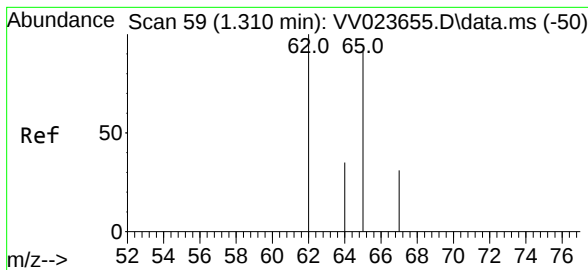

#3
 Vinyl chloride
 Concen: 2.104 ug/L
 RT: 1.310 min Scan# 59
 Delta R.T. -0.000 min
 Lab File: VV023948.D
 Acq: 13 Dec 2021 14:45

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 62 Resp: 18010
 Ion Ratio Lower Upper
 62 100
 64 33.5 25.5 47.3

