

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121321\
 Data File : VV023954.D
 Acq On : 13 Dec 2021 17:19
 Operator : SY/MD
 Sample : M4971-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 14 01:08:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 23 02:04:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7538	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	7386	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	4107	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	4506	0.589	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	118.000%
4) 1,2-Dichloroethane-d4	5.042	65	2848	0.548	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
7) 1,2-Dichloropropane-d6	6.068	67	3137	0.489	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	98.000%
8) Toluene-d8	7.317	98	9690	0.584	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	116.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2103	0.540	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.238	75	15	0.024	ug/L	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121321\
Data File : VV023954.D
Acq On : 13 Dec 2021 17:19
Operator : SY/MD
Sample : M4971-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 14 01:08:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 23 02:04:29 2021
Response via : Initial Calibration

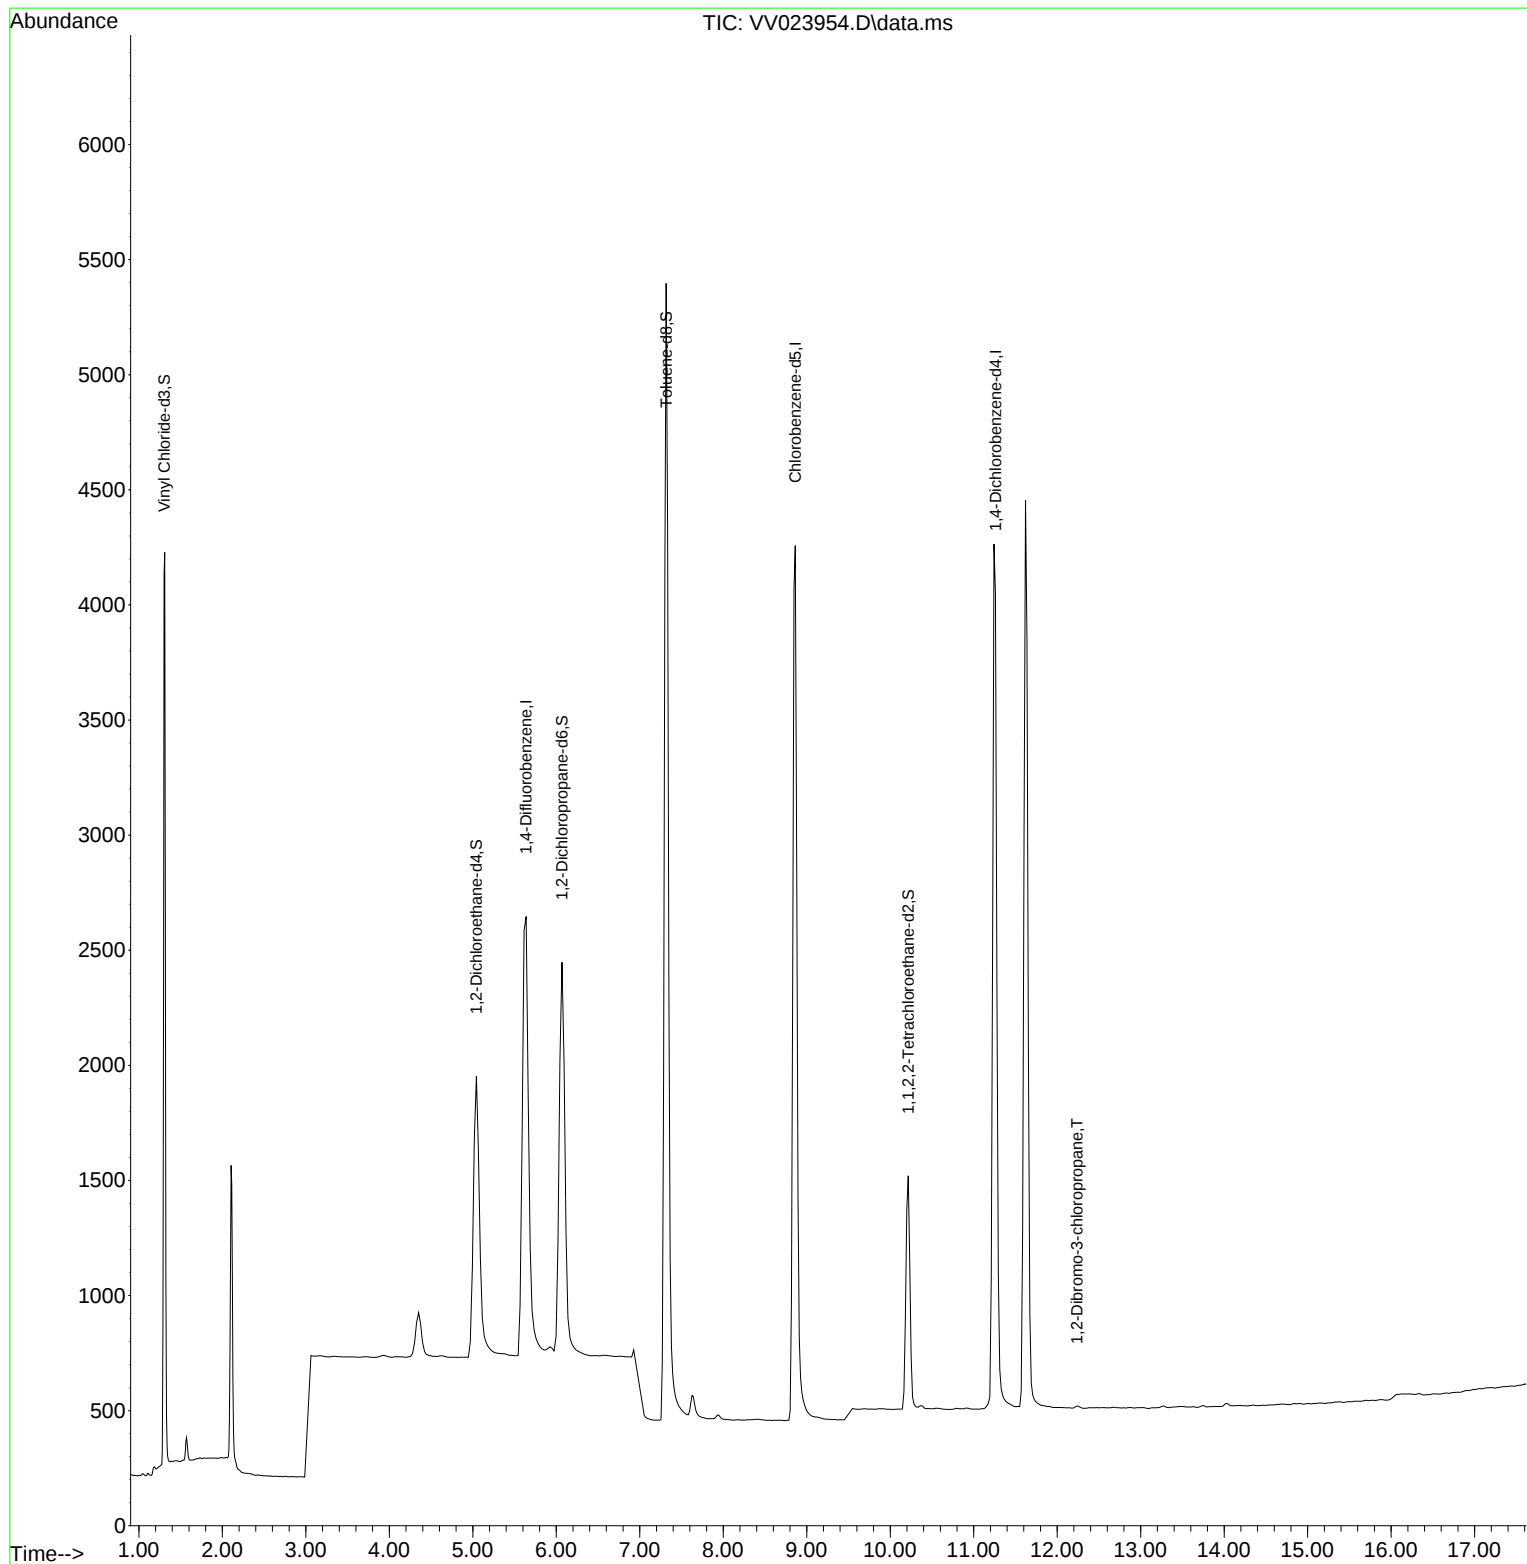

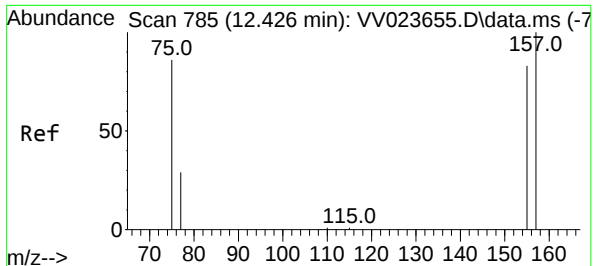

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.024 ug/L
 RT: 12.238 min Scan# 71
 Delta R.T. -0.189 min
 Lab File: VV023954.D
 Acq: 13 Dec 2021 17:19

Instrument :
 MSVOA_V
 ClientSampleId :

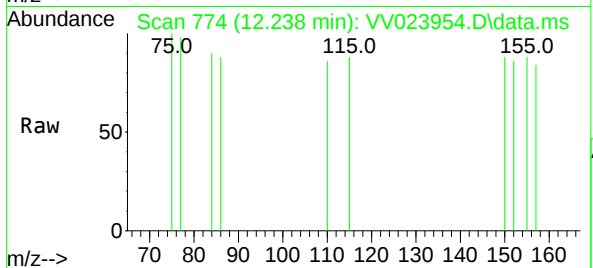

Tgt Ion: 75 Resp: 15
 Ion Ratio Lower Upper
 75 100
 157 84.5 85.7 128.5#
 155 87.9 74.3 111.5

